
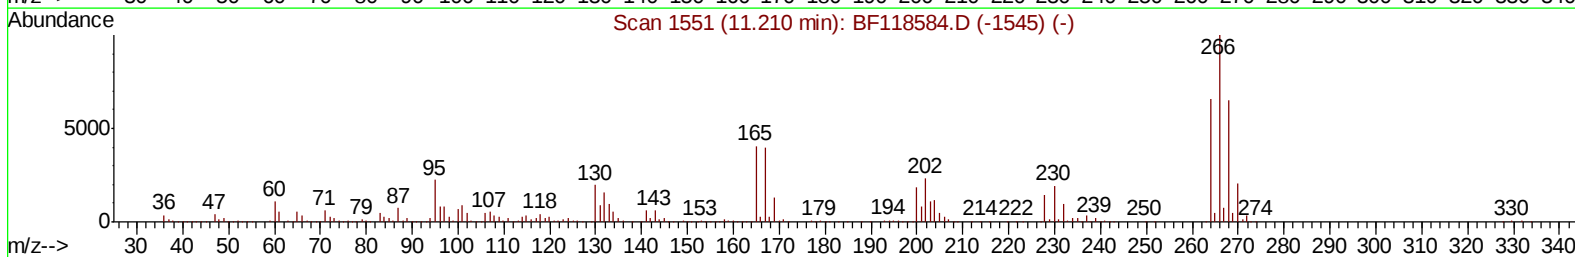
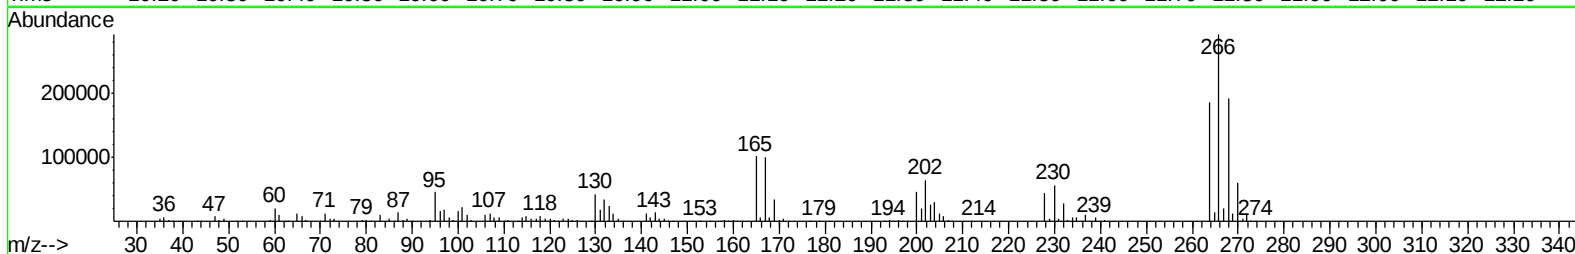


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF013020\
Data File : BF118748.D
Acq On : 30 Jan 2020 13:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 03:18:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 27 14:24:10 2020
Response via : Initial Calibration

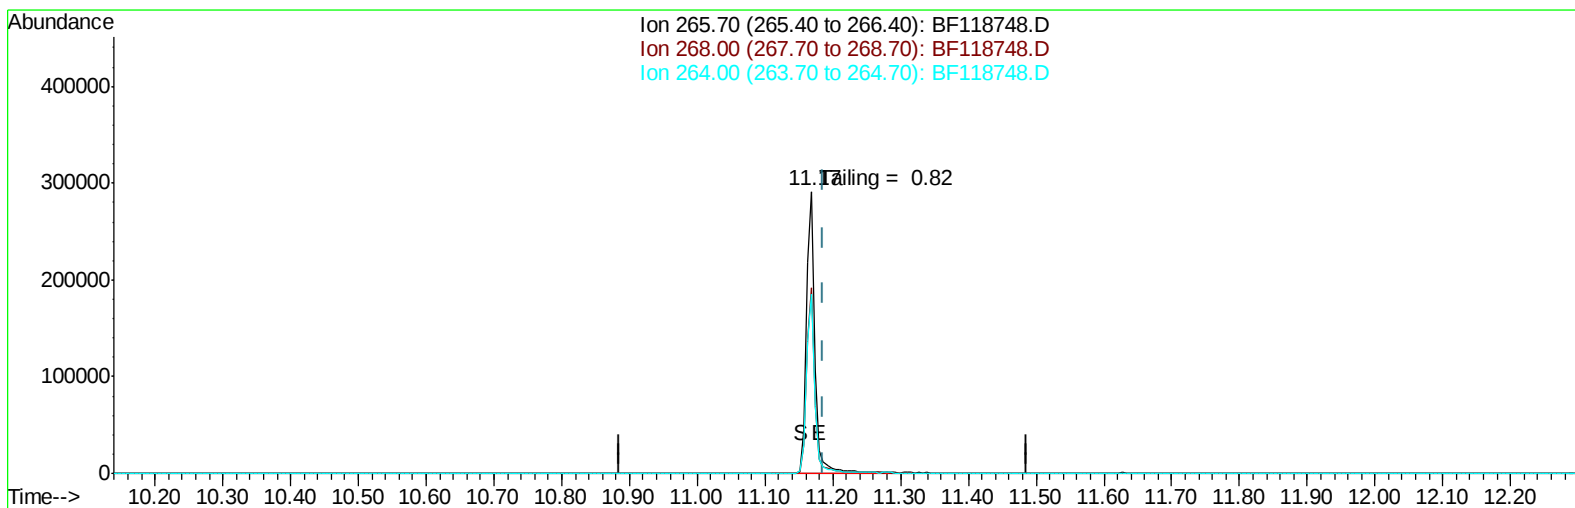

TIC: BF118748.D

(70) Pentachlorophenol (C)




11.169min (-0.018) 30268.78ng

response 262123

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	65.77
264.00	63.60	63.54
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF013020\
 Data File : BF118748.D
 Acq On : 30 Jan 2020 13:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 03:18:13 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 27 14:24:10 2020
 Response via : Initial Calibration

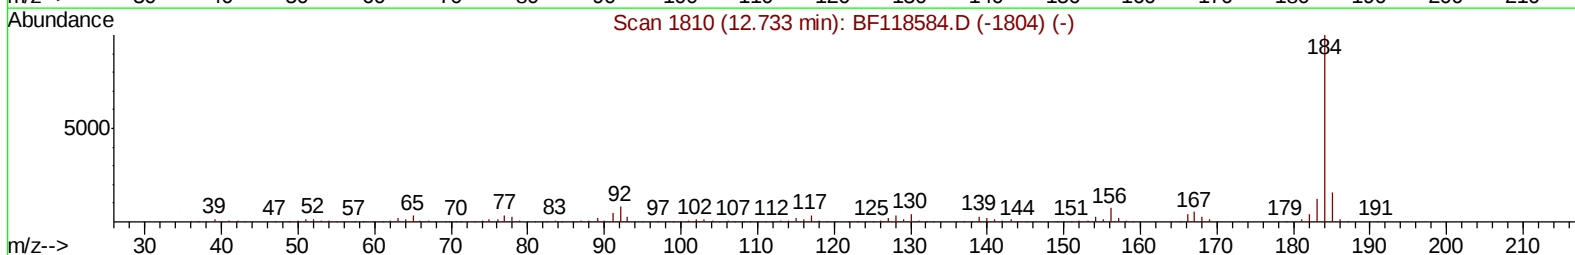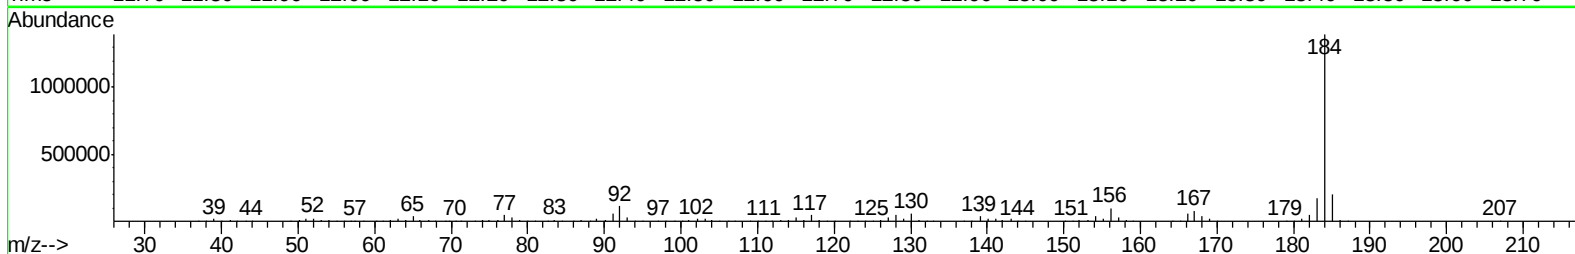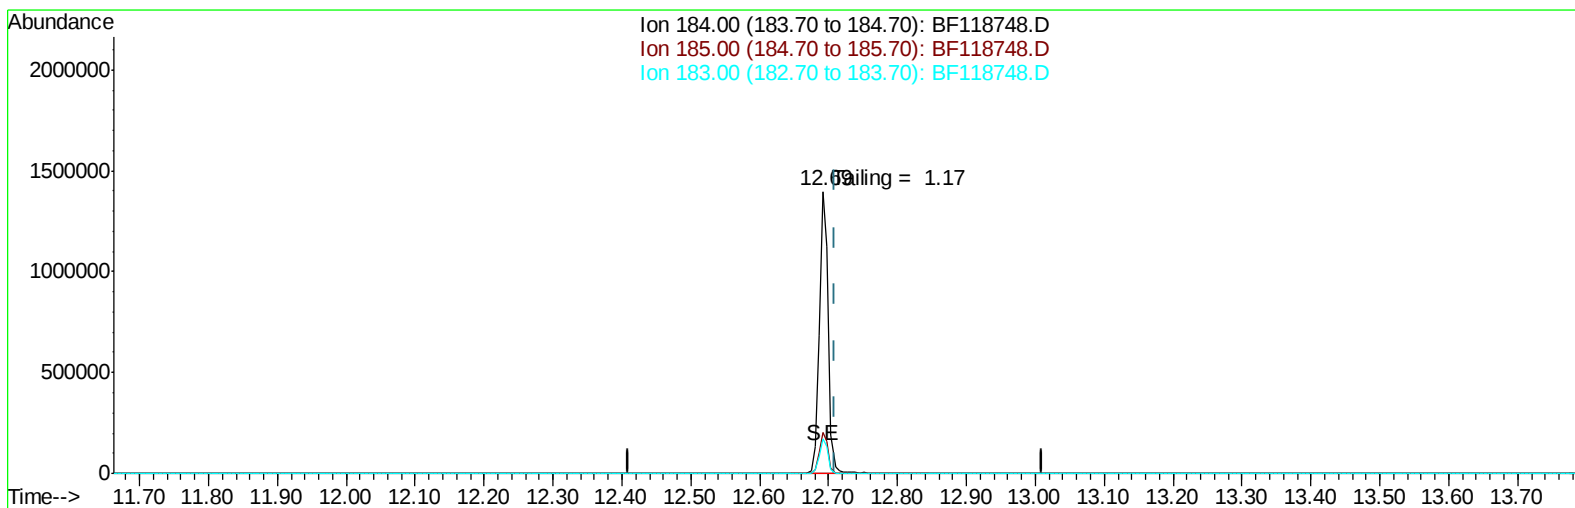

TIC: BF118748.D

(77) Benzidine

12.692min (-0.018) 0.00ng

response 1279264

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.68
183.00	12.10	12.29
0.00	0.00	0.00