

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF013020\
 Data File : BF118770.D
 Acq On : 30 Jan 2020 23:52
 Operator : CG/JU
 Sample : L1014-11 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OR-03-012920

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.451	568	572	580	rVB	719558	693058	36.39%	4.473%
2	6.463	740	744	759	rVB	836651	684201	35.92%	4.416%
3	6.840	805	808	812	rBV	1622455	1317773	69.19%	8.505%
4	6.998	831	835	838	rBV	769241	634969	33.34%	4.098%
5	7.392	899	902	906	rBV	483153	426266	22.38%	2.751%
6	8.128	1023	1027	1030	rBV	1879664	1678362	88.12%	10.832%
7	9.198	1205	1209	1212	rBV	1226130	931636	48.91%	6.013%
8	9.286	1221	1224	1228	rBV3	33060	34154	1.79%	0.220%
9	9.592	1273	1276	1278	rBV	55117	52968	2.78%	0.342%
10	9.881	1321	1325	1328	rBV	2267708	1826782	95.91%	11.790%
11	10.539	1431	1437	1440	rBV3	27257	32498	1.71%	0.210%
12	10.663	1454	1458	1463	rBV	587102	500652	26.29%	3.231%
13	10.804	1476	1482	1488	rVB2	51095	80305	4.22%	0.518%
14	11.239	1553	1556	1558	rBV2	35652	31431	1.65%	0.203%
15	11.269	1558	1561	1564	rVB2	44281	37498	1.97%	0.242%
16	11.363	1573	1577	1580	rBV	2051053	1751538	91.96%	11.305%
17	11.892	1664	1667	1671	rVB2	81067	80456	4.22%	0.519%
18	12.292	1733	1735	1741	rBV4	31760	49726	2.61%	0.321%
19	12.416	1754	1756	1759	rBV	38464	41270	2.17%	0.266%
20	12.574	1780	1783	1786	rBV	84000	81386	4.27%	0.525%
21	12.804	1820	1822	1825	rBV2	62270	63346	3.33%	0.409%
22	12.945	1843	1846	1850	rBV	1077743	957495	50.27%	6.180%
23	14.004	2022	2026	2029	rBV	2043010	1904706	100.00%	12.293%
24	15.468	2271	2275	2279	rBV	1312161	1601588	84.09%	10.337%


Sum of corrected areas: 15494064

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF013020\
Data File : BF118770.D
Acq On : 30 Jan 2020 23:52
Operator : CG/JU
Sample : L1014-11 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-03-012920

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

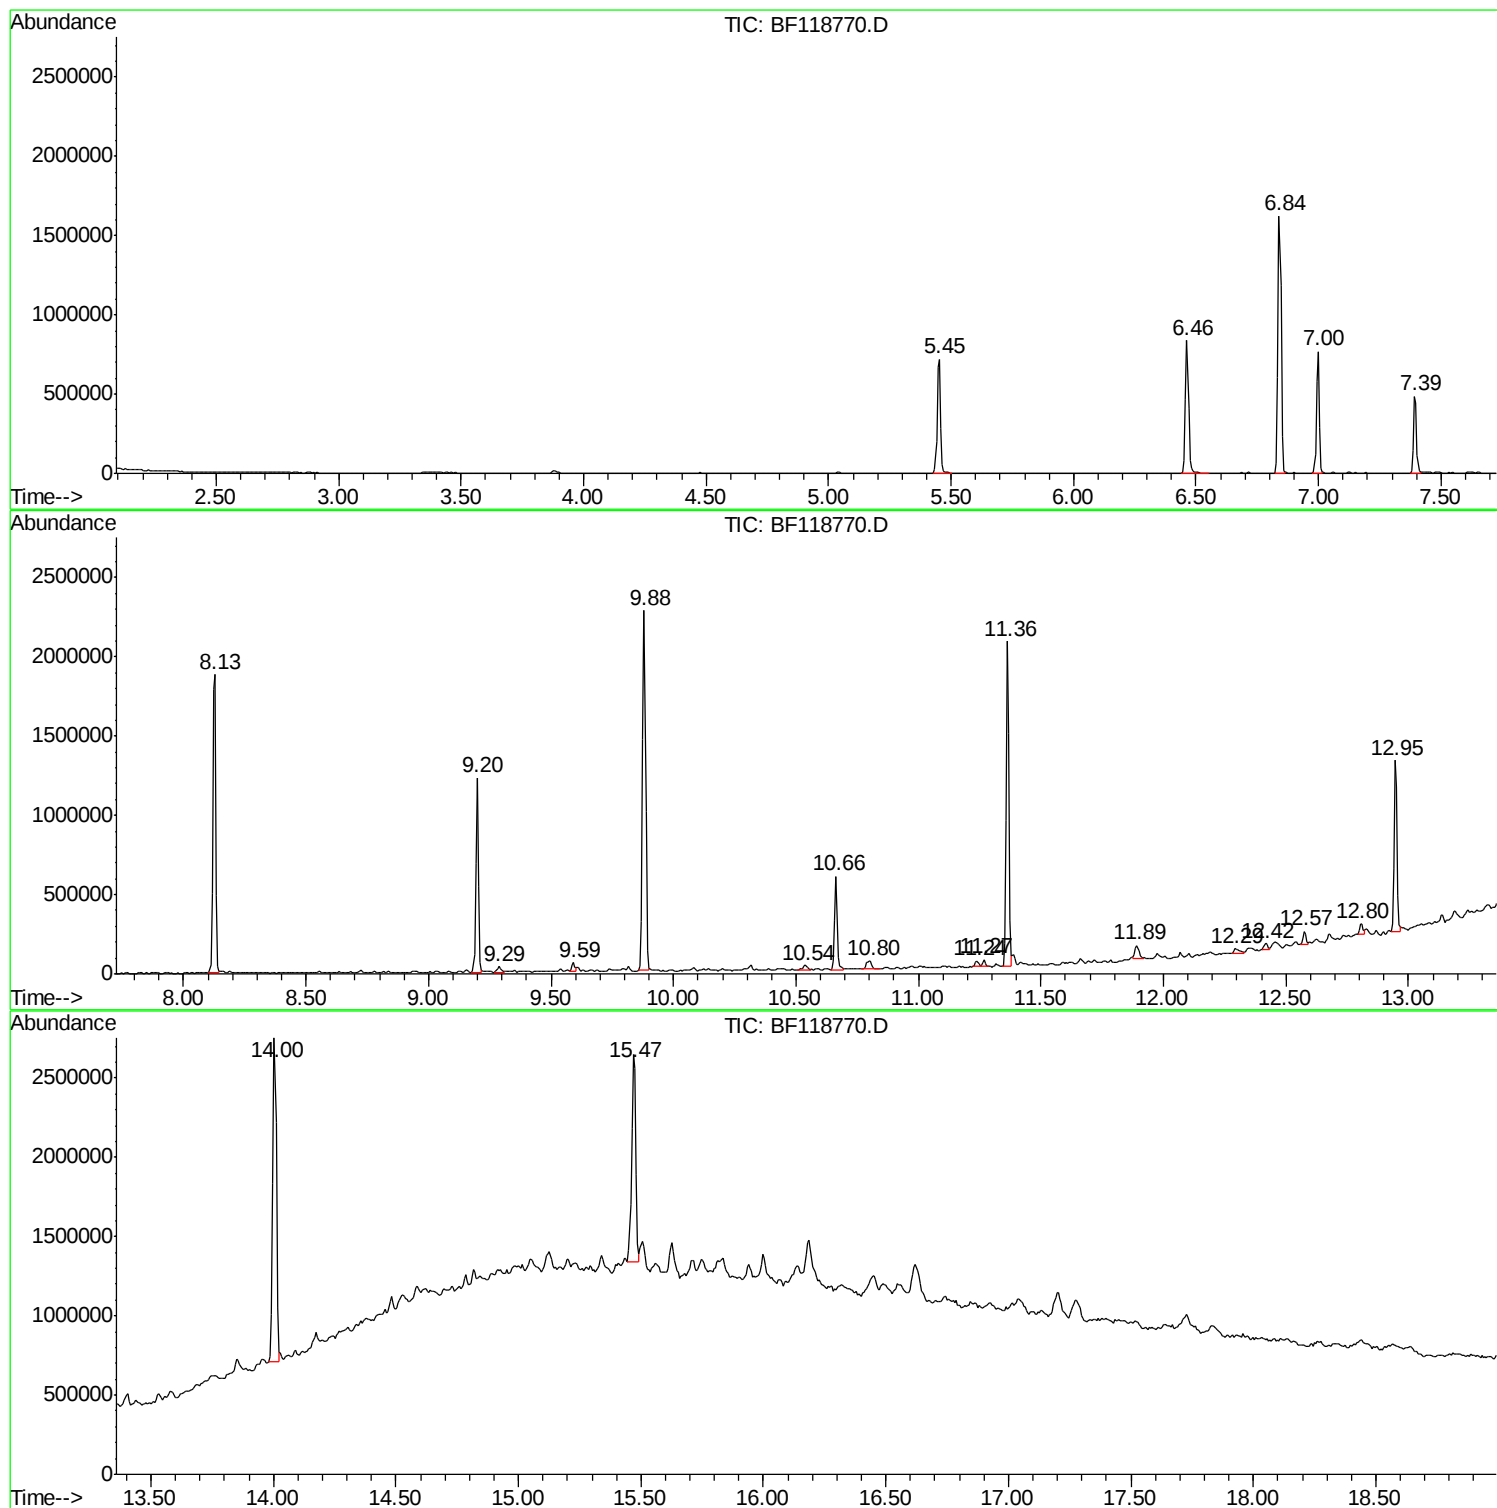

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF013020\
Data_File : BF118770.D
Acq_On : 30-Jan-2020 23:522
Operator : CG/JUU
Sample : L1014-11_5XX
Misc :
ALS_Vial : 23 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
OR-03-012920

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012020.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
