


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013020\
 Data File : BF118748.D
 Acq On : 30 Jan 2020 13:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 27 14:24:10 2020

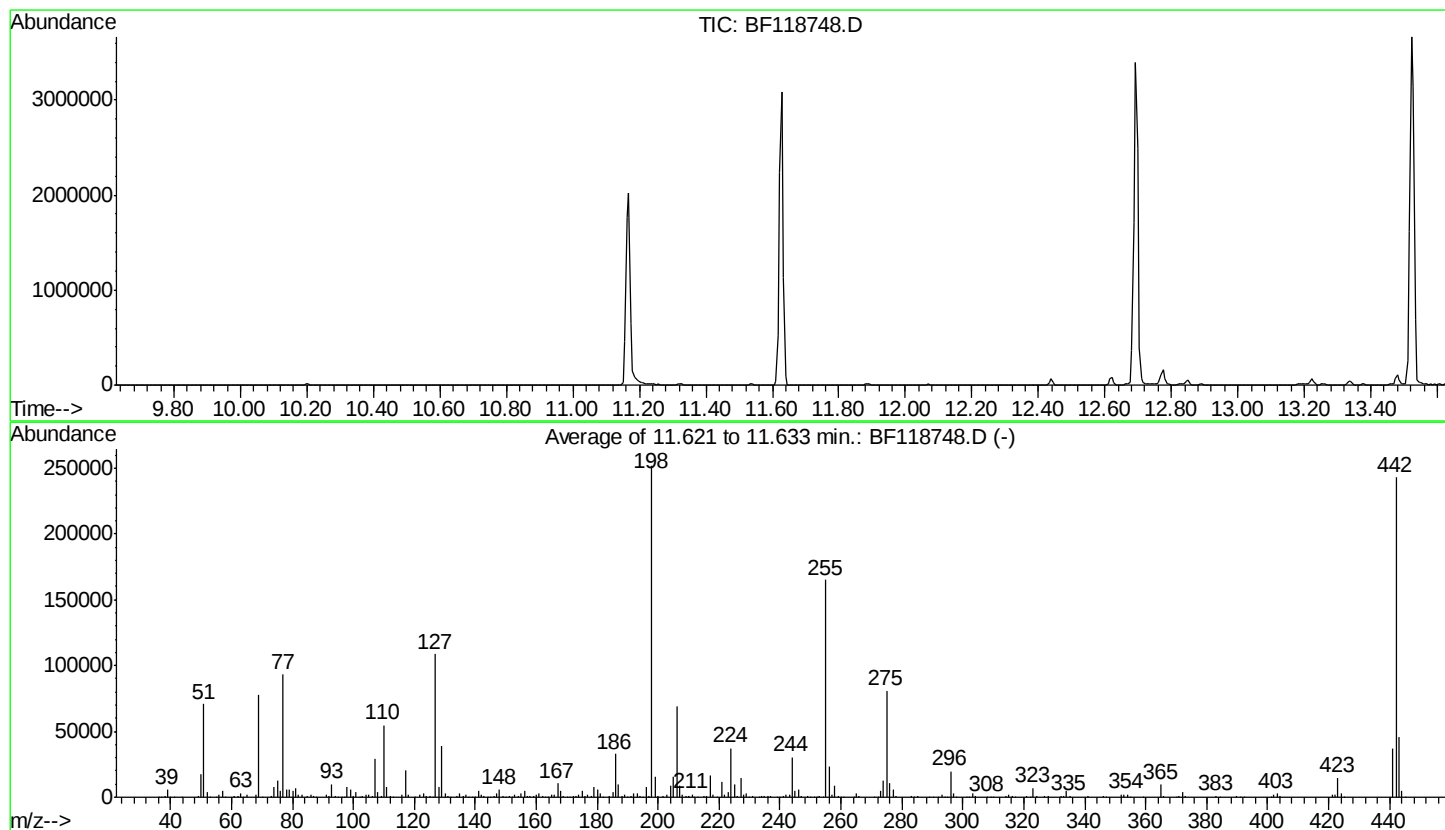

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.0	70568	PASS
68	69	0.00	2	2.0	1537	PASS
69	198	0.00	100	31.1	78317	PASS
70	69	0.00	2	0.5	400	PASS
127	198	10	80	43.2	108722	PASS
197	198	0.00	2	0.4	889	PASS
198	198	100	100	100.0	251901	PASS
199	198	5	9	6.4	16040	PASS
275	198	10	60	32.1	80736	PASS
365	198	1	100	3.7	9443	PASS
441	198	0.01	100	14.8	37266	PASS
442	198	50	100	96.5	243093	PASS
443	442	15	24	18.9	46002	PASS