
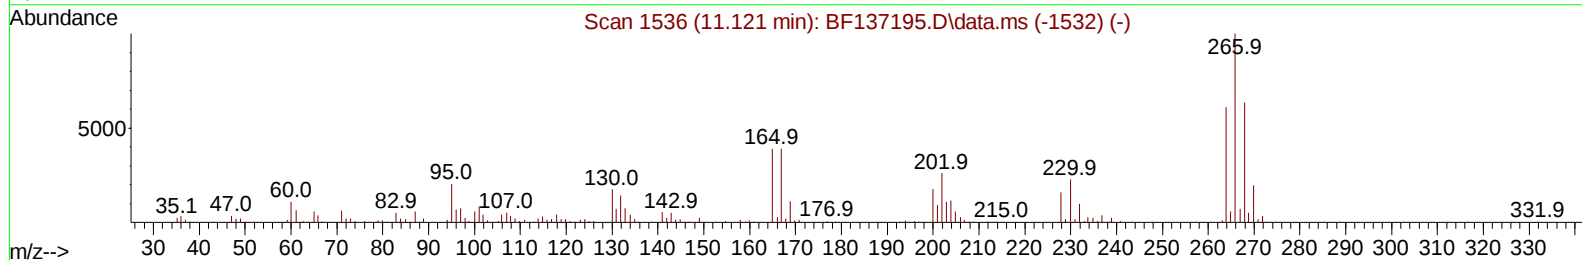
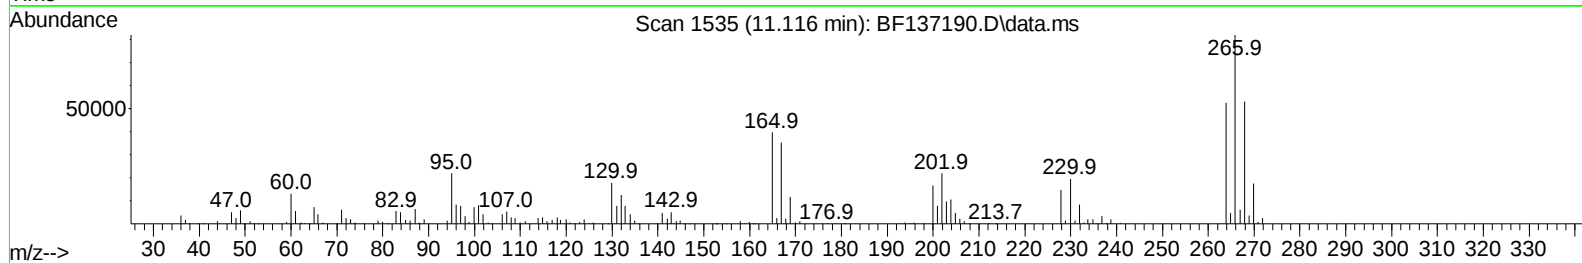


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013024\
Data File : BF137190.D
Acq On : 30 Jan 2024 10:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 05:03:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 04:56:22 2024
Response via : Initial Calibration

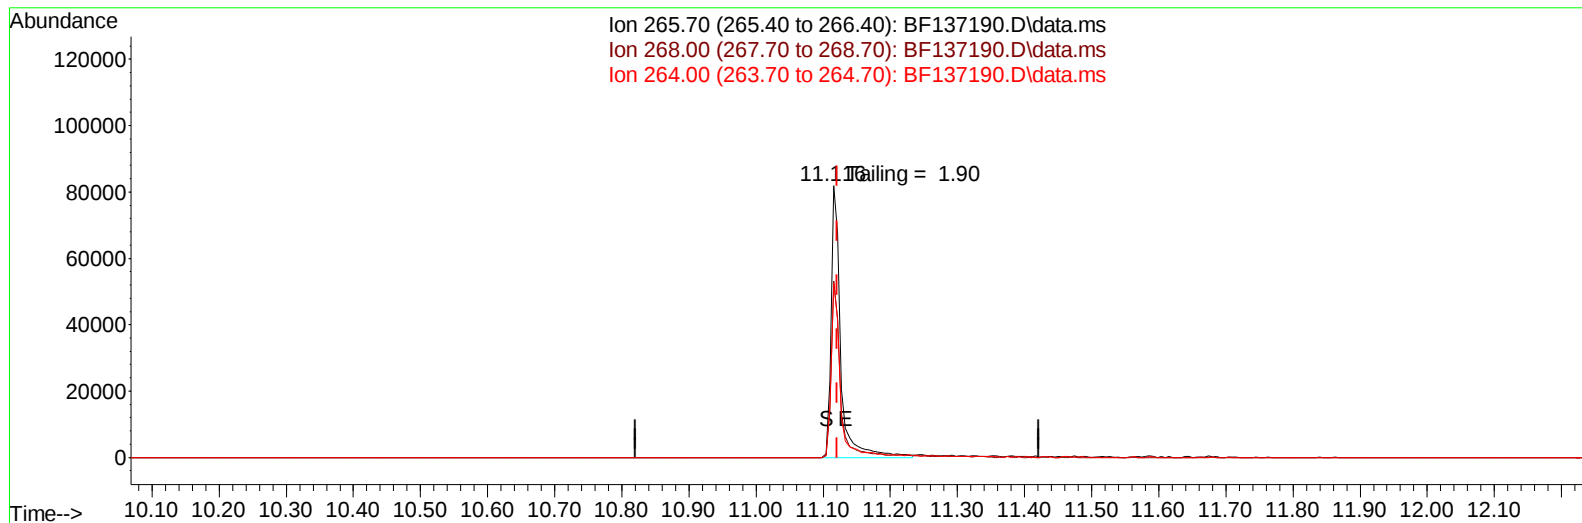

TIC: BF137190.D\data.ms

(70) Pentachlorophenol (C)




11.116min (-0.005) 33756.95 ng

response 83422

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.88
264.00	61.00	64.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013024\
Data File : BF137190.D
Acq On : 30 Jan 2024 10:53
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 05:03:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 04:56:22 2024
Response via : Initial Calibration

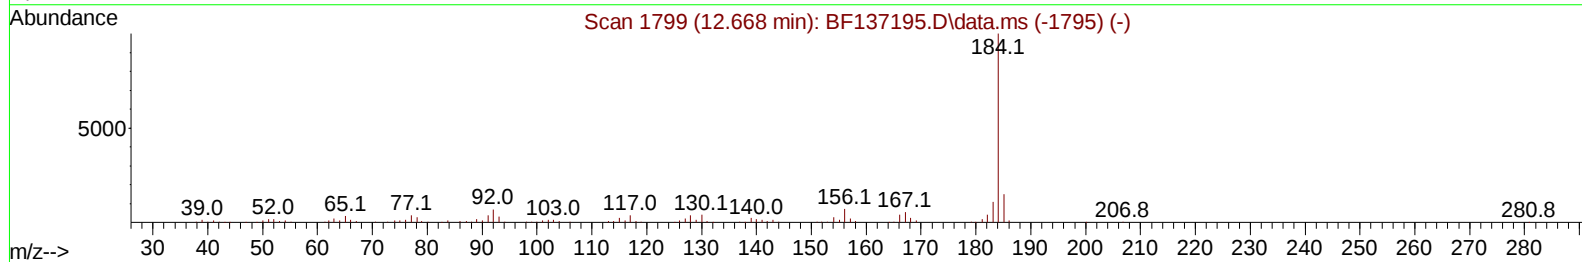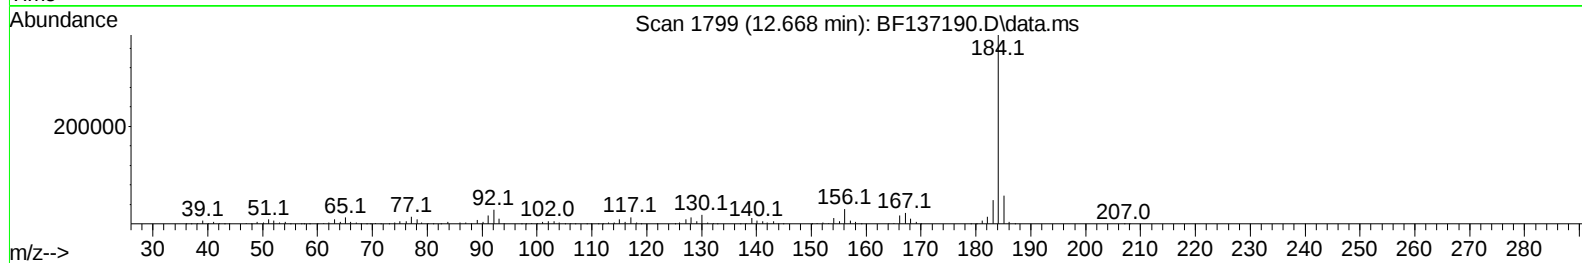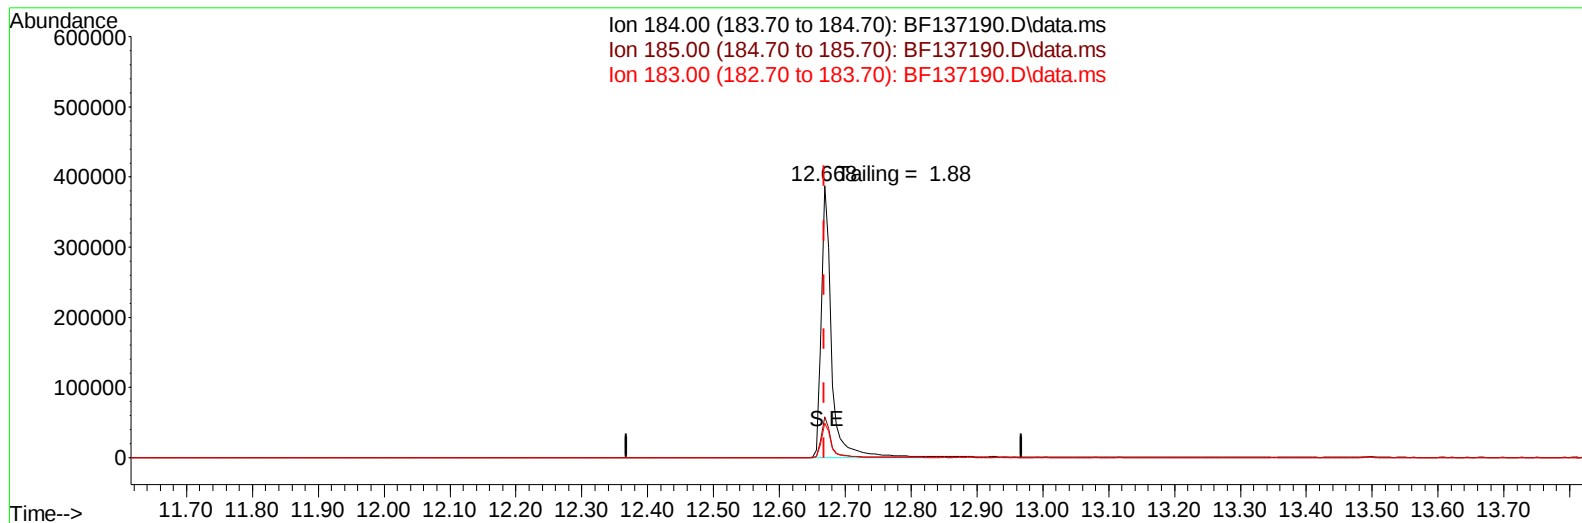

TIC: BF137190.D\data.ms

(77) Benzidine**12.668min (+ 0.000) 0.00 ng****response 404346**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.90
183.00	11.00	12.60
0.00	0.00	0.00