


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013024\
Data File : BF137190.D
Acq On : 30 Jan 2024 10:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 31 04:56:22 2024

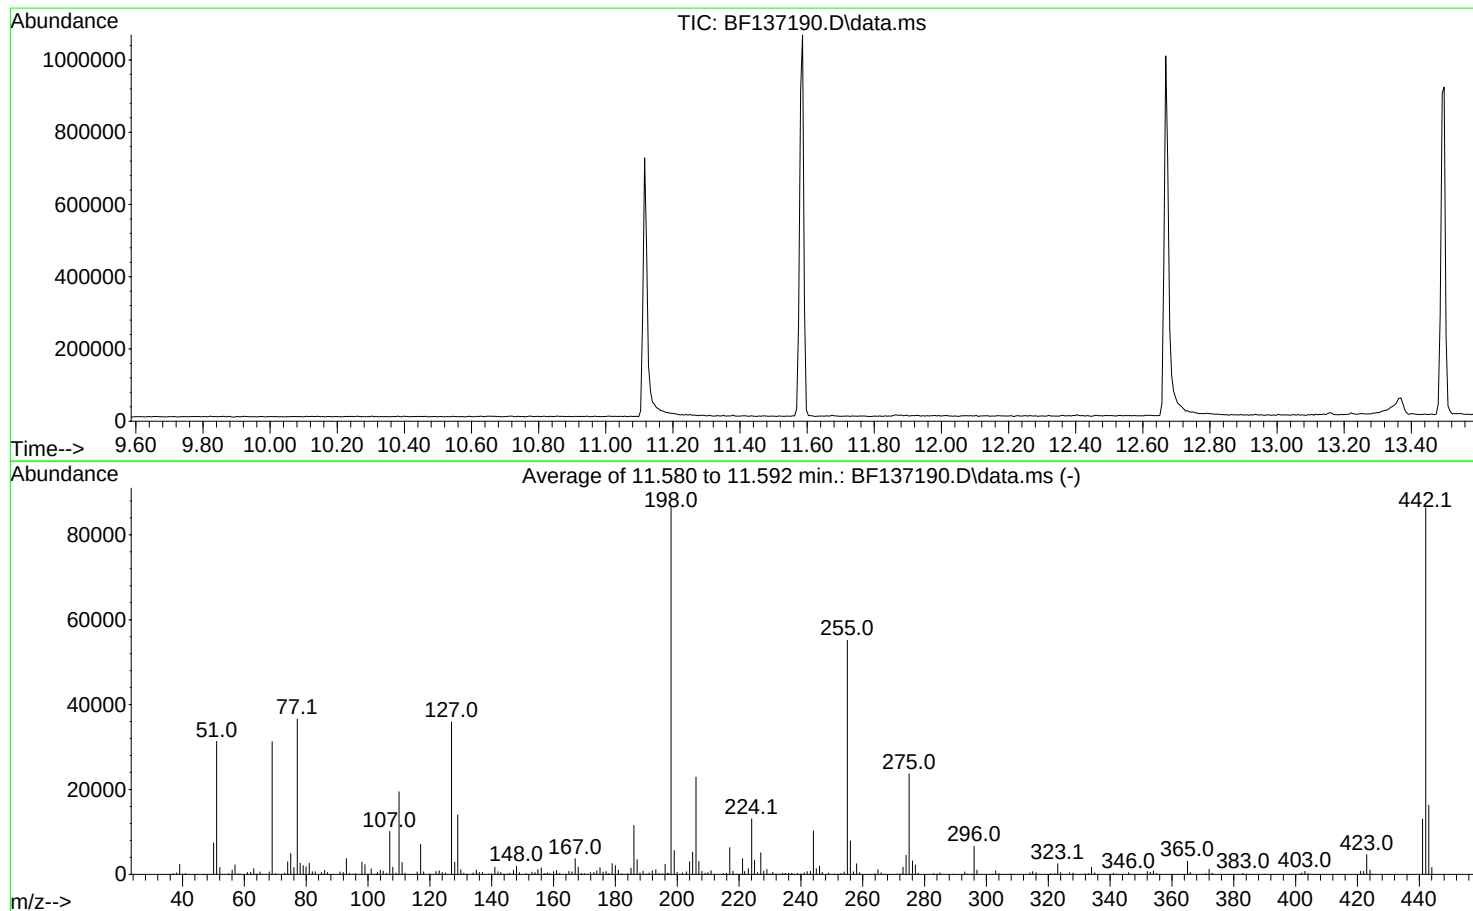




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	31322	PASS
68	69	0.00	2	1.8	569	PASS
69	198	0.00	100	36.1	31295	PASS
70	69	0.00	2	0.4	137	PASS
127	198	10	80	41.4	35880	PASS
197	198	0.00	2	0.3	251	PASS
198	198	100	100	100.0	86675	PASS
199	198	5	9	6.5	5638	PASS
275	198	10	60	27.3	23661	PASS
365	198	1	100	3.5	3059	PASS
441	198	0.01	100	15.1	13055	PASS
442	442	50	100	100.0	86411	PASS
443	442	15	24	18.8	16280	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013024\
Data File : BF137190.D
Acq On : 30 Jan 2024 10:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 31 05:03:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 04:56:22 2024
Response via : Initial Calibration

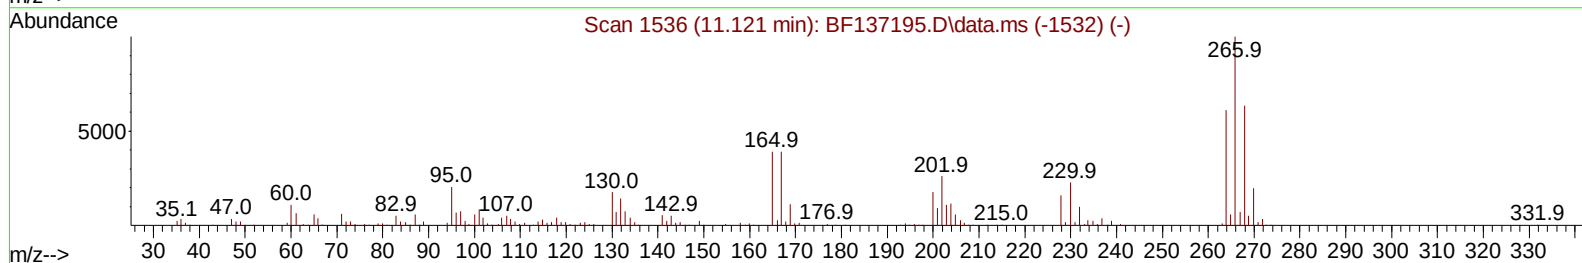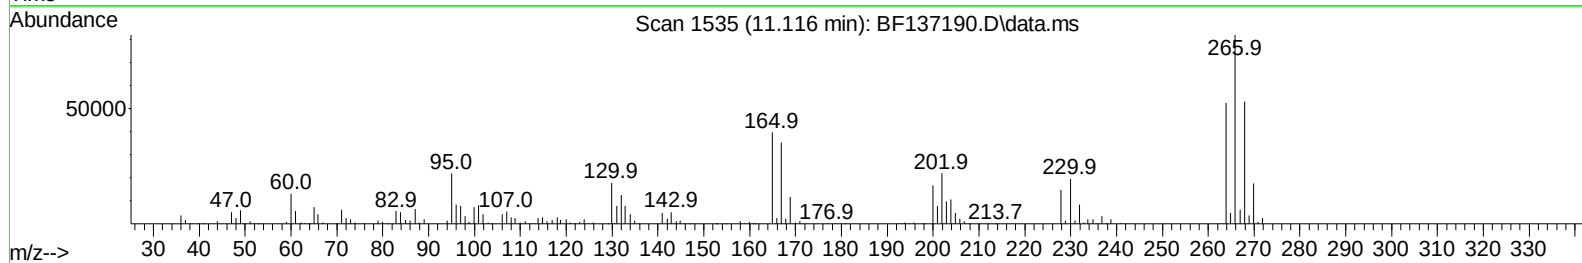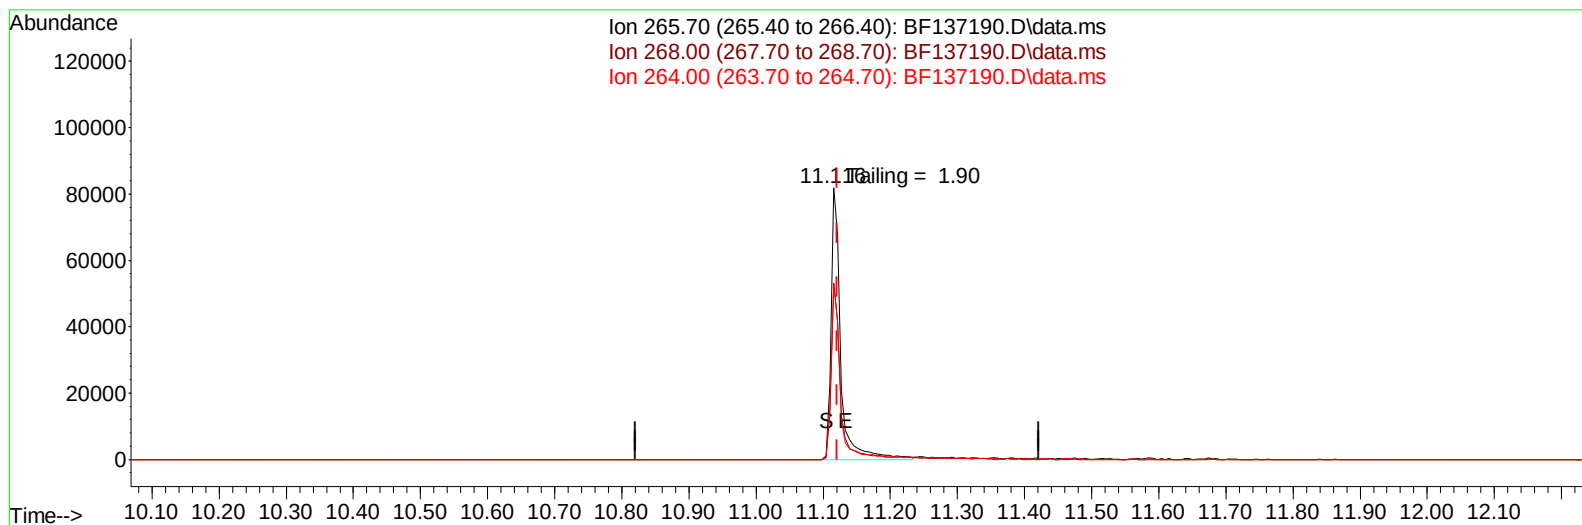

TIC: BF137190.D\data.ms

(70) Pentachlorophenol (C)

11.116min (-0.005) 33756.95 ng




response 83422

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.88
264.00	61.00	64.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013024\
Data File : BF137190.D
Acq On : 30 Jan 2024 10:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 31 05:03:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 04:56:22 2024
Response via : Initial Calibration

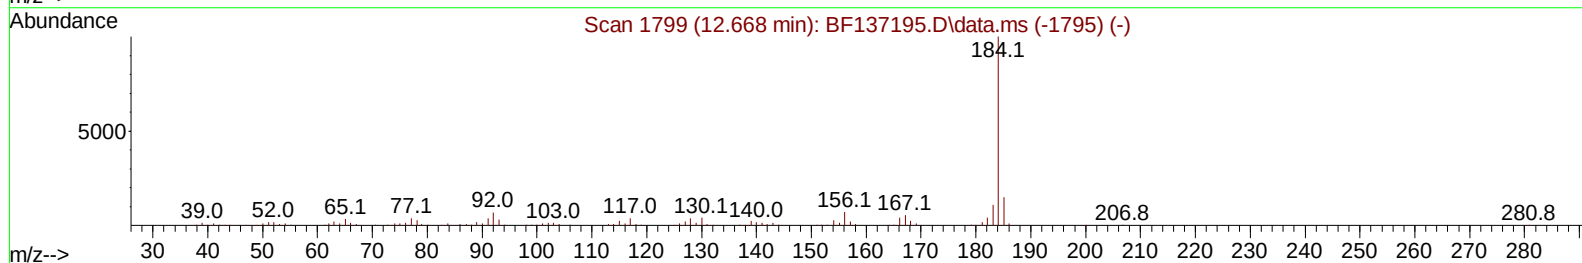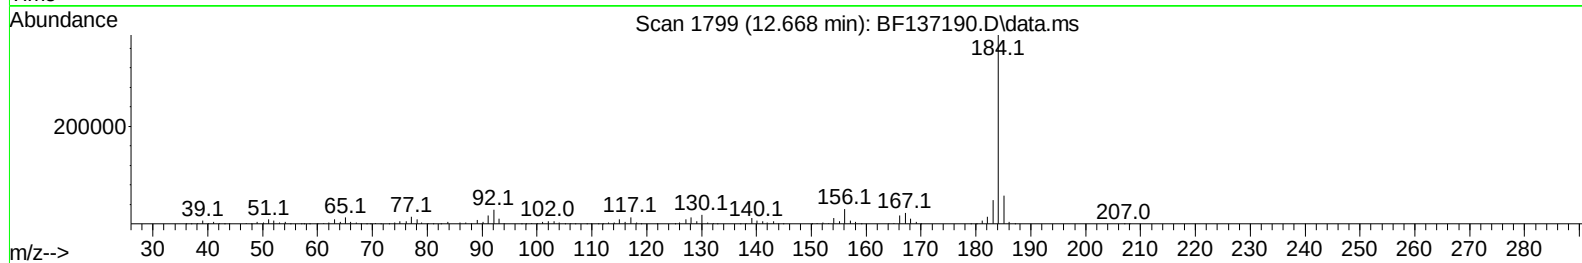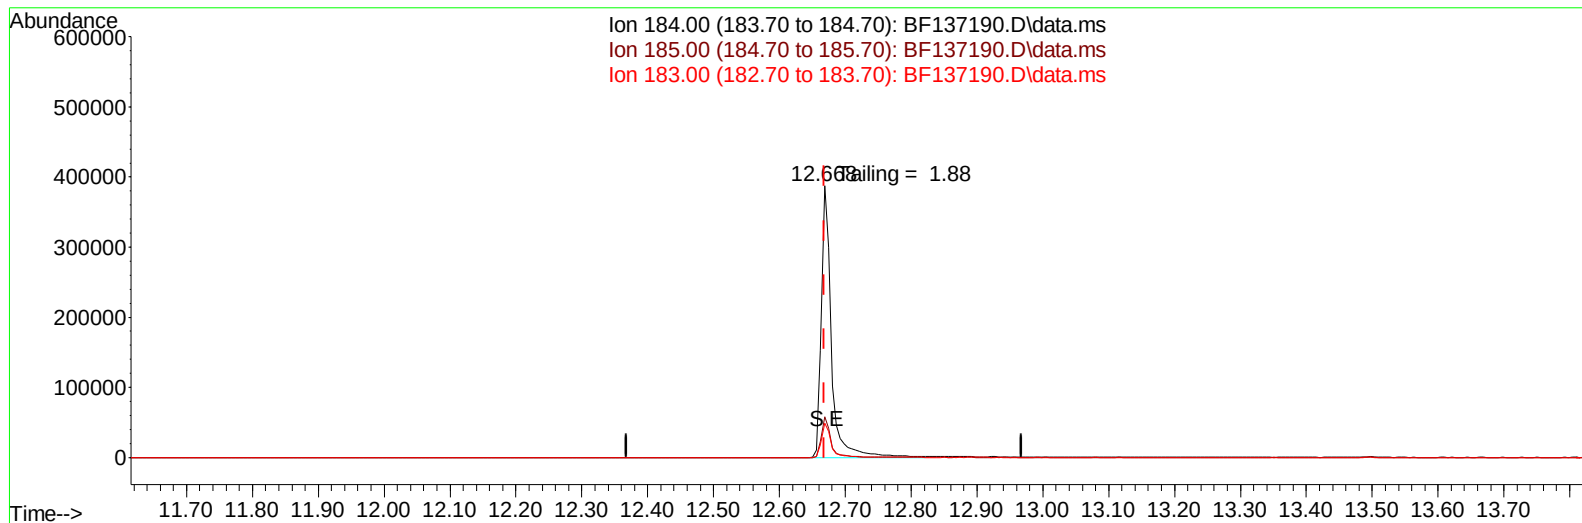

TIC: BF137190.D\data.ms

(77) Benzidine

12.668min (+ 0.000) 0.00 ng

response 404346

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.90
183.00	11.00	12.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/30/2024	BNA_F	<u>BF137190.D</u>
Compound Name	Response	Retention Time
DDT	155167	13.498
DDD	1648	13.221
DDE	0	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1648	156815	1.05

Instrument :
BNA_F
ClientSampleId :
DFTPP