
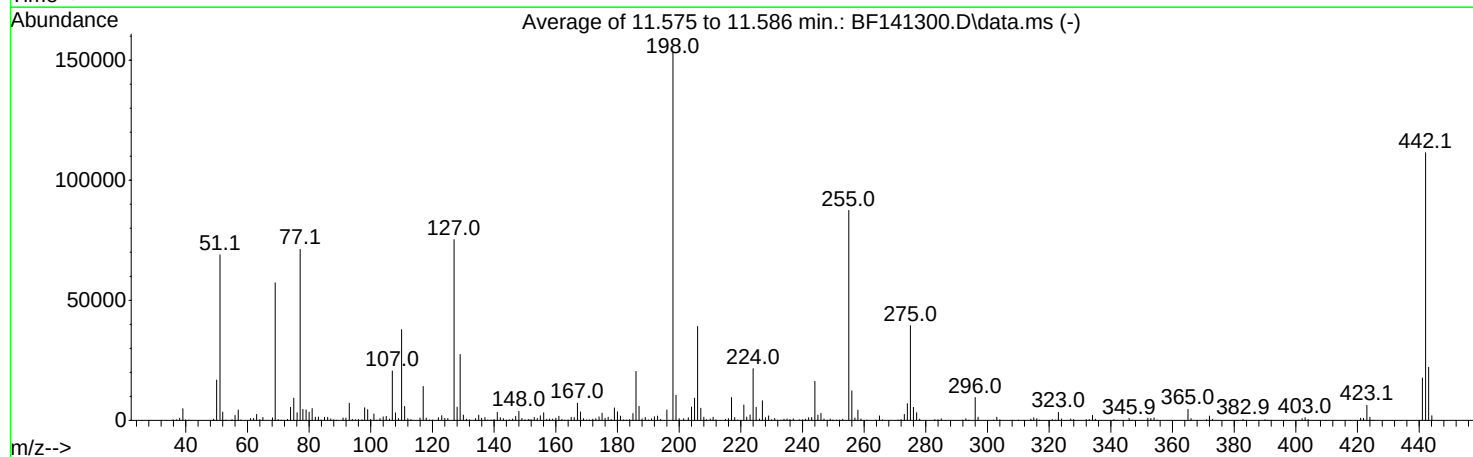


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013025\
Data File : BF141300.D
Acq On : 30 Jan 2025 08:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 29 17:41:25 2025

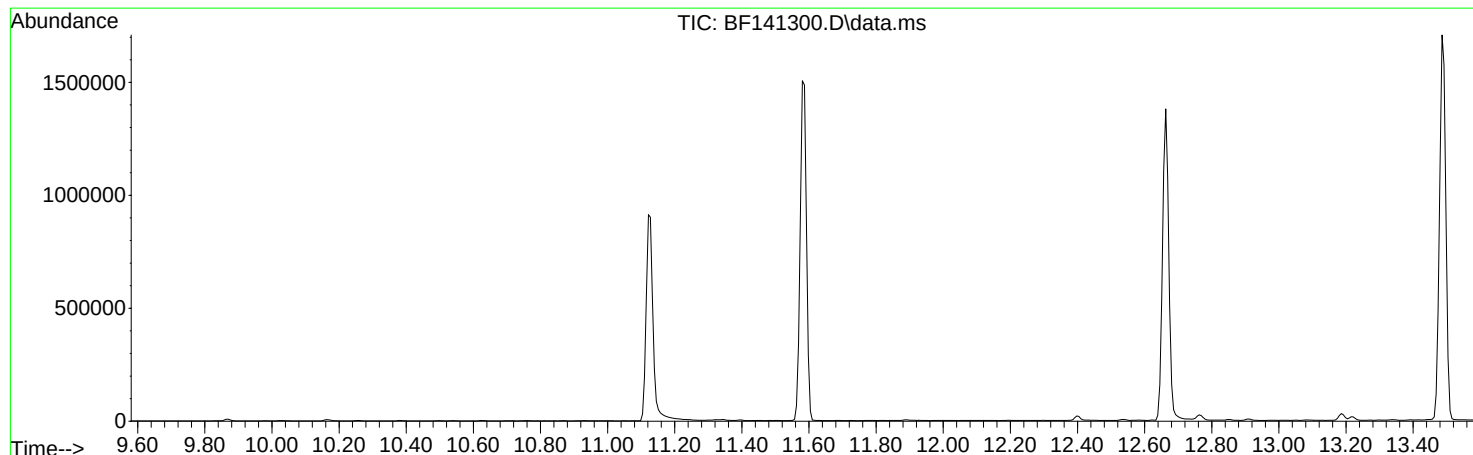

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.0	68947	PASS
68	69	0.00	2	1.9	1080	PASS
69	198	0.00	100	37.4	57275	PASS
70	69	0.00	2	0.6	350	PASS
127	198	10	80	49.1	75275	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	153189	PASS
199	198	5	9	6.8	10452	PASS
275	198	10	60	25.8	39467	PASS
365	198	1	100	3.0	4620	PASS
441	198	0.01	100	11.5	17662	PASS
442	442	50	100	100.0	111453	PASS
443	442	15	24	19.8	22114	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/30/2025	BNA_F	<u>BF141300.D</u>
Compound Name	Response	Retention Time
DDT	441101	13.486
DDD	12334	13.186
DDE	802	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13136	454237	2.89

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013025\
Data File : BF141300.D
Acq On : 30 Jan 2025 08:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 30 10:21:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

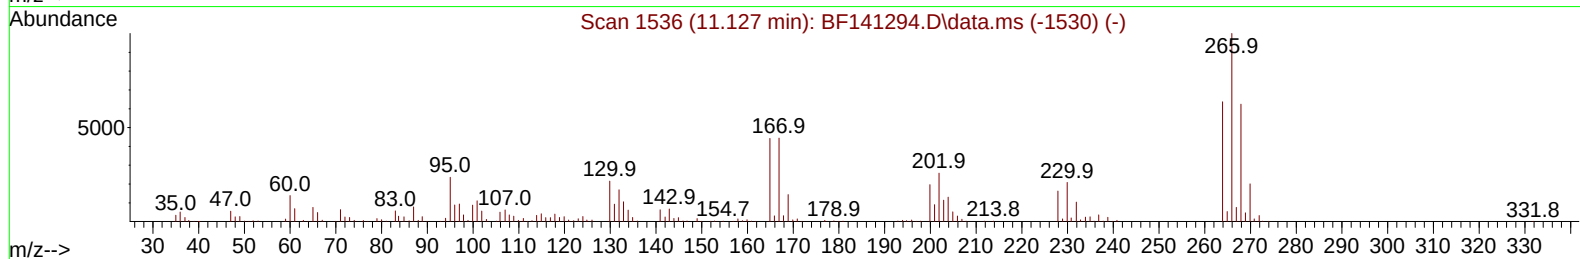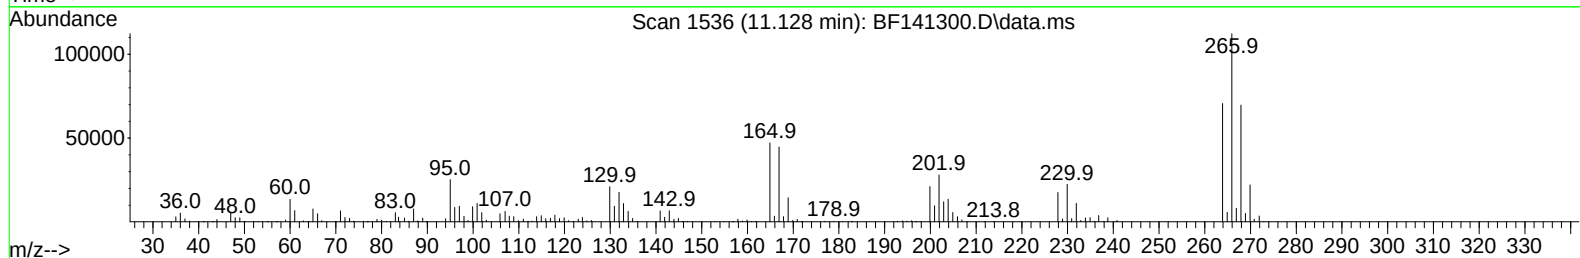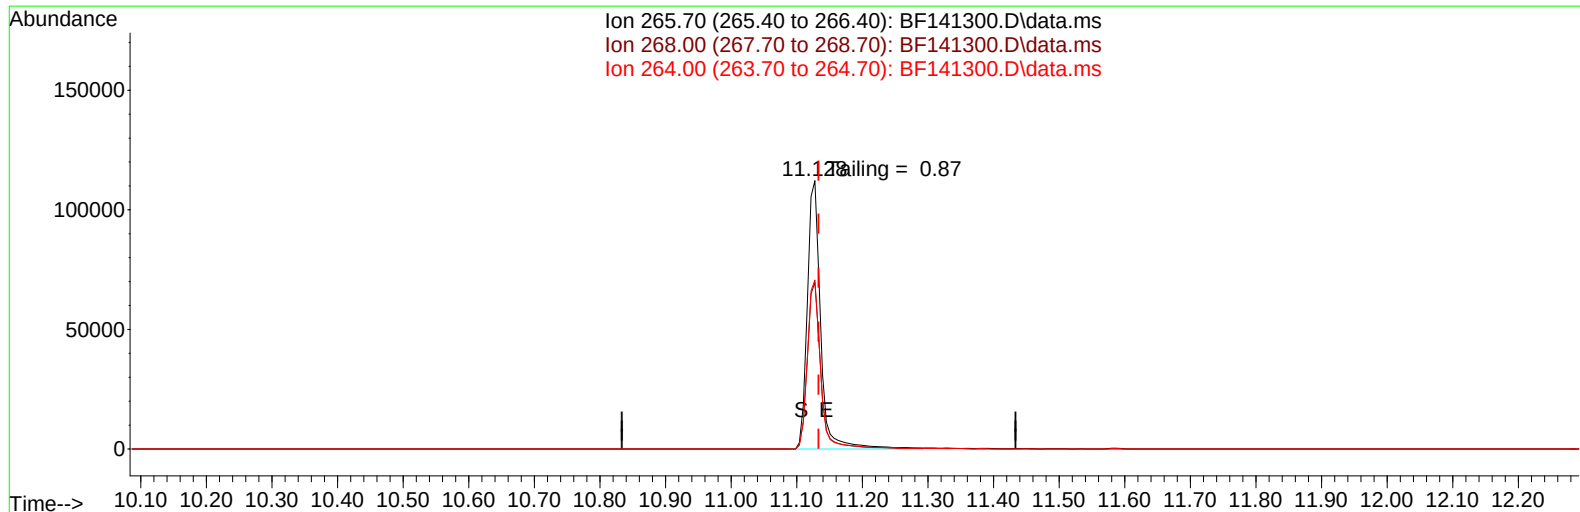

TIC: BF141300.D\data.ms

(70) Pentachlorophenol (C)

11.128min (-0.006) 13218.72 ng




response 160131

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.08
264.00	63.70	62.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013025\
Data File : BF141300.D
Acq On : 30 Jan 2025 08:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 30 10:21:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

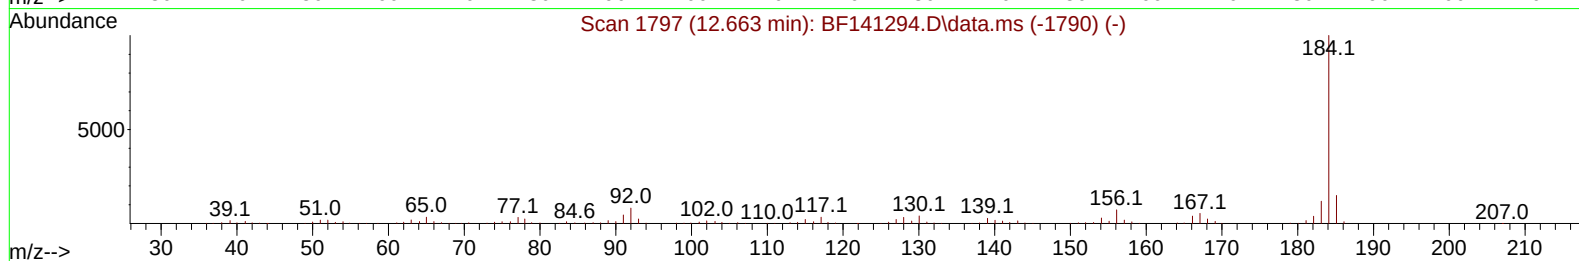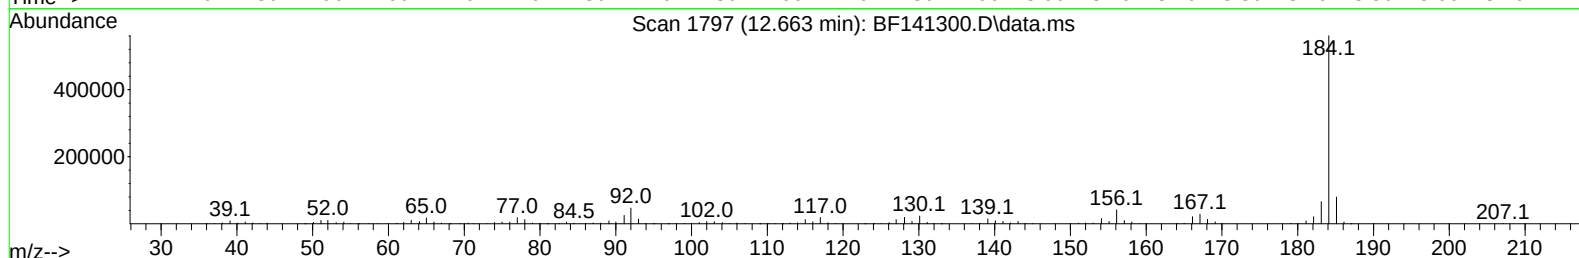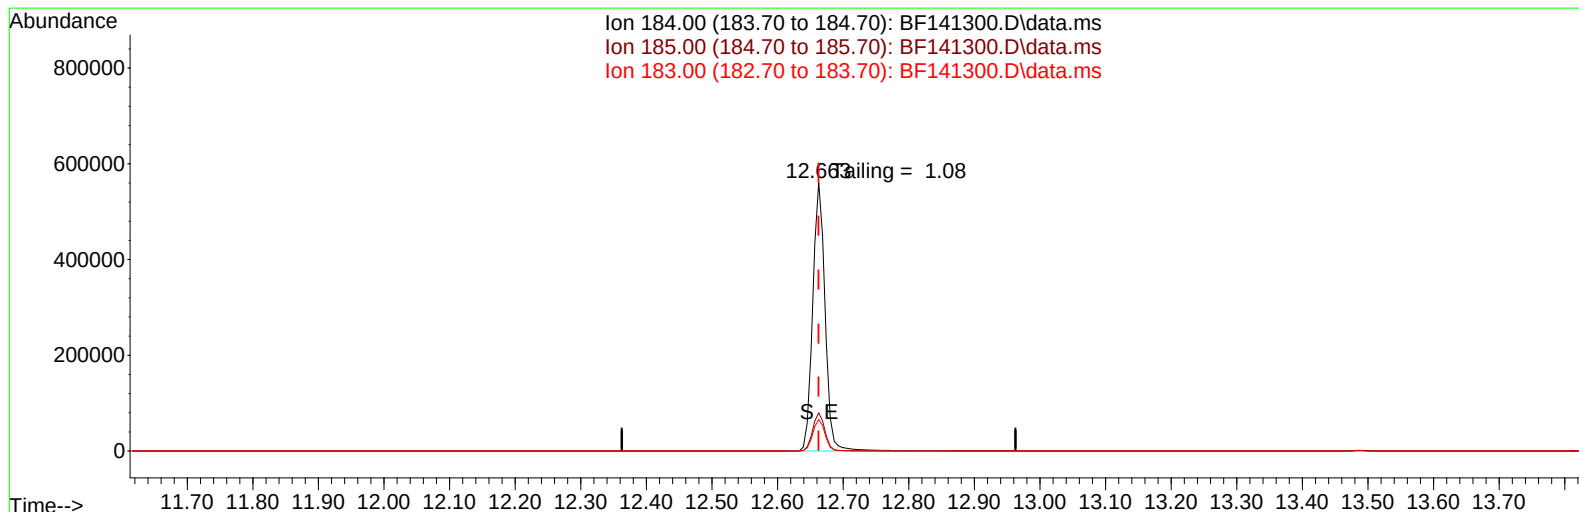

TIC: BF141300.D\data.ms

(77) Benzidine

12.663min (-0.000) 23068.63 ng

response 739544

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.27
183.00	11.90	11.79
0.00	0.00	0.00