
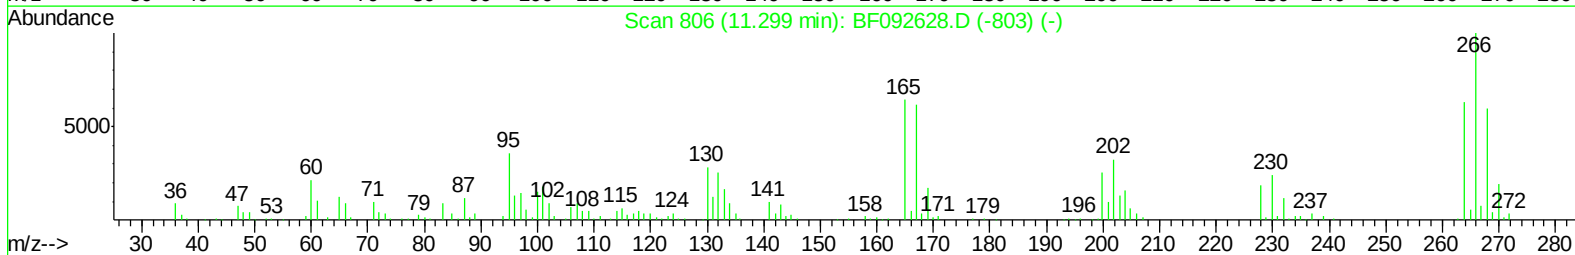
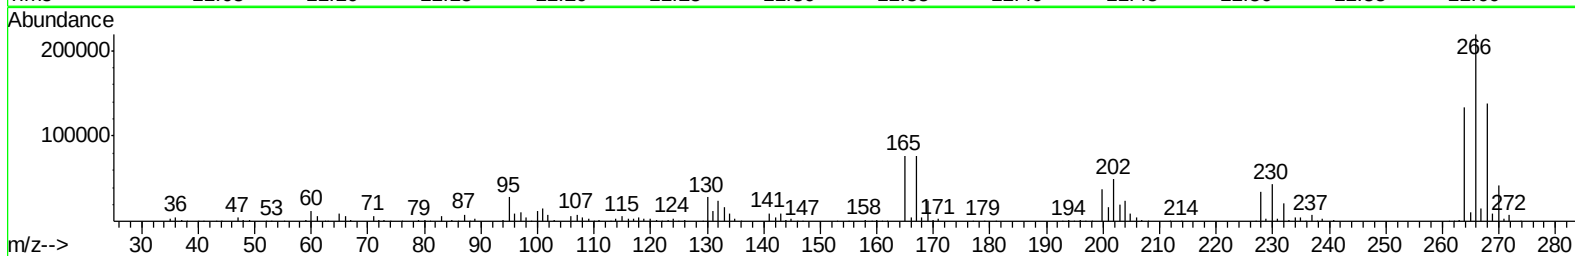


Data Path : Z:\HPCHEM1\BNA F\DATA\BF013117\
Data File : BF092678.D
Acq On : 31 Jan 2017 13:44
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 18:16:28 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 30 14:50:05 2017
Response via : Initial Calibration

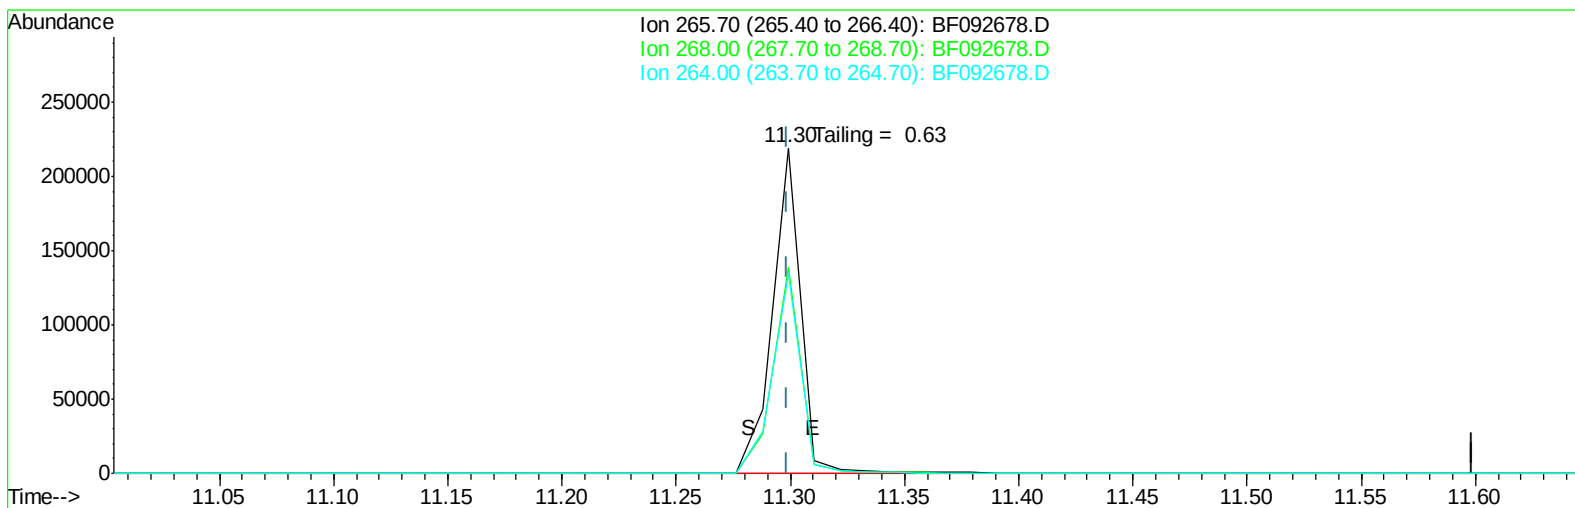

TIC: BF092678.D

(69) Pentachlorophenol (C)




11.299min (+0.000) 116991.97ng

response 191164

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	63.24
264.00	62.90	61.37
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF013117\
Data File : BF092678.D
Acq On : 31 Jan 2017 13:44
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 18:16:28 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 30 14:50:05 2017
Response via : Initial Calibration

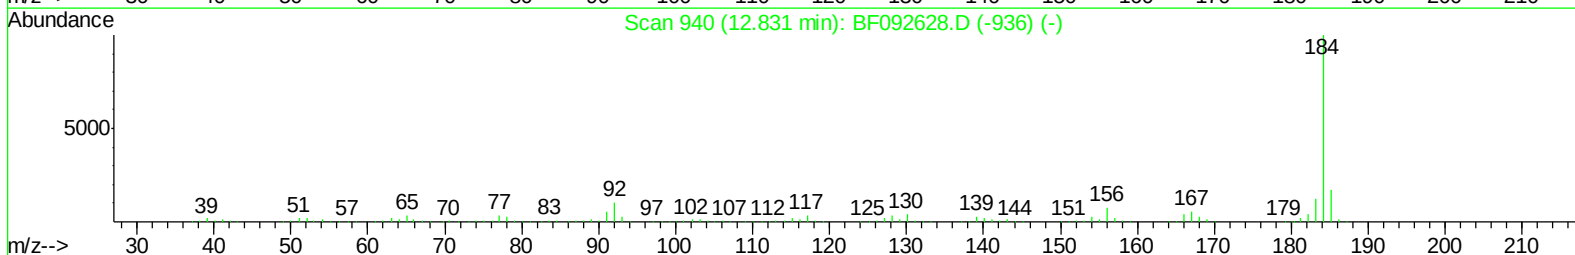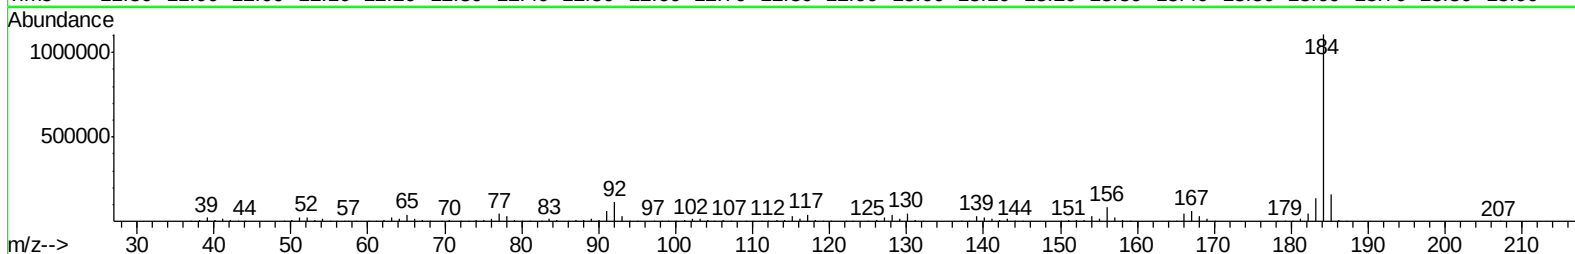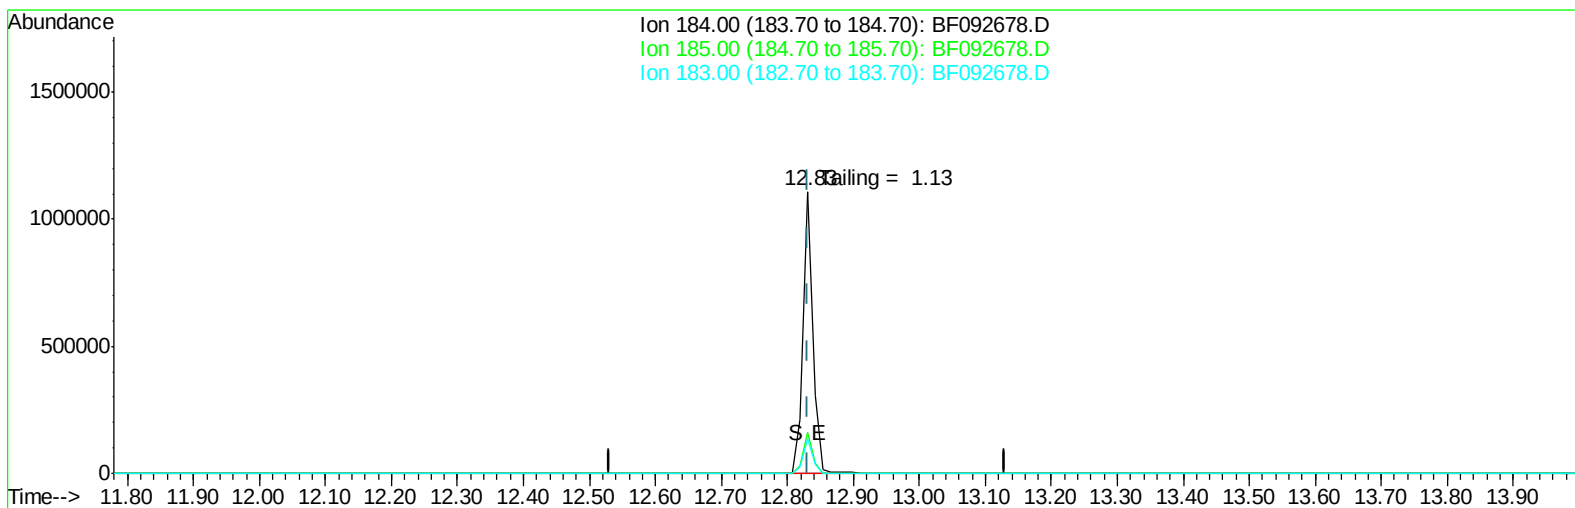

TIC: BF092678.D

(76) Benzidine

12.831min (-0.000) 58730.51ng

response 1148724

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.48
183.00	11.50	12.36
0.00	0.00	0.00