
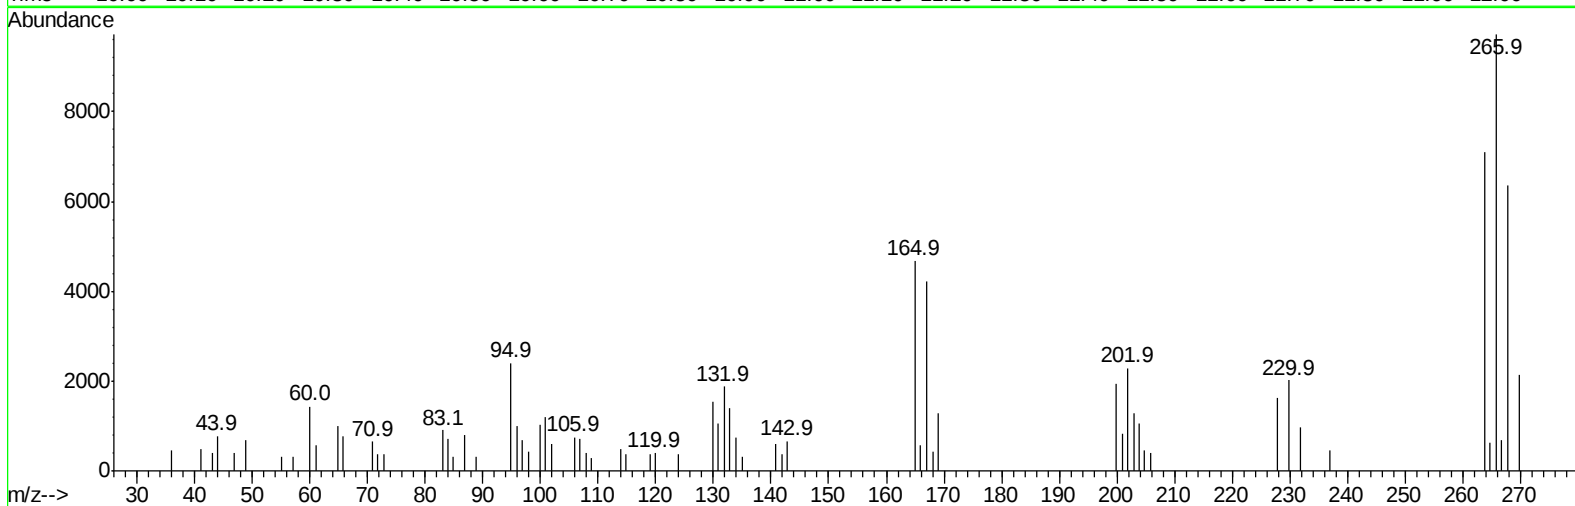


Data Path : U:\HPCHEM1\BNA F\DATA\BF013118\
Data File : BF102684.D
Acq On : 1 Feb 2018 5:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 07:02:18 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 18:38:00 2018
Response via : Initial Calibration

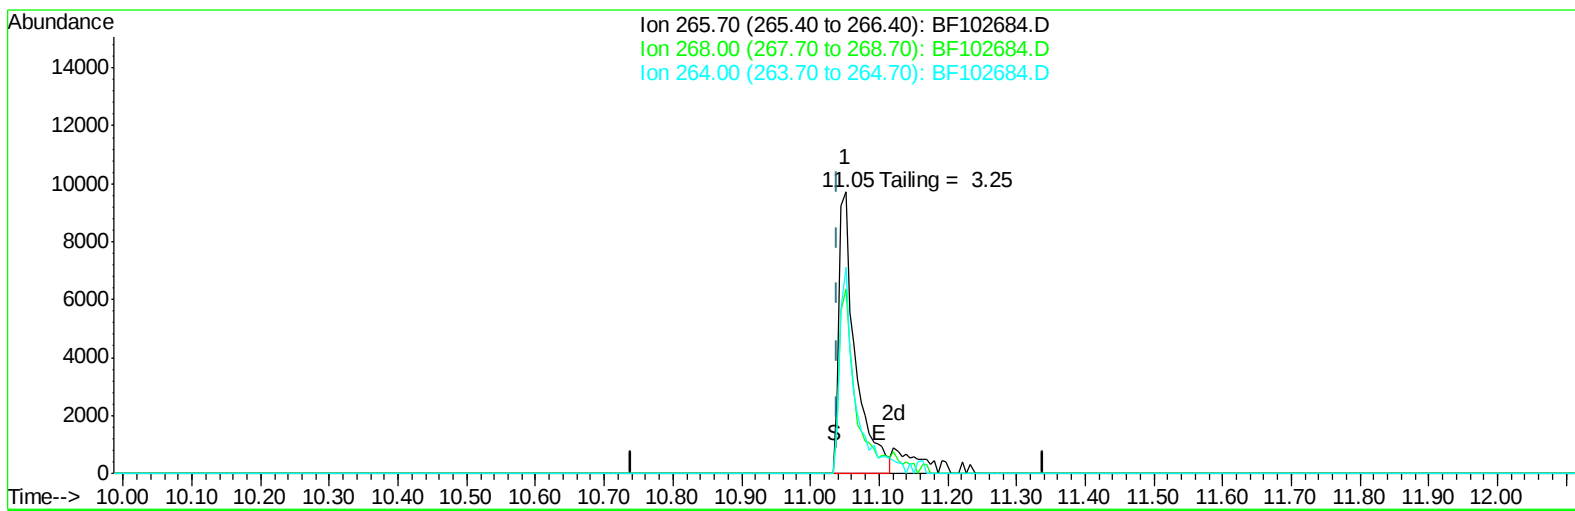

TIC: BF102684.D

(69) Pentachlorophenol (C)

11.051min (+0.012) 0.00ng

response 15829

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.36
264.00	61.90	79.55#
0.00	0.00	0.00