
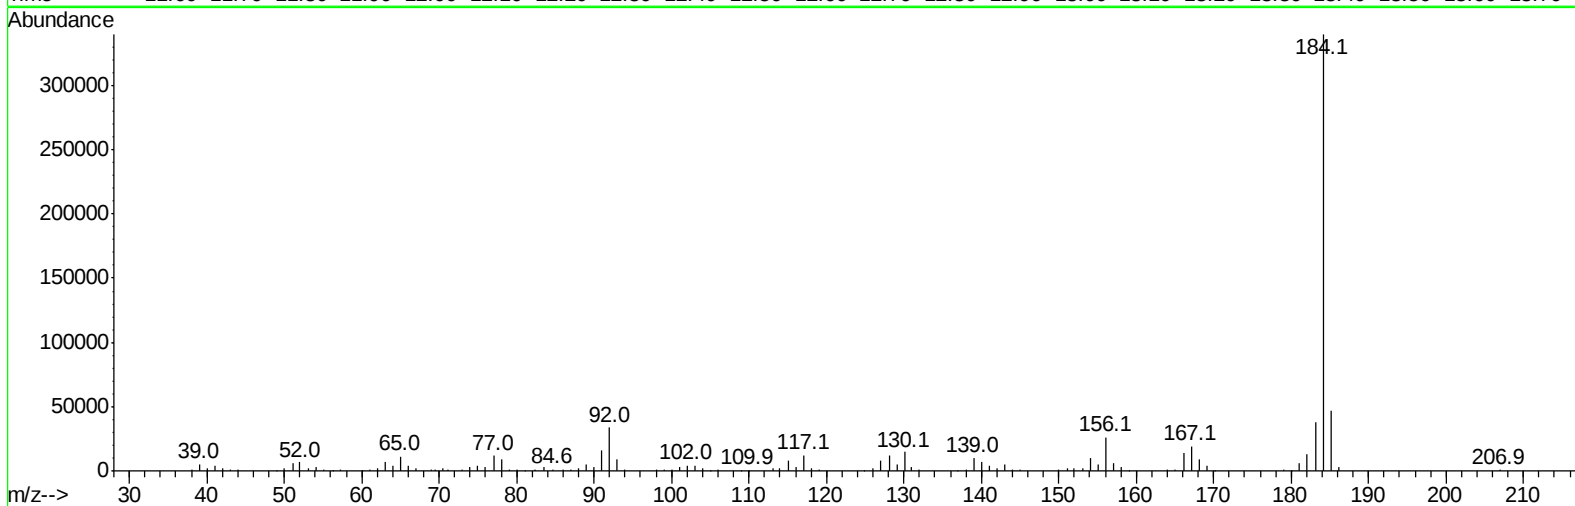


Data Path : U:\HPCHEM1\BNA F\DATA\BF013118\
Data File : BF102658.D
Acq On : 31 Jan 2018 16:22
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 06:55:49 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 18:38:00 2018
Response via : Initial Calibration

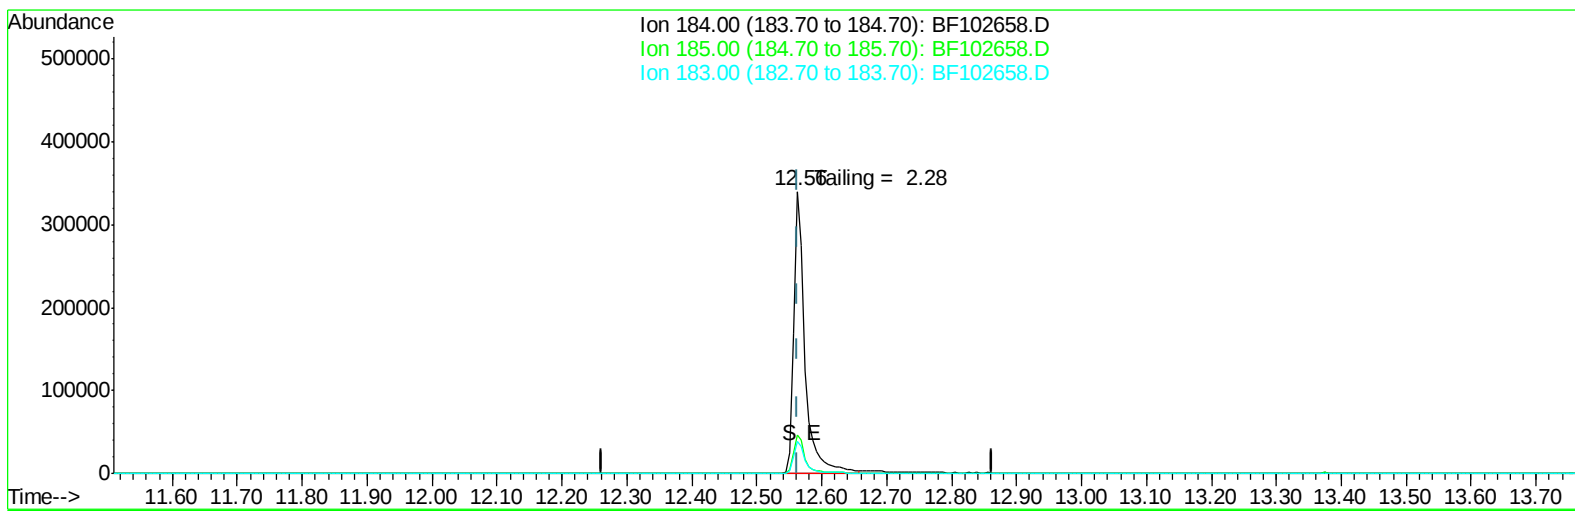

TIC: BF102658.D

(76) Benzidine



12.563min (+0.000) 0.00ng

response 419295

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.66
183.00	11.60	11.26
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF013118\
Data File : BF102658.D
Acq On : 31 Jan 2018 16:22
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 06:55:49 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 18:38:00 2018
Response via : Initial Calibration

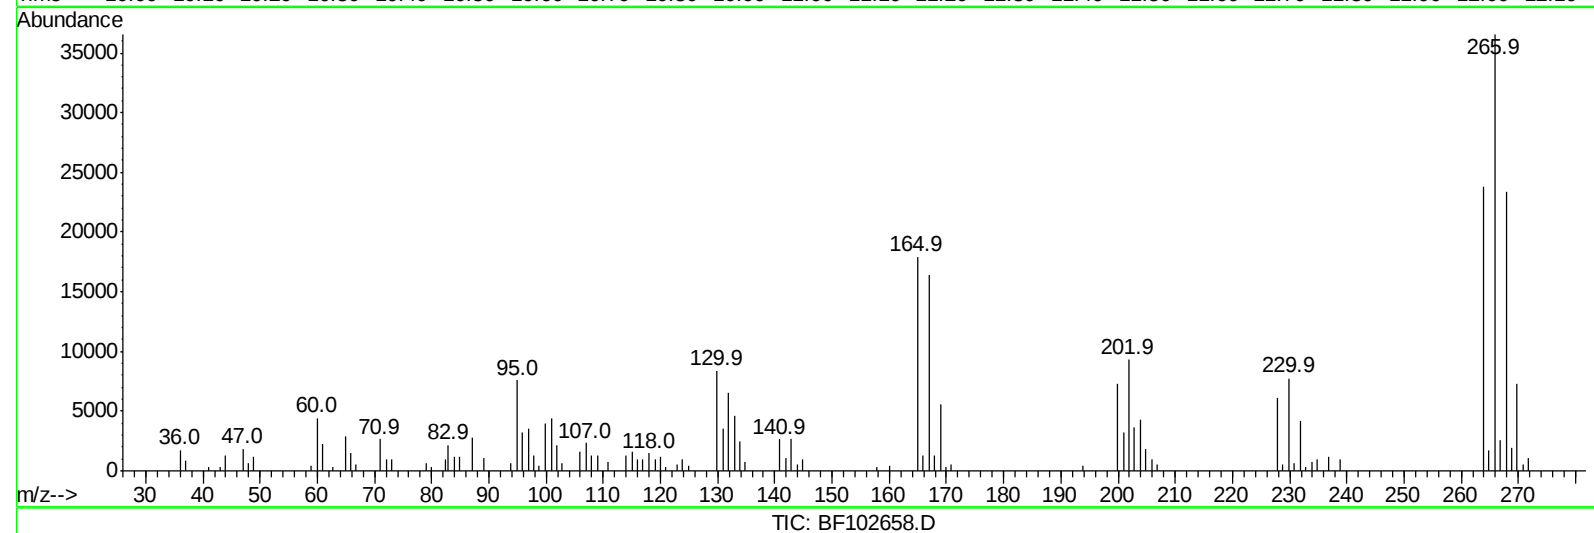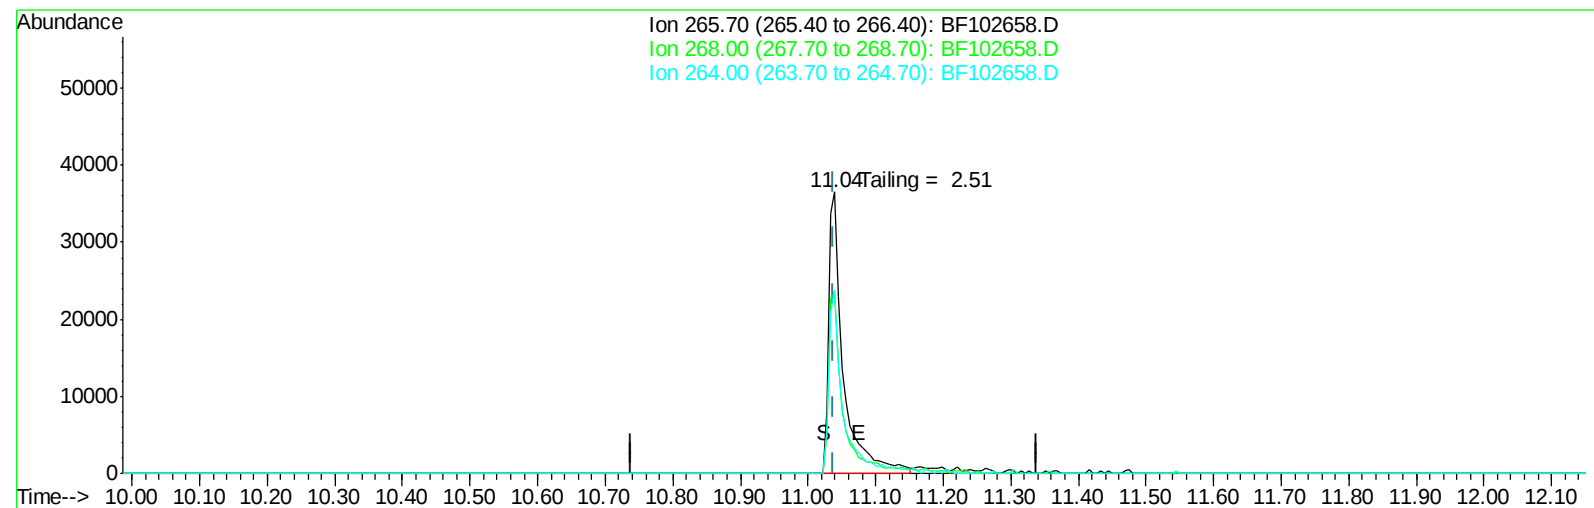

(69) Pentachlorophenol (C)

11.039min (+0.000) 18941.59ng

response 56304

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.89
264.00	61.90	65.05
0.00	0.00	0.00