

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF013118\
 Data File : BF102663.D
 Acq On : 31 Jan 2018 19:10
 Operator : SJ/JU
 Sample : J1015-20 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-02-013018-A

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.340	548	553	556	rBV2	13438	21252	1.75%	0.303%
2	6.386	726	731	736	rBV4	16518	36963	3.04%	0.527%
3	6.486	745	748	758	rBV2	31551	50538	4.15%	0.721%
4	6.698	781	784	801	rBV	749788	815250	66.95%	11.627%
5	6.857	808	811	819	rBV	43623	46185	3.79%	0.659%
6	7.286	881	884	897	rBV2	14951	34179	2.81%	0.487%
7	7.986	999	1003	1026	rBV	1130175	1143585	93.92%	16.309%
8	9.063	1182	1186	1195	rBV	77978	85664	7.04%	1.222%
9	9.457	1250	1253	1258	rVB3	9452	12949	1.06%	0.185%
10	9.733	1297	1300	1314	rVB	1299854	1217670	100.00%	17.366%
11	10.163	1369	1373	1376	rVB2	12730	13811	1.13%	0.197%
12	10.286	1392	1394	1401	rVB2	14467	17045	1.40%	0.243%
13	10.533	1433	1436	1444	rVB3	35438	36841	3.03%	0.525%
14	10.633	1450	1453	1458	rVB3	15583	19996	1.64%	0.285%
15	11.104	1531	1533	1538	rVB4	11294	16488	1.35%	0.235%
16	11.221	1549	1553	1556	rBV	1117191	1049079	86.15%	14.962%
17	11.298	1564	1566	1572	rVB	24811	30851	2.53%	0.440%
18	11.757	1641	1644	1650	rVB3	18082	20981	1.72%	0.299%
19	11.833	1654	1657	1660	rBV2	19783	22658	1.86%	0.323%
20	12.298	1733	1736	1740	rVB6	10089	15813	1.30%	0.226%
21	12.433	1756	1759	1763	rBV	169518	150552	12.36%	2.147%
22	12.663	1792	1798	1805	rBV	131884	162303	13.33%	2.315%
23	12.721	1805	1808	1811	rVB5	10780	13308	1.09%	0.190%
24	12.798	1816	1821	1825	rBV	82711	78980	6.49%	1.126%
25	12.880	1831	1835	1841	rBV8	12208	21185	1.74%	0.302%
26	12.992	1852	1854	1857	rVB2	20594	16548	1.36%	0.236%
27	13.057	1862	1865	1868	rVB3	14861	13679	1.12%	0.195%
28	13.092	1868	1871	1876	rBV5	15179	23754	1.95%	0.339%
29	13.221	1890	1893	1900	rBV8	12937	20687	1.70%	0.295%
30	13.504	1939	1941	1948	rBV6	10848	14571	1.20%	0.208%
31	13.857	1996	2001	2005	rBV2	747993	801481	65.82%	11.430%
32	14.227	2062	2064	2066	rBV2	13859	12503	1.03%	0.178%
33	14.486	2106	2108	2111	rBV4	17050	18782	1.54%	0.268%
34	14.874	2172	2174	2177	rBV	52054	66619	5.47%	0.950%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF013118\
Data File : BF102663.D
Acq On : 31 Jan 2018 19:10
Operator : SJ/JU
Sample : J1015-20 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-013018-A

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	15.227	2231	2234	2238	rVB	48073	55931	4.59%	0.798%
36	15.280	2238	2243	2254	rBV	605987	833099	68.42%	11.881%


Sum of corrected areas: 7011780

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF013118\
Data File : BF102663.D
Acq On : 31 Jan 2018 19:10
Operator : SJ/JU
Sample : J1015-20 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-013018-A

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

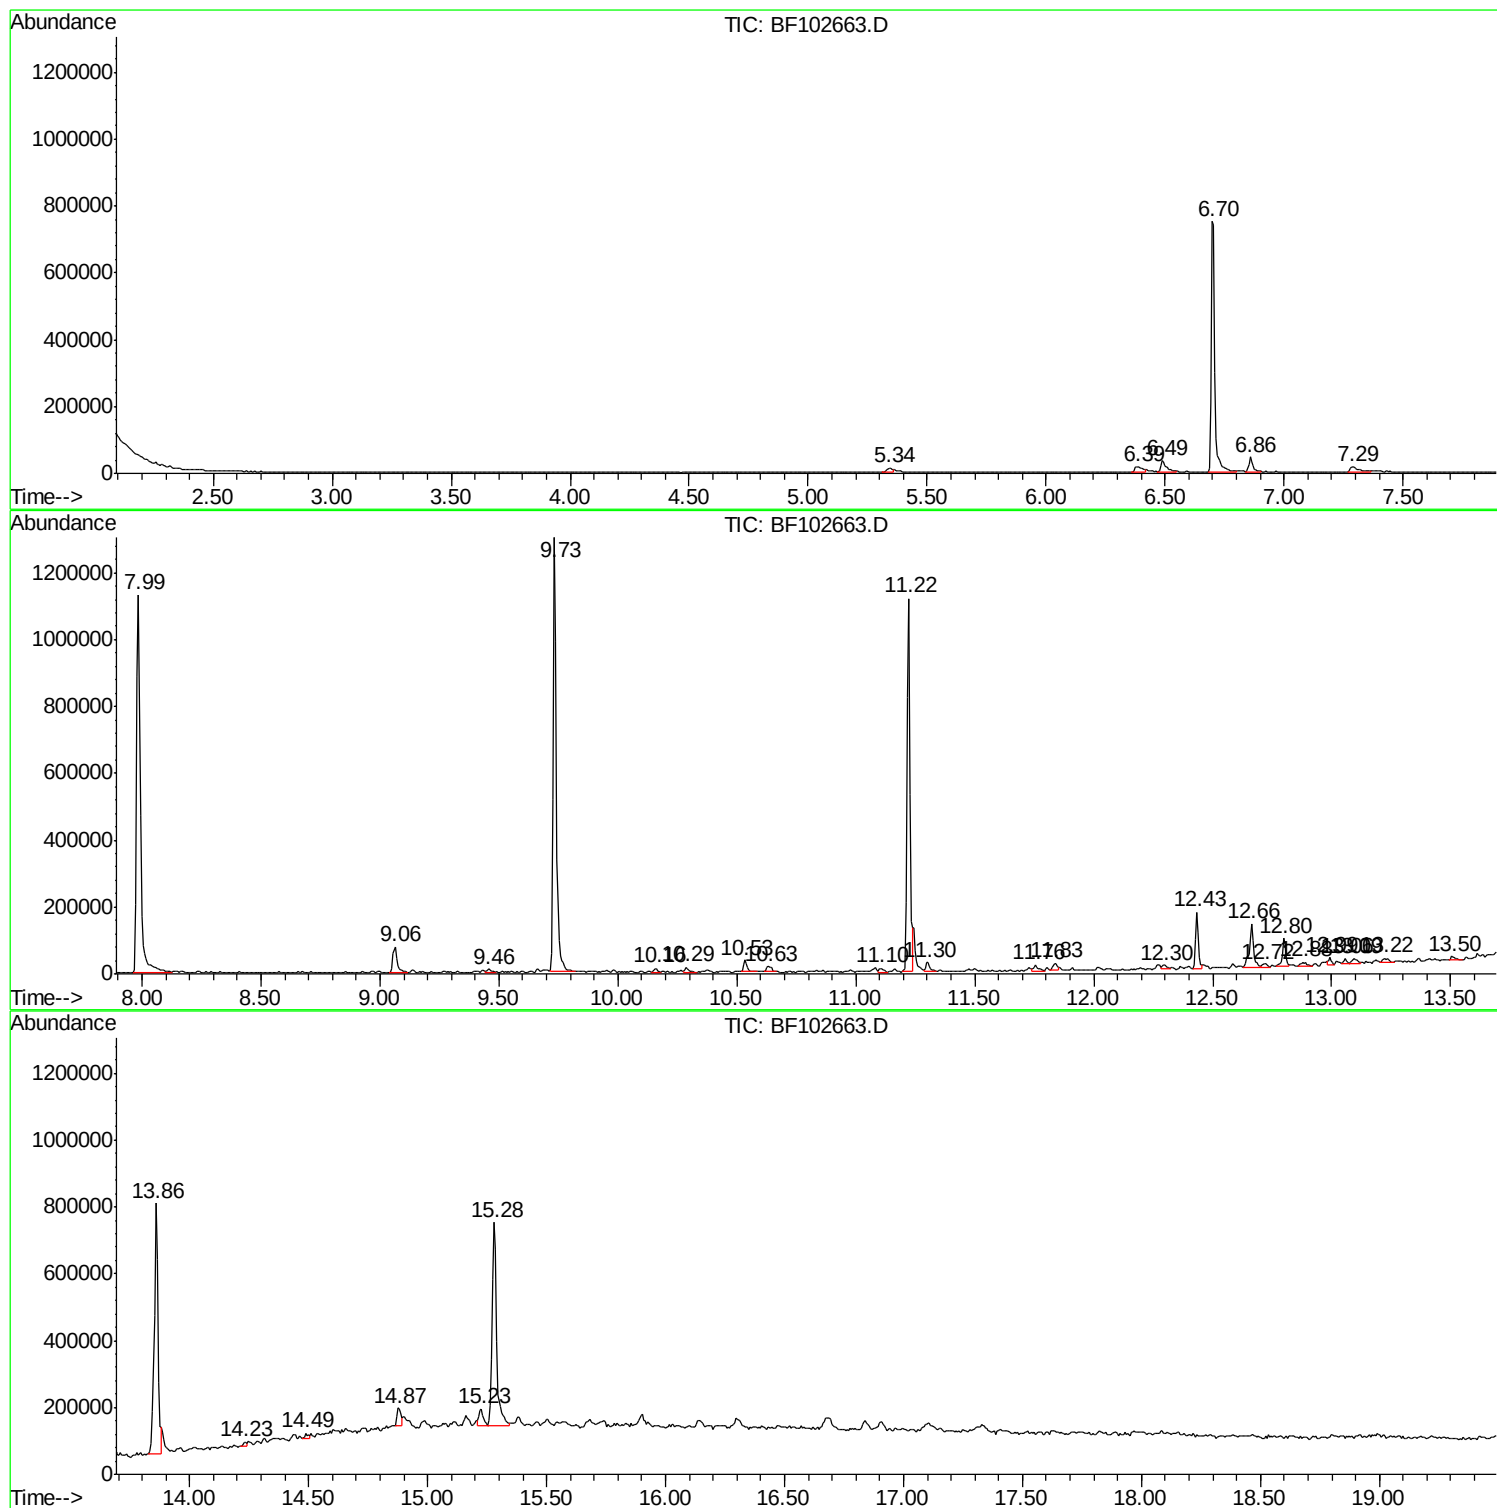

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF013118\
Data_File : BF102663.D
Acq_On : 31-Jan-2018 19:100
Operator : SJ/JUU
Sample : J1015-20-10XX
Misc :
ALS_Vial : 6 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
CL-02-013018-A

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
