


Data Path : Z:\HPCHEM1\BNA F\Data\BF013118\
 Data File : BF102658.D
 Acq On : 31 Jan 2018 16:22
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 31 18:38:00 2018

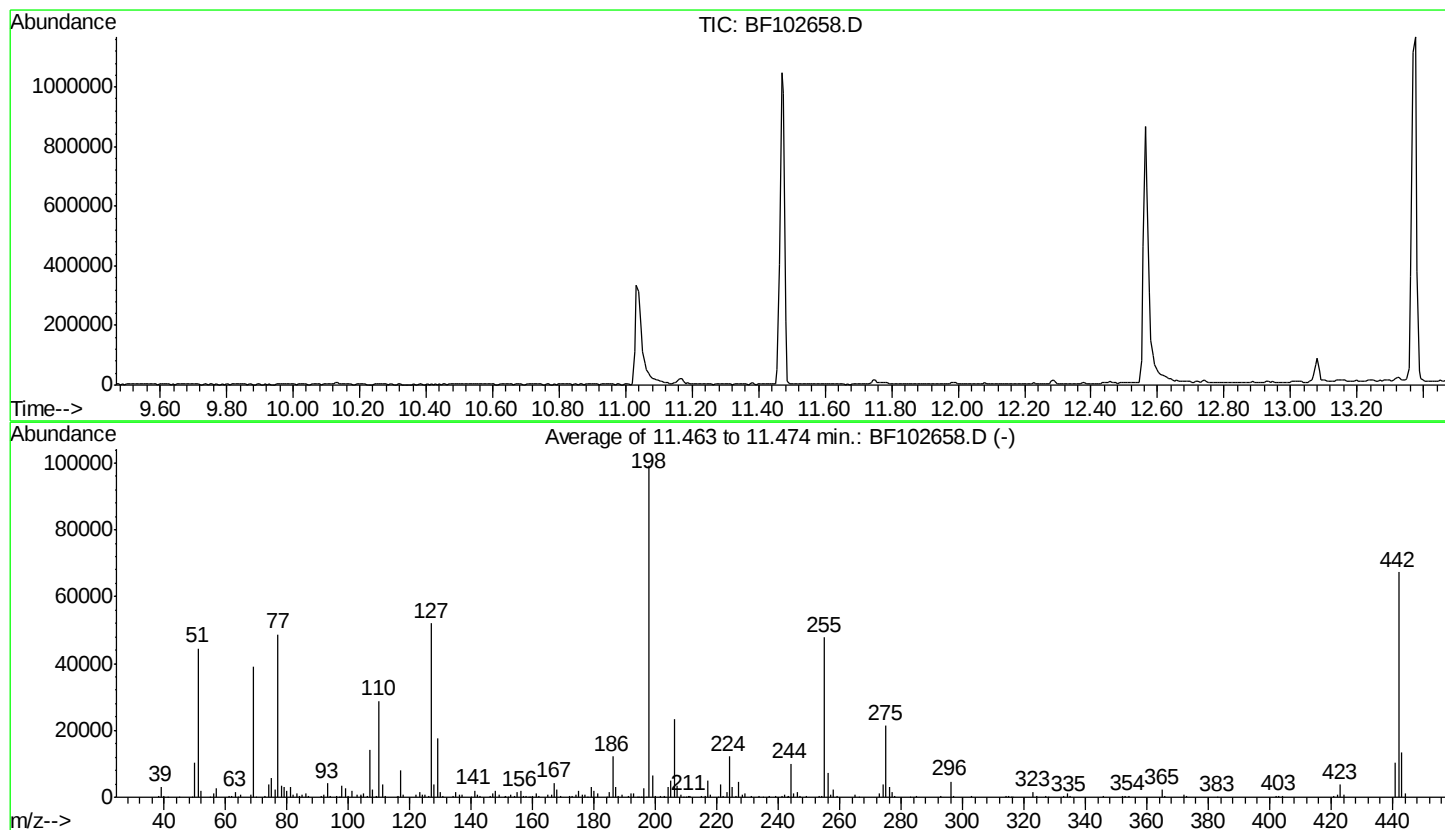

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.9	44507	PASS
68	69	0.00	2	1.8	694	PASS
69	198	0.00	100	39.3	39016	PASS
70	69	0.00	2	0.4	160	PASS
127	198	10	80	52.4	52021	PASS
197	198	0.00	2	0.1	124	PASS
198	198	100	100	100.0	99221	PASS
199	198	5	9	6.8	6710	PASS
275	198	10	60	21.5	21345	PASS
365	198	1	100	2.3	2289	PASS
441	443	0.01	100	78.8	10517	PASS
442	198	50	100	67.8	67242	PASS
443	442	15	24	19.9	13351	PASS