
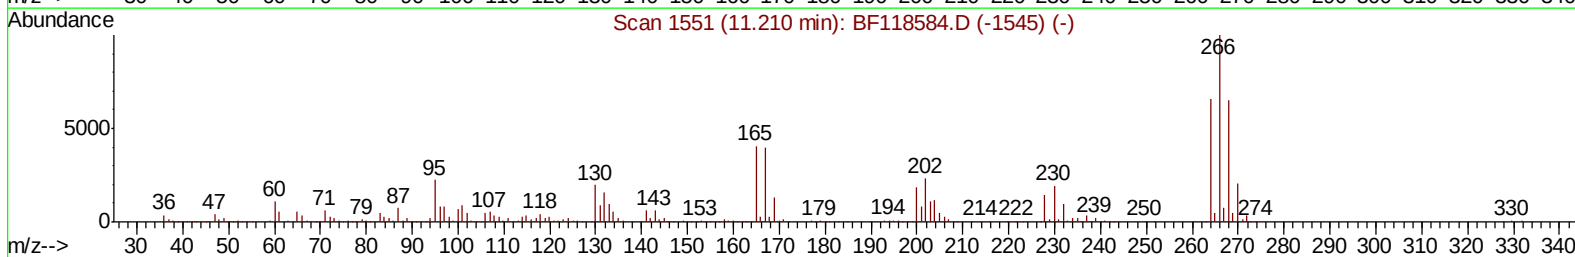
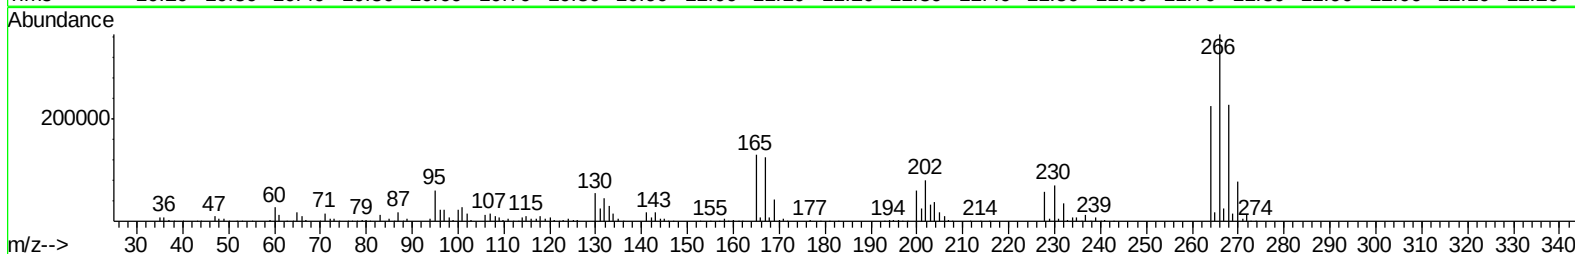


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF013120\
Data File : BF118773.D
Acq On : 31 Jan 2020 11:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 23:00:54 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 27 14:24:10 2020
Response via : Initial Calibration

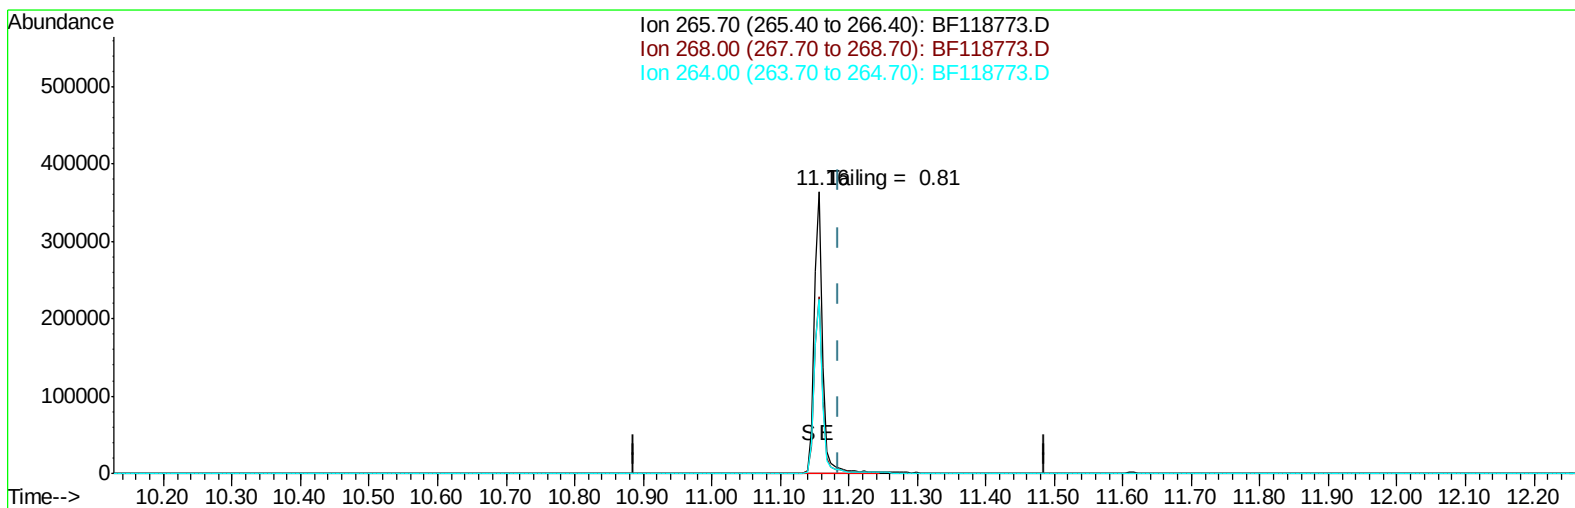

TIC: BF118773.D

(70) Pentachlorophenol (C)




11.157min (-0.030) 27681.73ng

response 322716

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	62.68
264.00	63.60	61.67
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF013120\
 Data File : BF118773.D
 Acq On : 31 Jan 2020 11:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 23:00:54 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 27 14:24:10 2020
 Response via : Initial Calibration

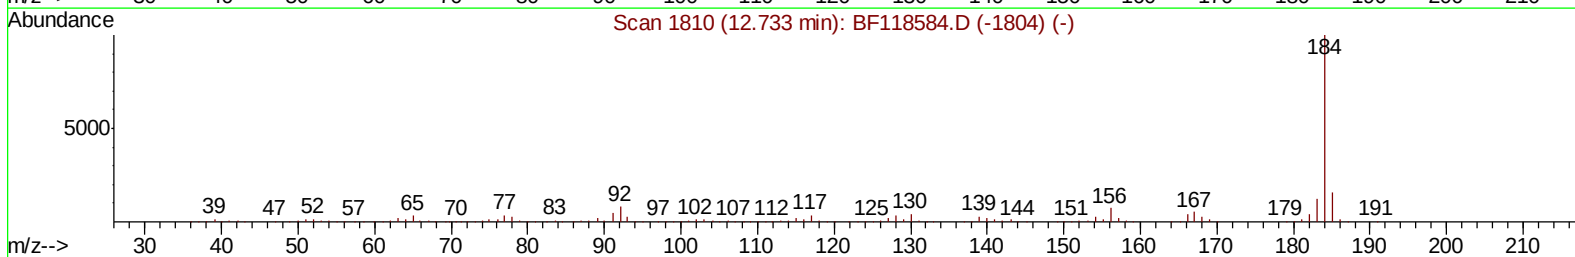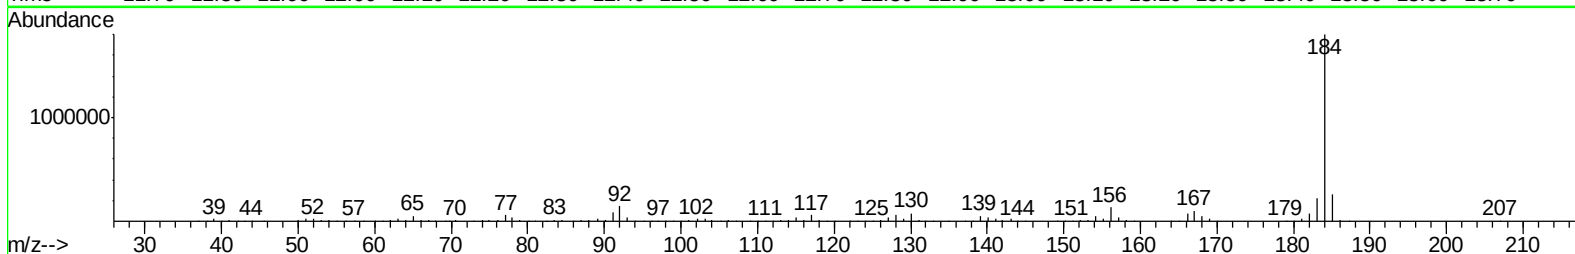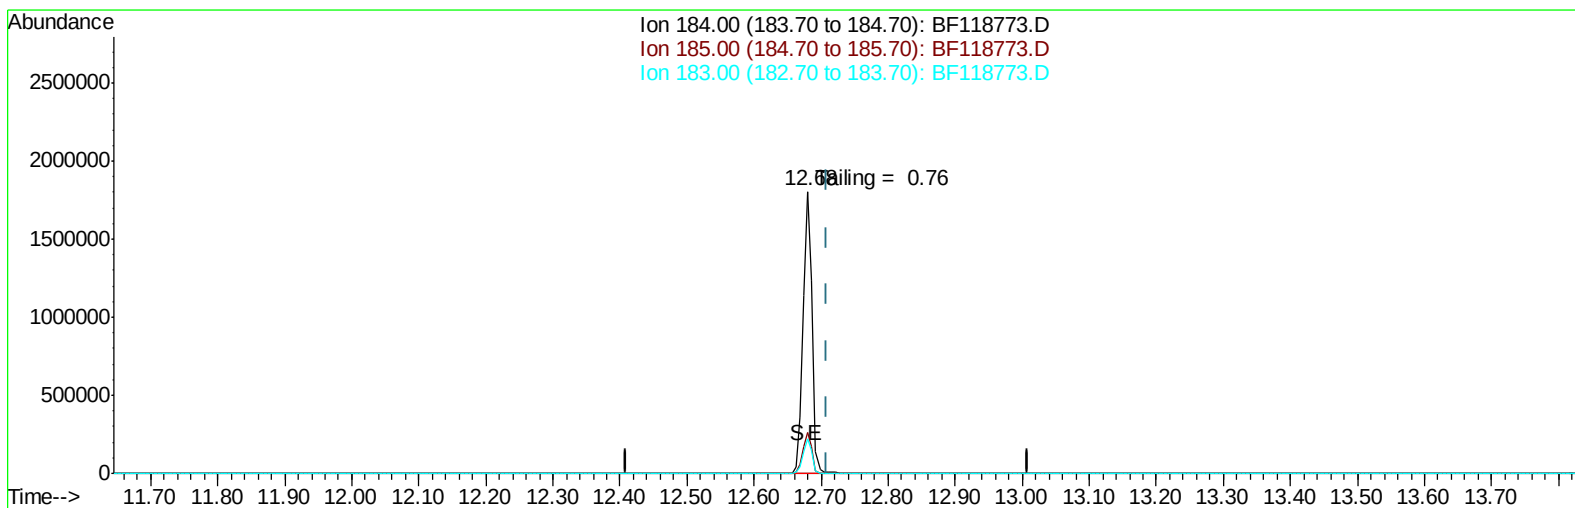

TIC: BF118773.D

(77) Benzidine

12.680min (-0.030) 0.00ng

response 1698092

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.74
183.00	12.10	12.44
0.00	0.00	0.00