


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF013120\
 Data File : BF118773.D
 Acq On : 31 Jan 2020 11:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 27 14:24:10 2020

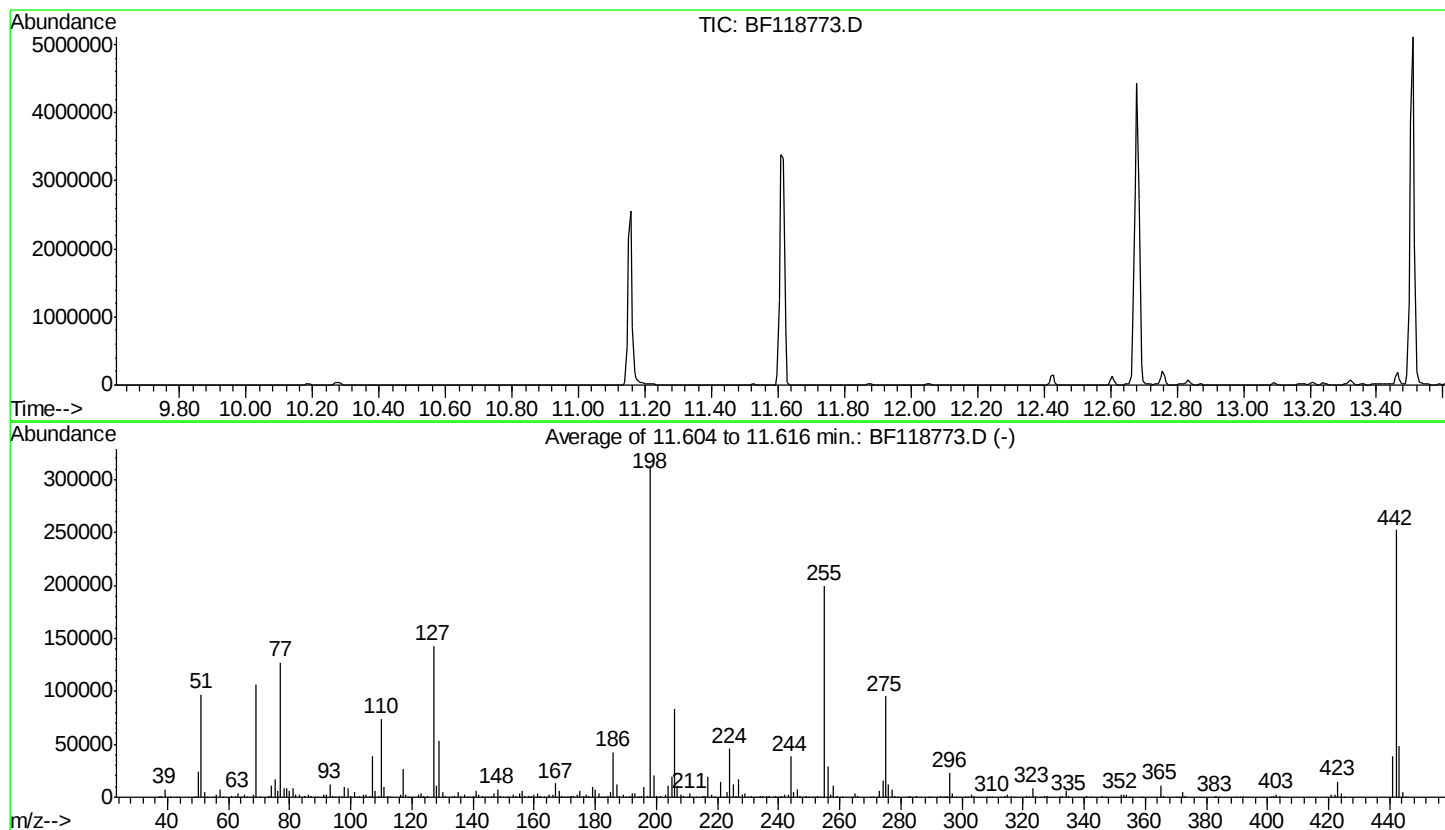

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.9	96872	PASS
68	69	0.00	2	1.9	2061	PASS
69	198	0.00	100	34.2	106917	PASS
70	69	0.00	2	0.5	549	PASS
127	198	10	80	45.6	142669	PASS
197	198	0.00	2	0.6	1848	PASS
198	198	100	100	100.0	313066	PASS
199	198	5	9	6.5	20481	PASS
275	198	10	60	30.4	95218	PASS
365	198	1	100	3.6	11129	PASS
441	198	0.01	100	12.4	38877	PASS
442	198	50	100	80.6	252440	PASS
443	442	15	24	19.2	48570	PASS