


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013122\
 Data File : BF126740.D
 Acq On : 31 Jan 2022 09:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 27 03:09:40 2022

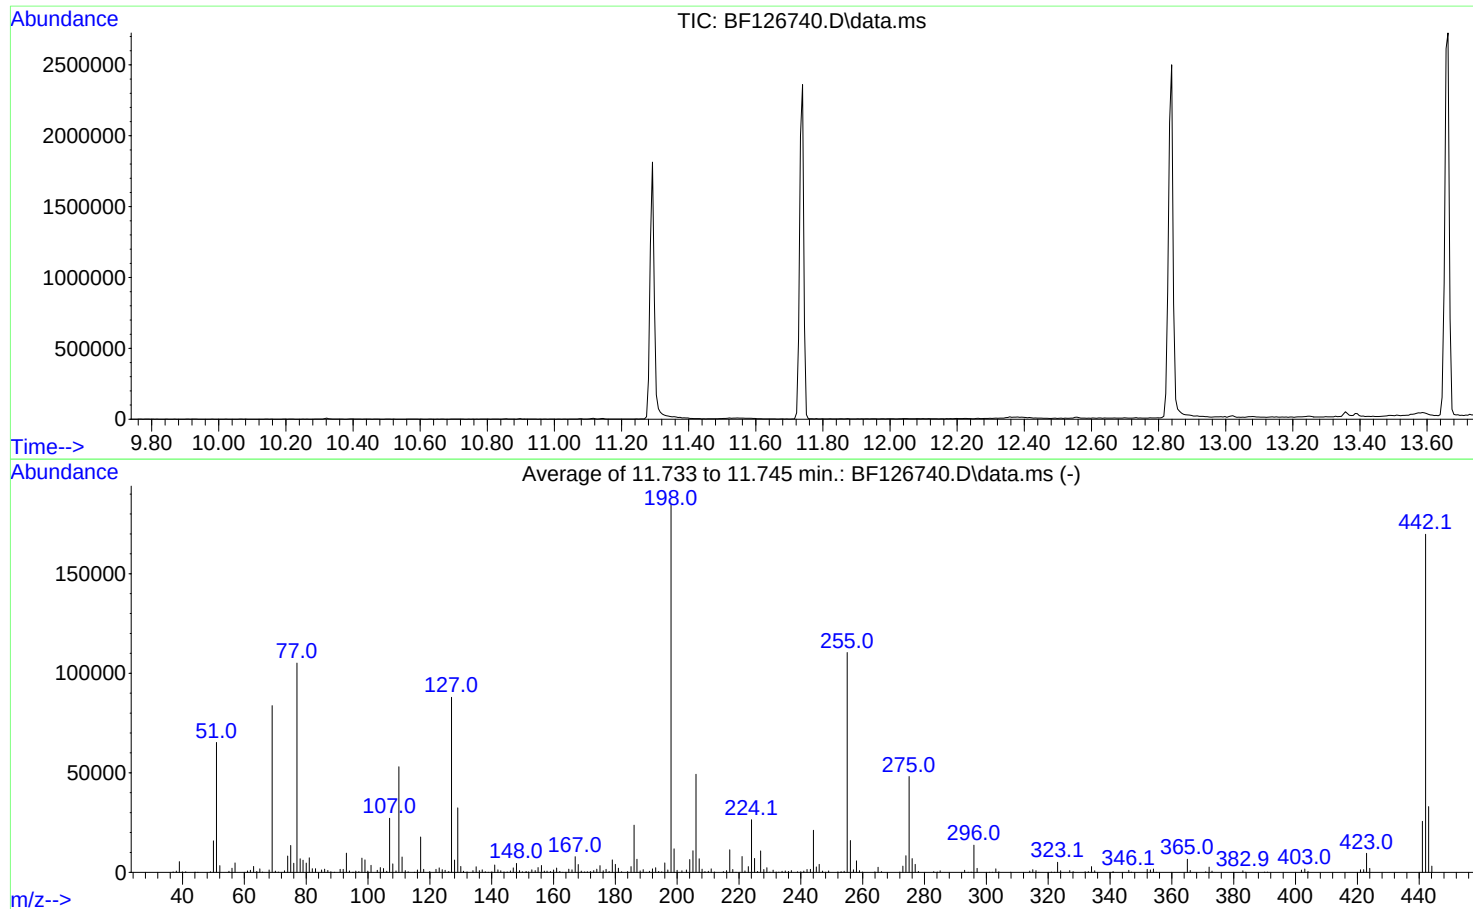




AutoFind: Scans 1640, 1641, 1642; Background Corrected with Scan 1635

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	65234	PASS
68	69	0.00	2	1.5	1229	PASS
69	198	0.00	100	45.3	83747	PASS
70	69	0.00	2	0.8	641	PASS
127	198	10	80	47.6	87947	PASS
197	198	0.00	2	0.6	1190	PASS
198	198	100	100	100.0	184763	PASS
199	198	5	9	6.4	11830	PASS
275	198	10	60	26.0	48107	PASS
365	198	1	100	3.6	6591	PASS
441	198	0.01	100	13.9	25611	PASS
442	442	50	100	100.0	169837	PASS
443	442	15	24	19.4	33021	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013122\
Data File : BF126740.D
Acq On : 31 Jan 2022 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 01 06:28:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 27 03:09:40 2022
Response via : Initial Calibration

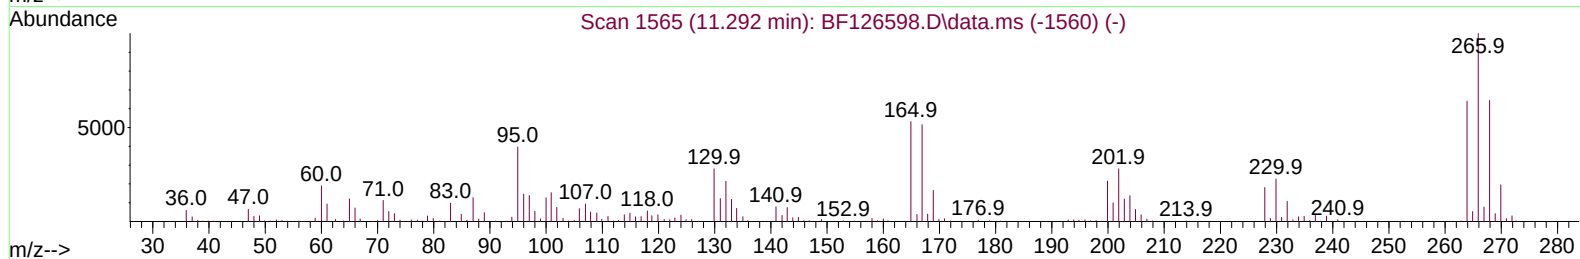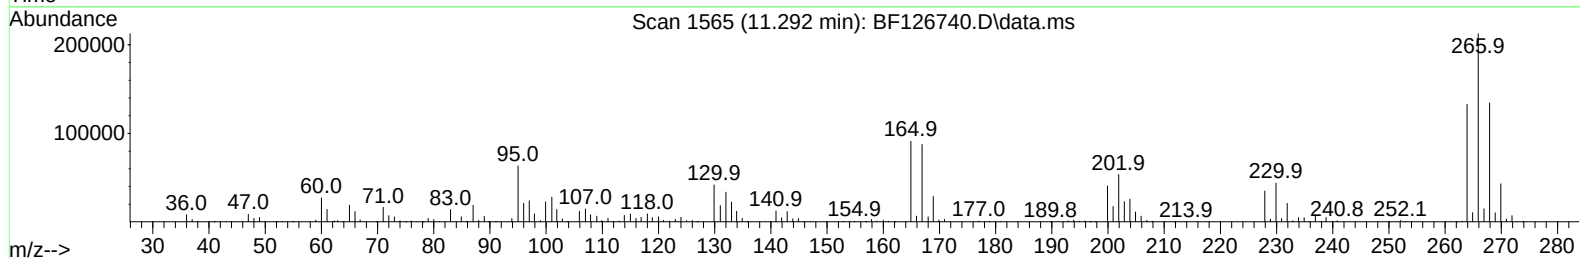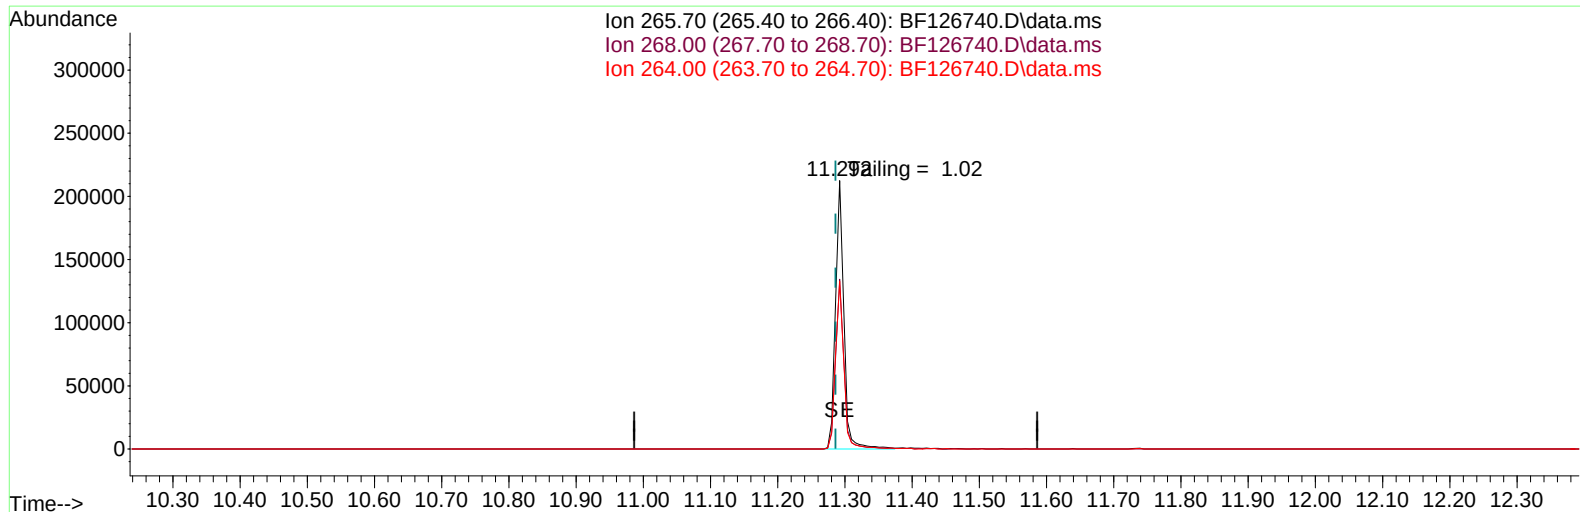

TIC: BF126740.D\data.ms

(70) Pentachlorophenol (C)

11.292min (+ 0.006) 35482.33 ng




response 185462

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	63.28
264.00	63.00	62.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013122\
Data File : BF126740.D
Acq On : 31 Jan 2022 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 01 06:28:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 27 03:09:40 2022
Response via : Initial Calibration

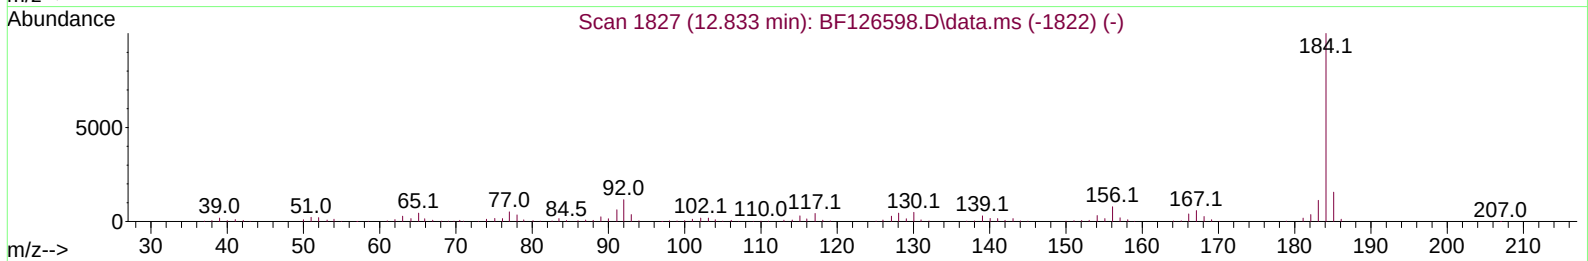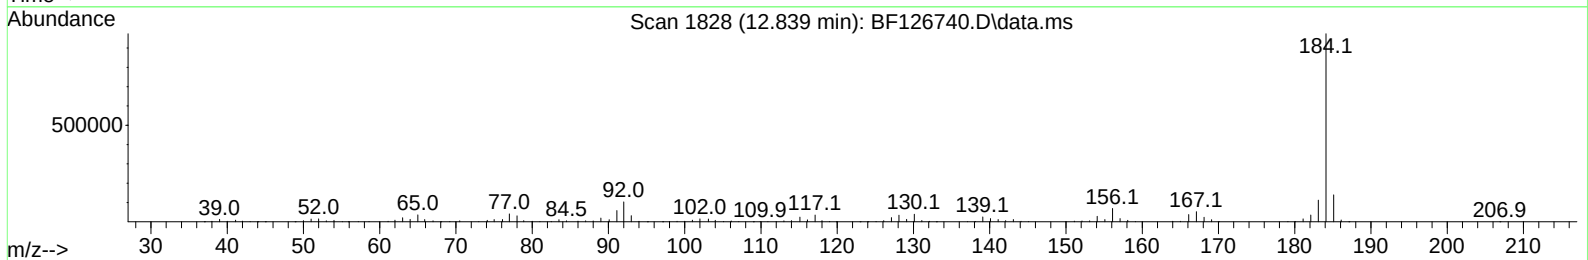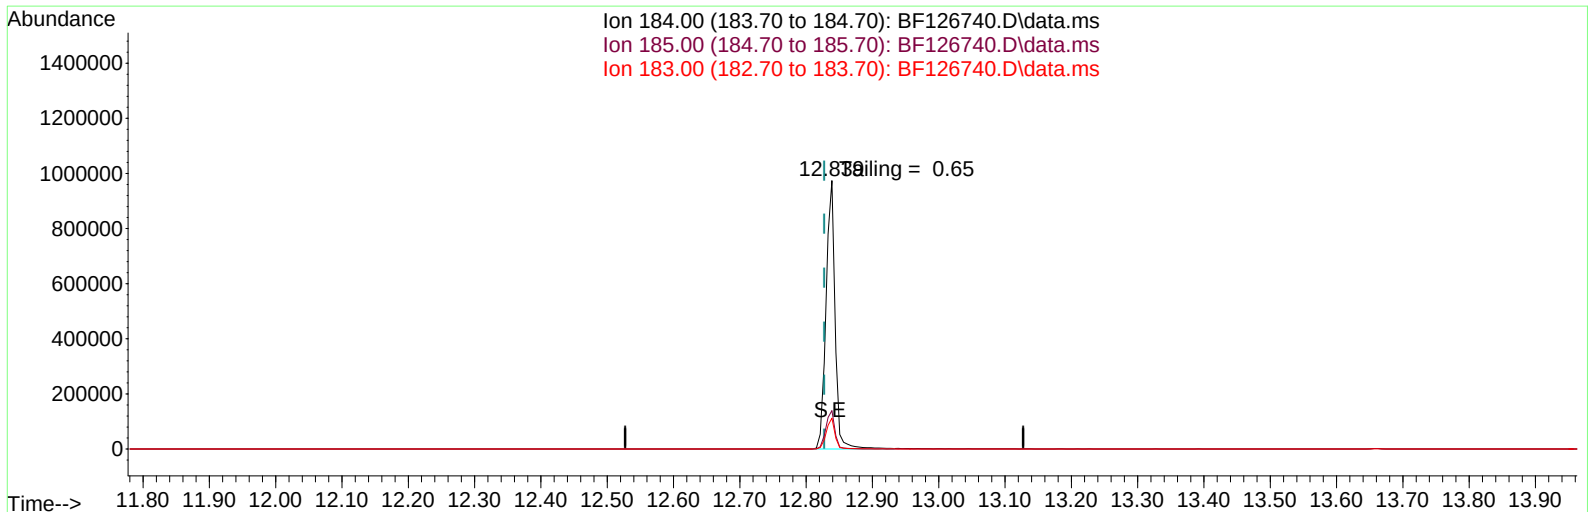

TIC: BF126740.D\data.ms

(77) Benzidine

12.839min (+ 0.012) 0.00 ng

response 930526

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.34
183.00	10.20	11.54
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/31/2022	BNA_F	<u>BF126740.D</u>
Compound Name	Response	Retention Time
DDT	483910	13.662
DDD	7815	13.357
DDE	2016	13.021
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9831	493741	1.99

Instrument :
BNA_F
ClientSampleId :
DFTPP