


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013123\
Data File : BF132233.D
Acq On : 31 Jan 2023 15:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Feb 01 05:24:37 2023

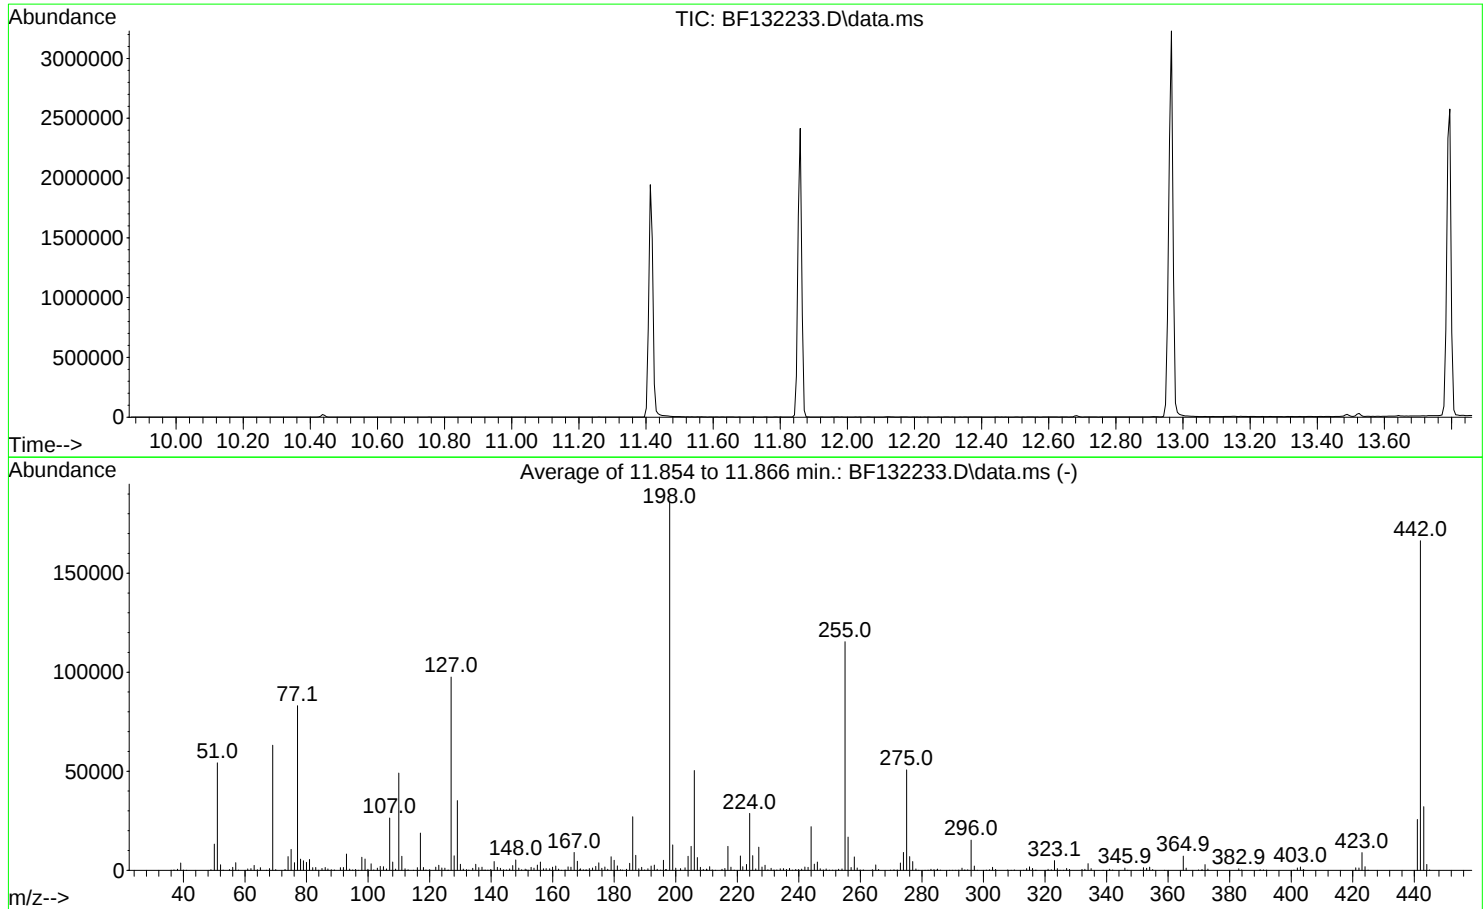




AutoFind: Scans 1533, 1534, 1535; Background Corrected with Scan 1528

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.2	54249	PASS
68	69	0.00	2	1.4	885	PASS
69	198	0.00	100	34.0	63125	PASS
70	69	0.00	2	0.5	343	PASS
127	198	10	80	52.5	97579	PASS
197	198	0.00	2	0.2	380	PASS
198	198	100	100	100.0	185736	PASS
199	198	5	9	6.9	12777	PASS
275	198	10	60	27.3	50699	PASS
365	198	1	100	3.9	7185	PASS
441	198	0.01	100	13.8	25637	PASS
442	442	50	100	100.0	166421	PASS
443	442	15	24	19.3	32117	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013123\
Data File : BF132233.D
Acq On : 31 Jan 2023 15:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 01 07:54:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 01 05:24:37 2023
Response via : Initial Calibration

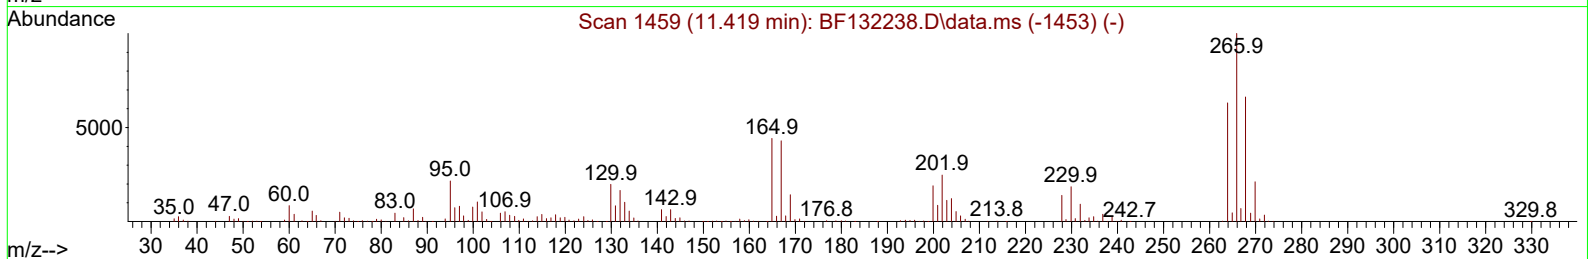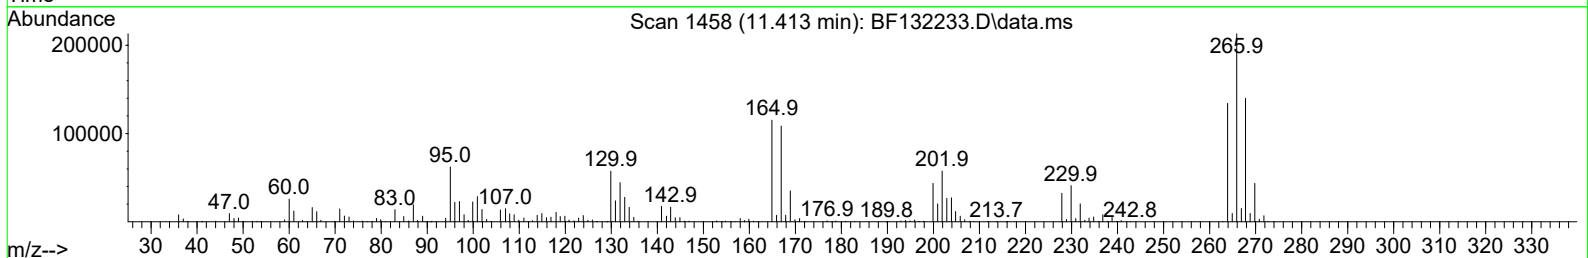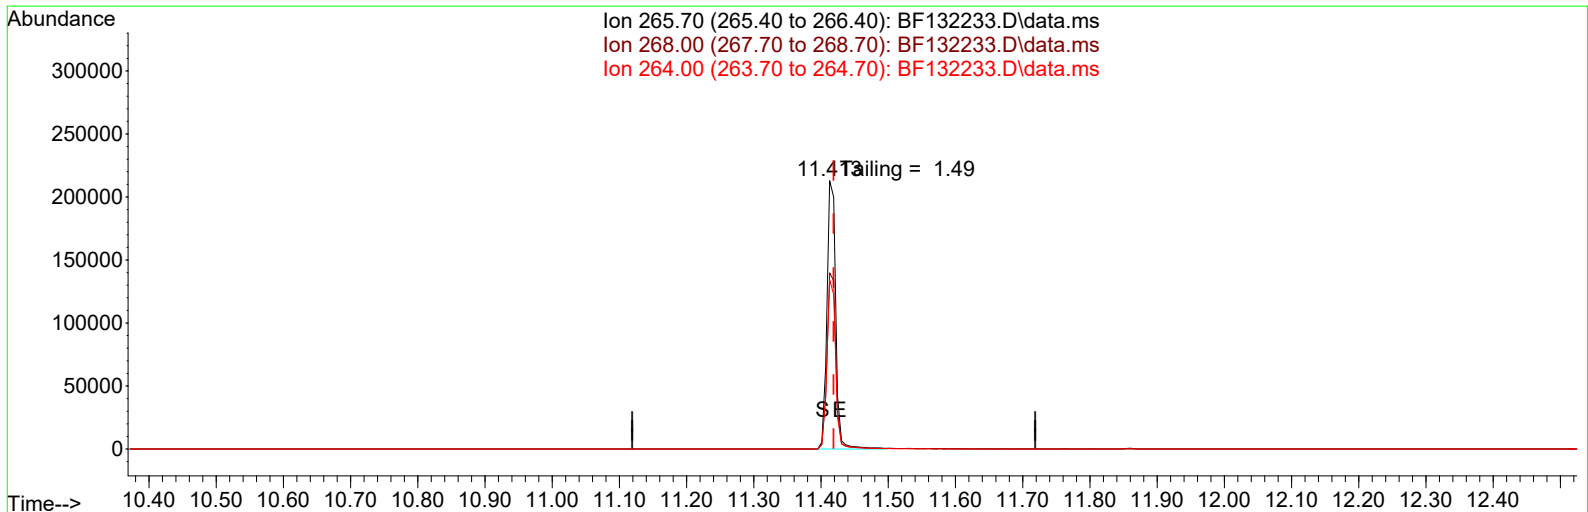

TIC: BF132233.D\data.ms

(70) Pentachlorophenol (C)

11.413min (-0.006) 28137.33 ng




response 194456

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	65.63
264.00	63.10	63.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013123\
Data File : BF132233.D
Acq On : 31 Jan 2023 15:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 01 07:54:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 01 05:24:37 2023
Response via : Initial Calibration

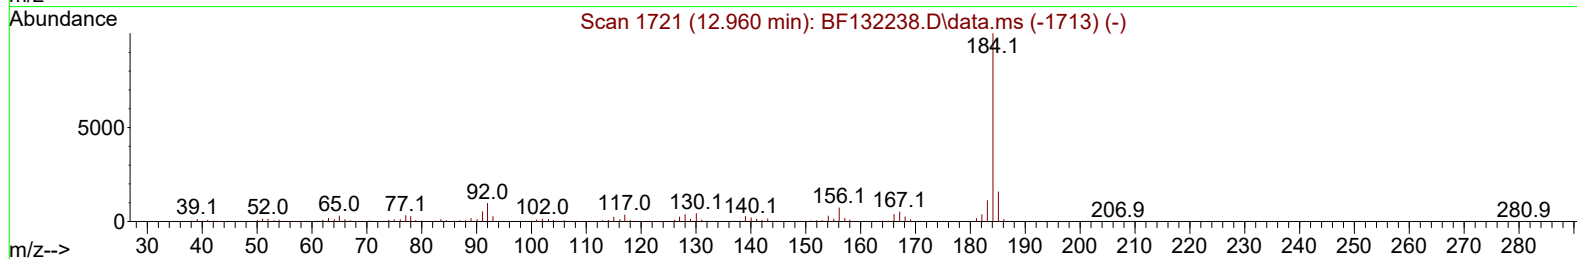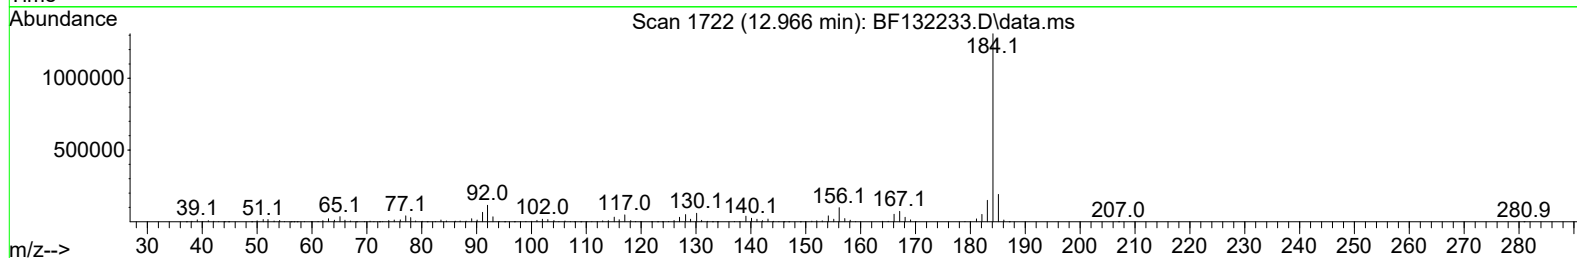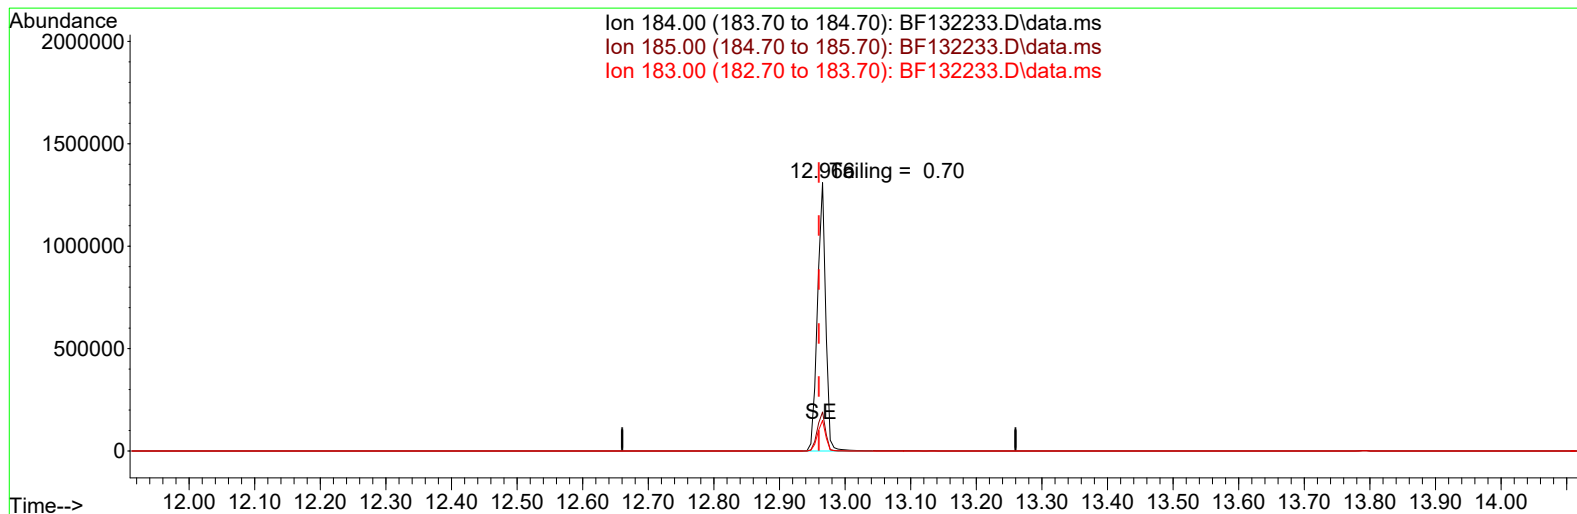

TIC: BF132233.D\data.ms

(77) Benzidine

12.966min (+ 0.006) 0.00 ng

response 1139760

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.59
183.00	11.10	11.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/31/2023	BNA_F	<u>BF132233.D</u>
Compound Name	Response	Retention Time
DDT	428648	13.795
DDD	6697	13.524
DDE	315	13.148
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7012	435660	1.61

Instrument :
BNA_F
ClientSampleId :
DFTPP