
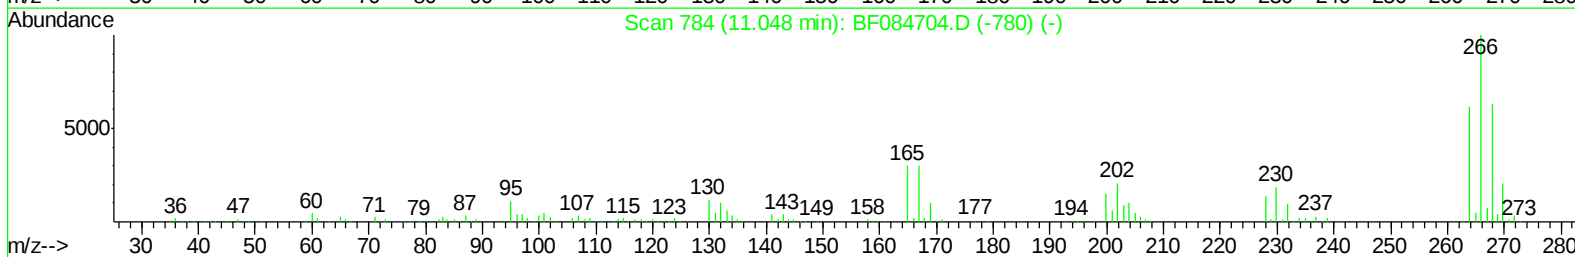
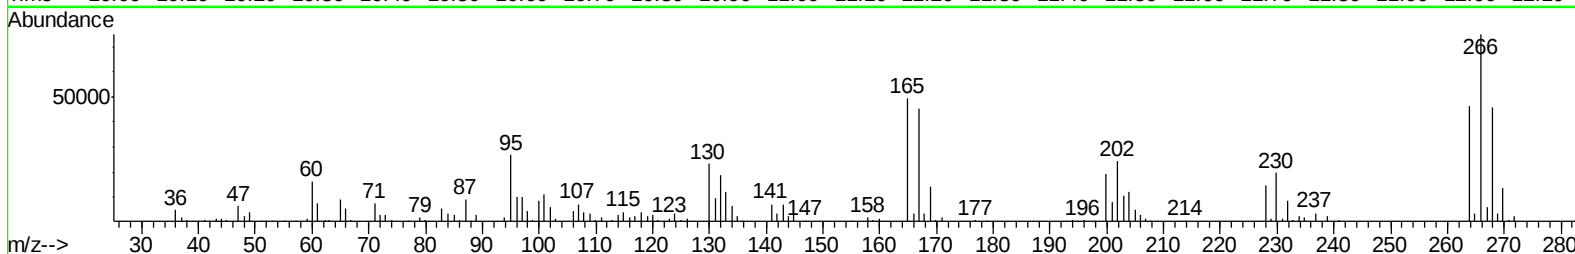


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020116\
Data File : BF084700.D
Acq On : 1 Feb 2016 10:31
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 02 06:42:21 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 01 14:55:11 2016
Response via : Initial Calibration

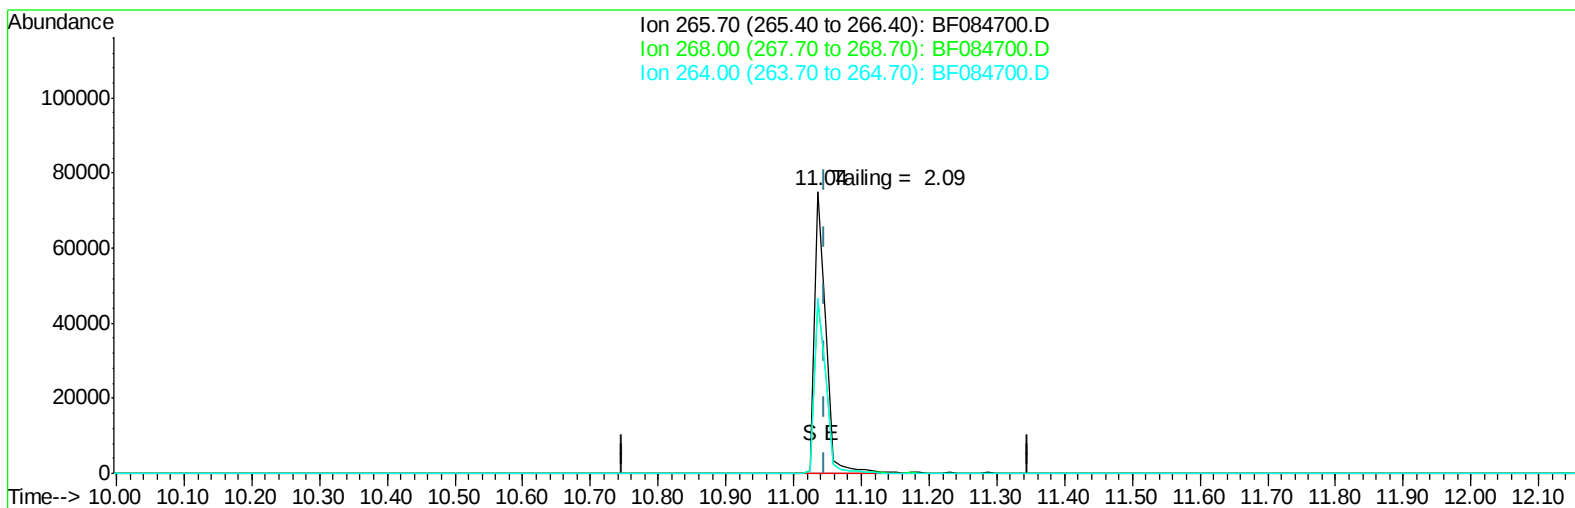

TIC: BF084700.D

(69) Pentachlorophenol (C)




11.036min (-0.011) 0.00ng

response 87531

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	61.00
264.00	62.70	62.14
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020116\
Data File : BF084700.D
Acq On : 1 Feb 2016 10:31
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 02 06:42:21 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 01 14:55:11 2016
Response via : Initial Calibration

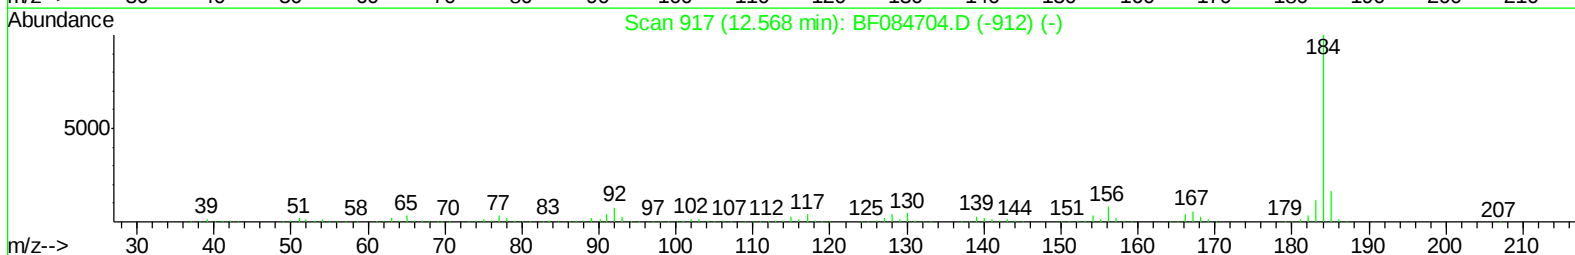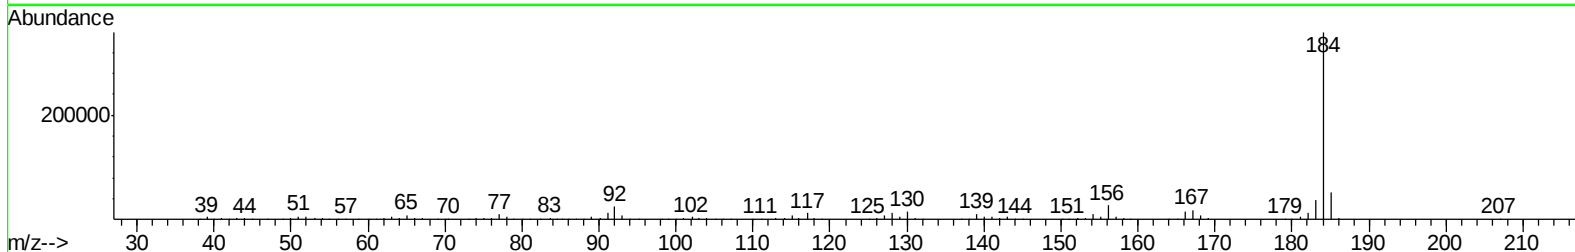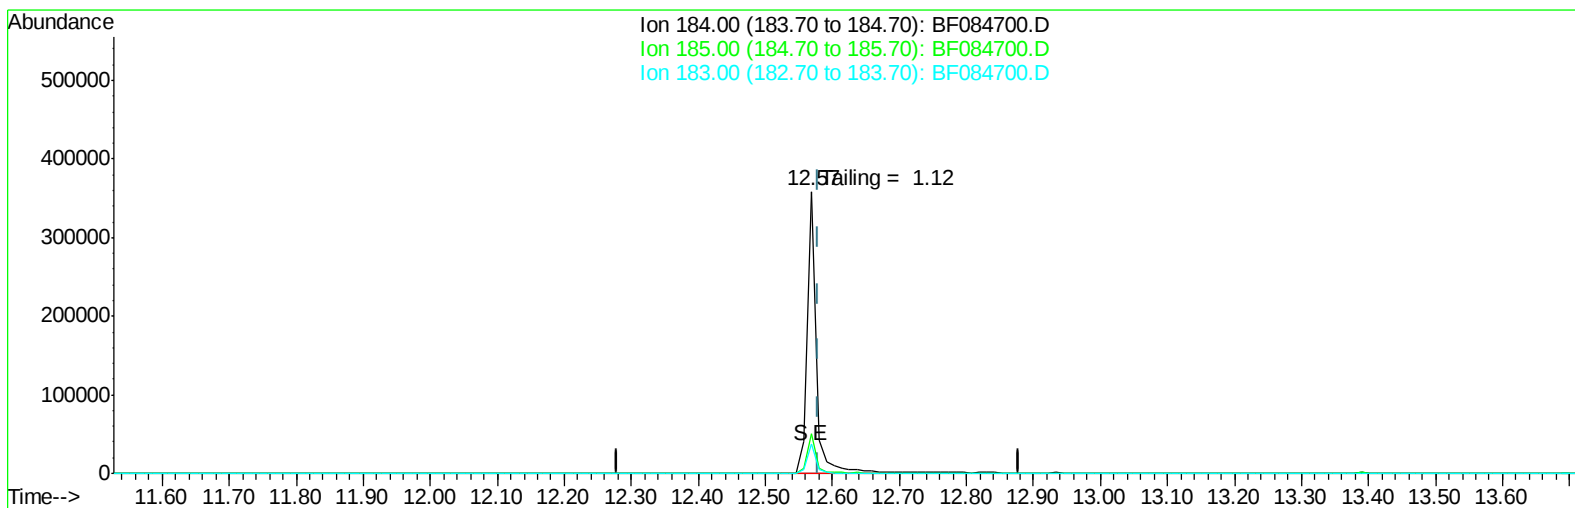

TIC: BF084700.D

(76) Benzidine

12.568min (-0.011) -20.00ng

response 341272

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.26
183.00	12.30	10.64
0.00	0.00	0.00