


Data Path : Z:\HPCHEM1\BNA_F\Data\BF020116\
 Data File : BF084700.D
 Acq On : 1 Feb 2016 10:31
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 01 14:55:11 2016

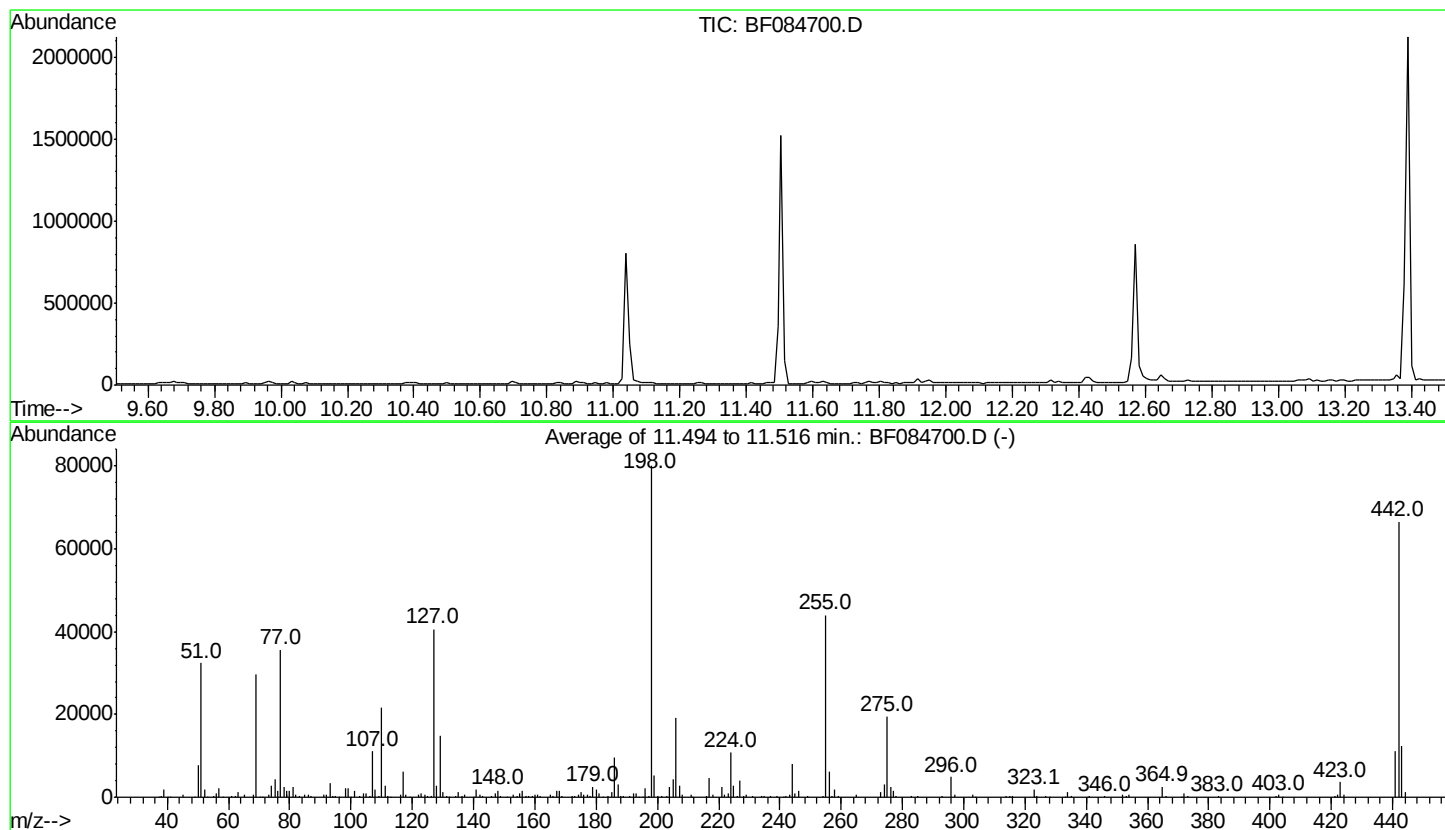

AutoFind: Scans 823, 824, 825; Background Corrected with Scan 820

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	32383	PASS
68	69	0.00	2	1.9	570	PASS
69	198	0.00	100	37.1	29724	PASS
70	69	0.00	2	0.5	138	PASS
127	198	10	80	50.7	40663	PASS
197	198	0.00	2	0.5	386	PASS
198	198	100	100	100.0	80136	PASS
199	198	5	9	6.4	5124	PASS
275	198	10	60	24.2	19368	PASS
365	198	1	100	3.2	2533	PASS
441	442	0.01	24	16.6	11081	PASS
442	198	50	100	83.1	66619	PASS
443	442	15	24	18.7	12429	PASS