


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020116\
 Data File : BF084722.D
 Acq On : 1 Feb 2016 21:17
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 01 14:55:11 2016

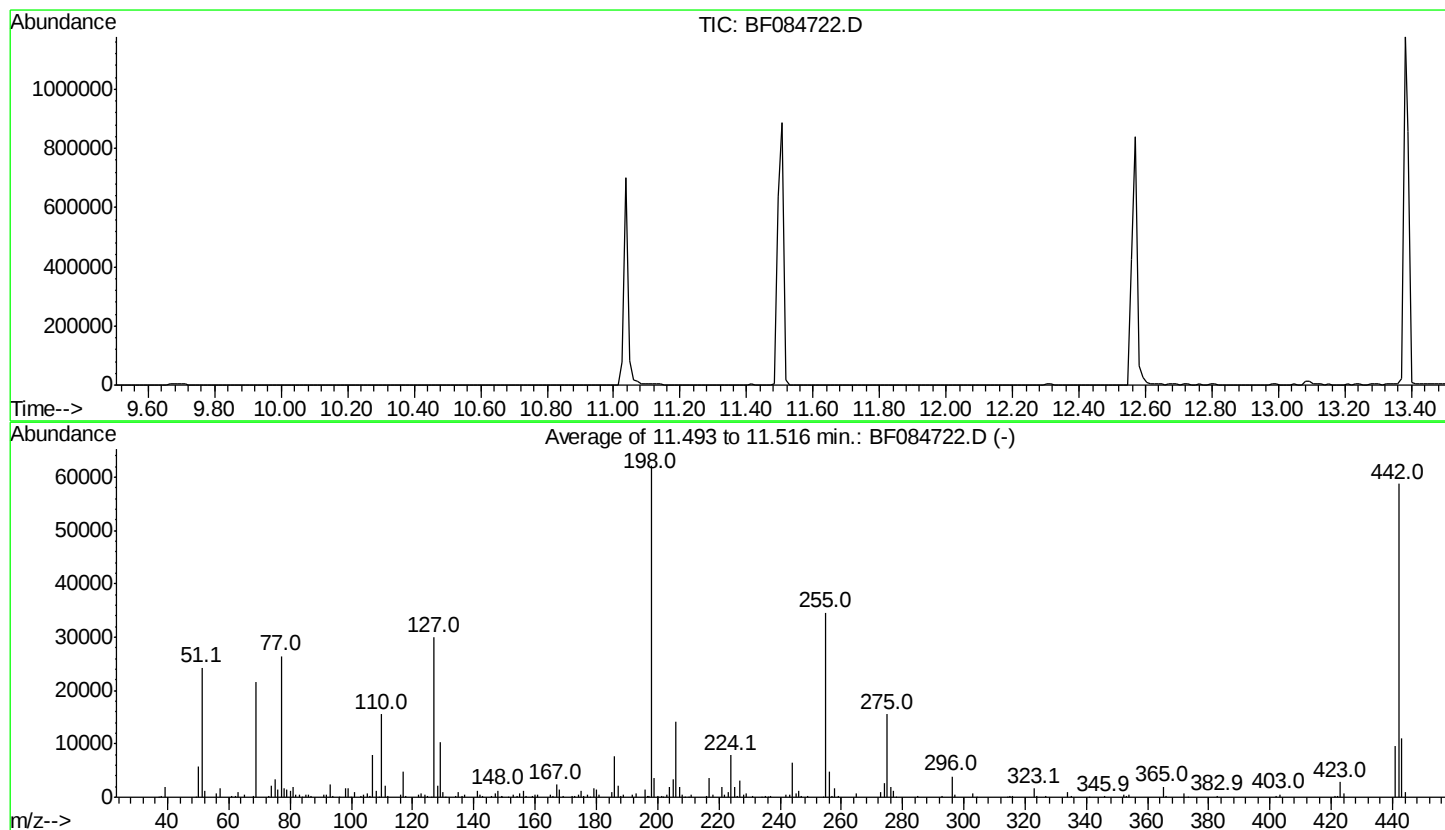

AutoFind: Scans 823, 824, 825; Background Corrected with Scan 819

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	24234	PASS
68	69	0.00	2	1.6	356	PASS
69	198	0.00	100	34.8	21629	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.1	29873	PASS
197	198	0.00	2	0.3	180	PASS
198	198	100	100	100.0	62133	PASS
199	198	5	9	6.0	3704	PASS
275	198	10	60	25.1	15579	PASS
365	198	1	100	3.1	1926	PASS
441	442	0.01	24	16.3	9587	PASS
442	198	50	100	94.6	58753	PASS
443	442	15	24	18.7	10974	PASS