
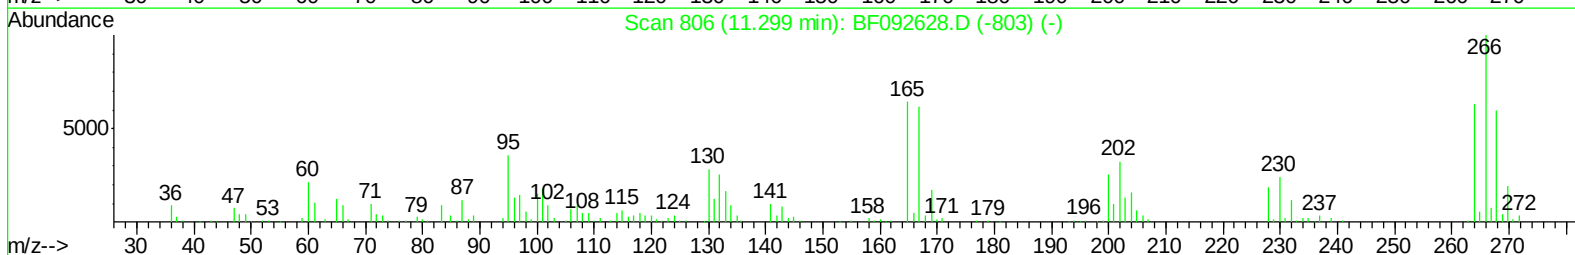
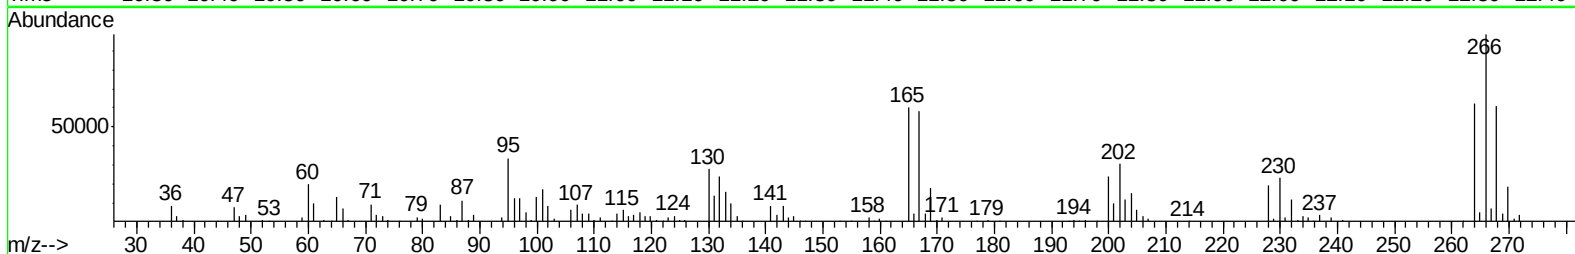


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020117\
Data File : BF092723.D
Acq On : 2 Feb 2017 1:14
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 02 07:47:26 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 30 14:50:05 2017
Response via : Initial Calibration

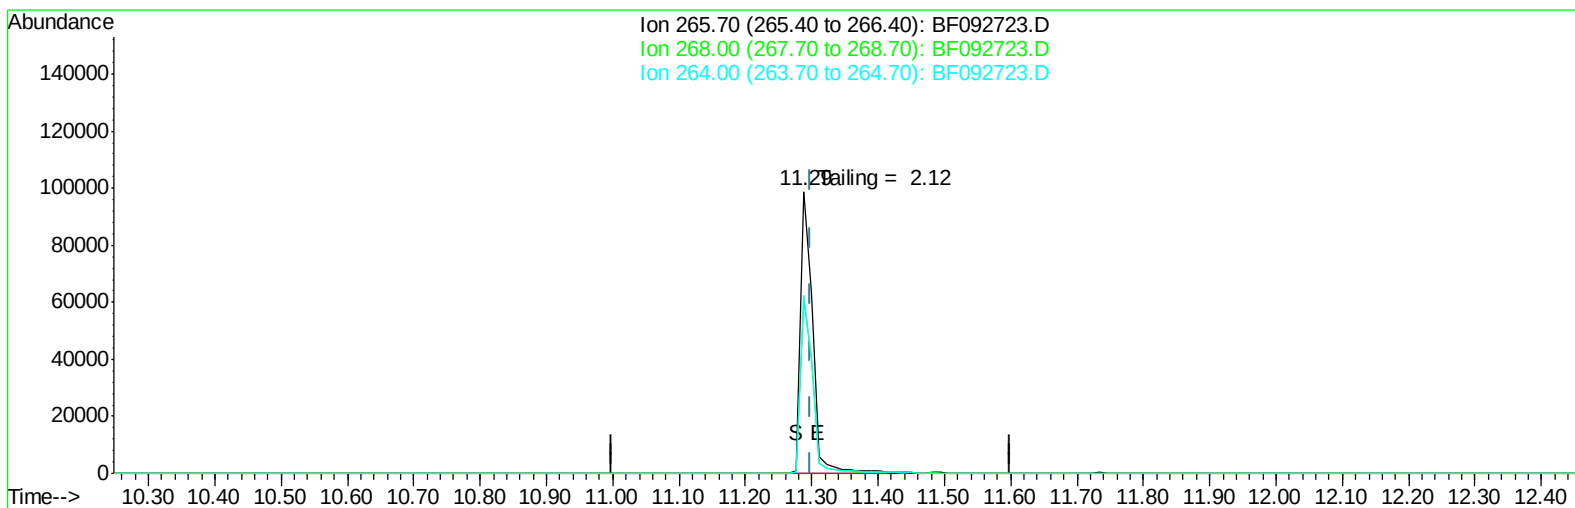

TIC: BF092723.D

(69) Pentachlorophenol (C)




11.288min (-0.011) 86963.16ng

response 124778

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	62.06
264.00	62.90	63.04
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020117\
Data File : BF092723.D
Acq On : 2 Feb 2017 1:14
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 02 07:47:26 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 30 14:50:05 2017
Response via : Initial Calibration

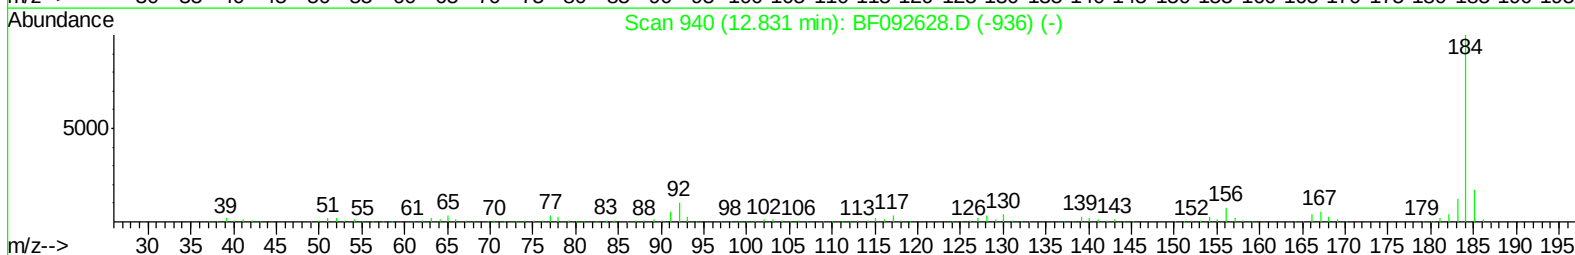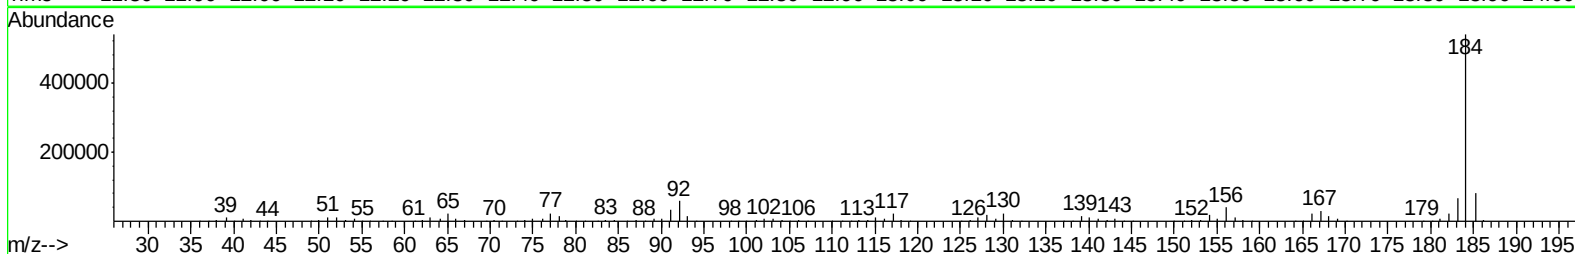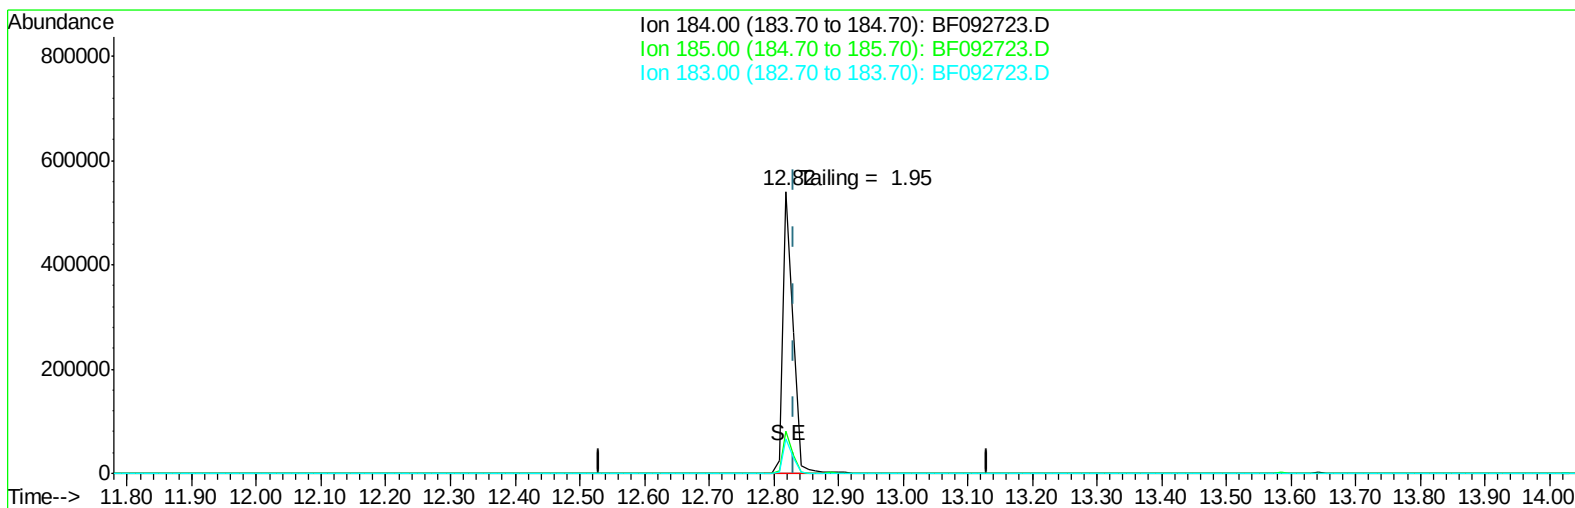

TIC: BF092723.D

(76) Benzidine

12.819min (-0.011) 47371.51ng

response 603570

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	15.00
183.00	11.50	12.44
0.00	0.00	0.00