

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020117\
 Data File : BF092705.D
 Acq On : 1 Feb 2017 15:41
 Operator : SJ/MA
 Sample : PB96625BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB96625BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.498	209	211	216	rBV	38796	64770	1.54%	0.178%
2	5.138	264	267	278	rBV	1375060	1824547	43.33%	5.009%
3	5.561	301	304	307	rBV	3574387	3629928	86.20%	9.966%
4	6.590	391	394	396	rBV	3597533	4210861	100.00%	11.561%
5	6.716	402	405	407	rBV	3943829	3677506	87.33%	10.097%
6	6.944	422	425	427	rBV	1178120	986312	23.42%	2.708%
7	7.104	436	439	441	rBV	3080390	3117549	74.04%	8.559%
8	7.504	471	474	477	rBV	1794406	2547011	60.49%	6.993%
9	8.236	535	538	540	rBV	1322810	1301116	30.90%	3.572%
10	9.310	629	632	635	rBV	3263502	4175992	99.17%	11.465%
11	9.996	689	692	694	rBV	1537588	1413332	33.56%	3.880%
12	10.785	758	761	764	rBV2	1871018	2171493	51.57%	5.962%
13	11.482	820	822	825	rBV	1384527	1299901	30.87%	3.569%
14	13.071	958	961	964	rBV	3675190	3692636	87.69%	10.138%
15	14.122	1050	1053	1055	rBV	1398427	1271706	30.20%	3.491%
16	15.585	1178	1181	1184	rBV	745770	996481	23.66%	2.736%
17	16.557	1262	1266	1270	rBV2	17668	42358	1.01%	0.116%


Sum of corrected areas: 36423499

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020117\
Data File : BF092705.D
Acq On : 1 Feb 2017 15:41
Operator : SJ/MA
Sample : PB96625BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB96625BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

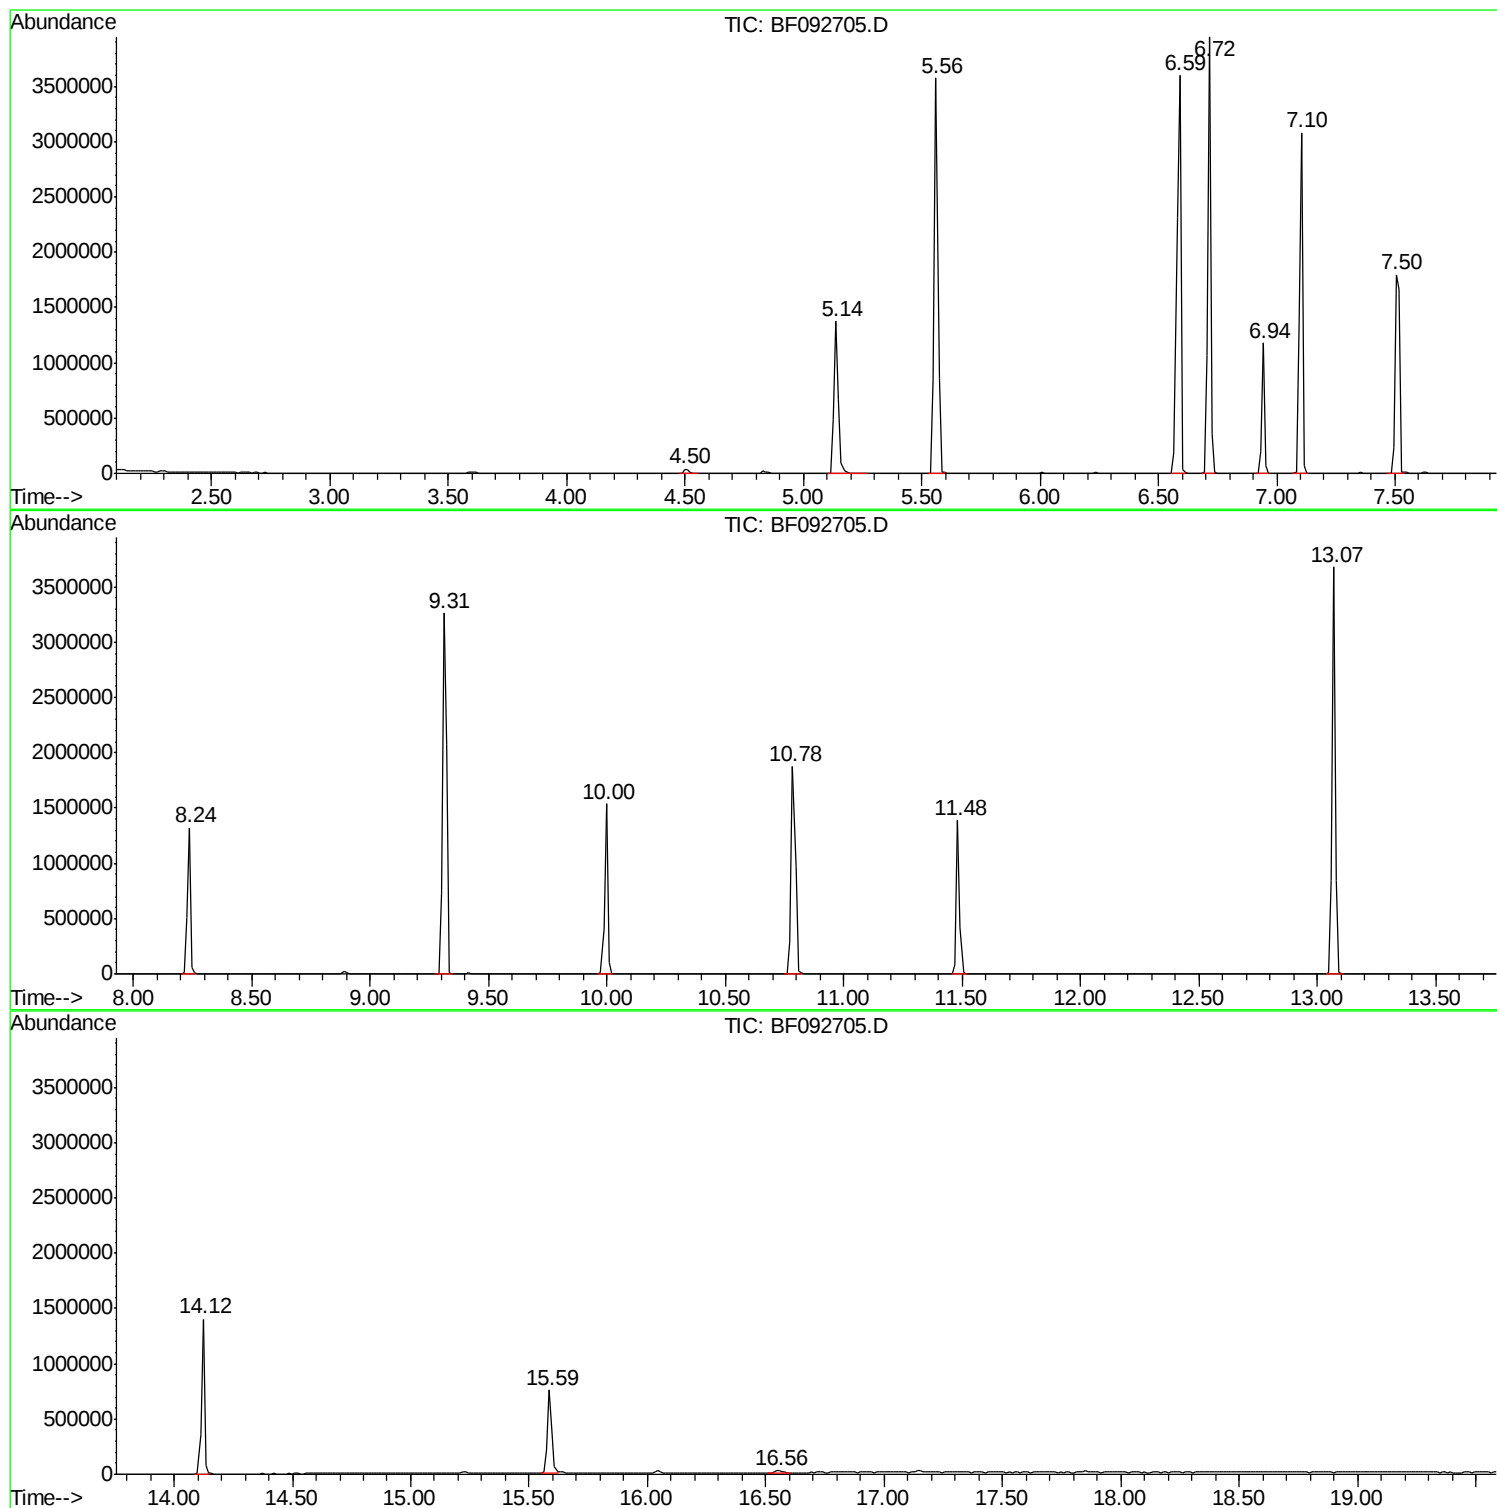

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020117\
Data File : BF092705.D
Acq On : 1 Feb 2017 15:41
Operator : SJ/MA
Sample : PB96625BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB96625BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.14	37.00 ng	1824550	1,4-Dichlorobenzene-d4	6.94

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
2		3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33
3		2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	33
4		Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	28
5		Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23

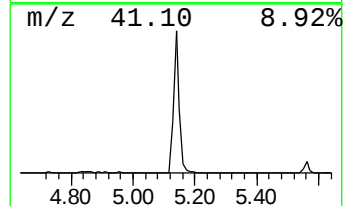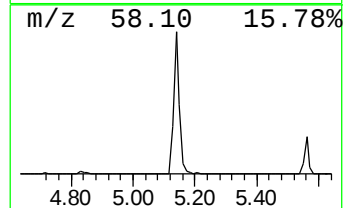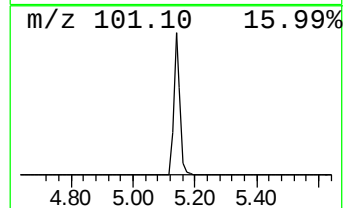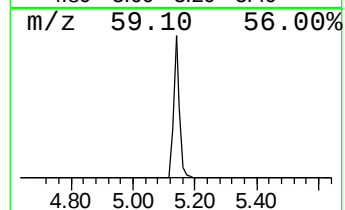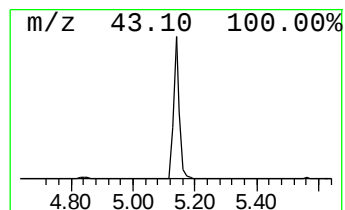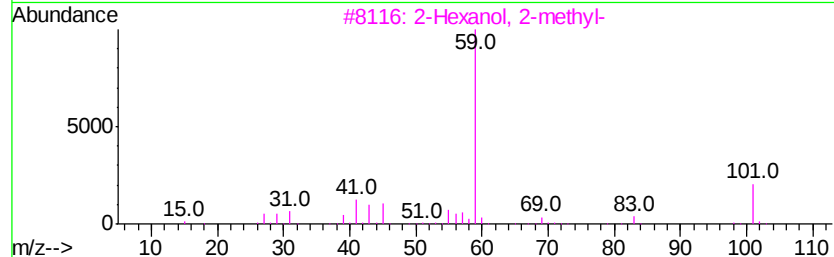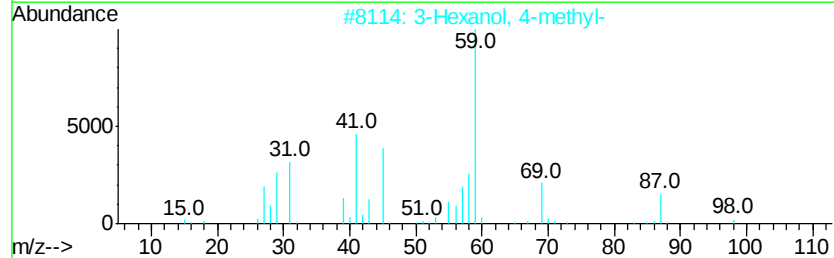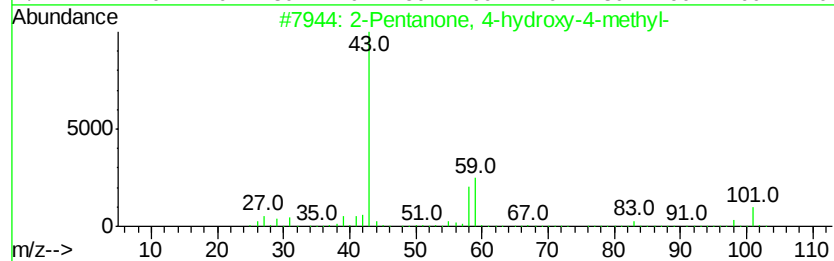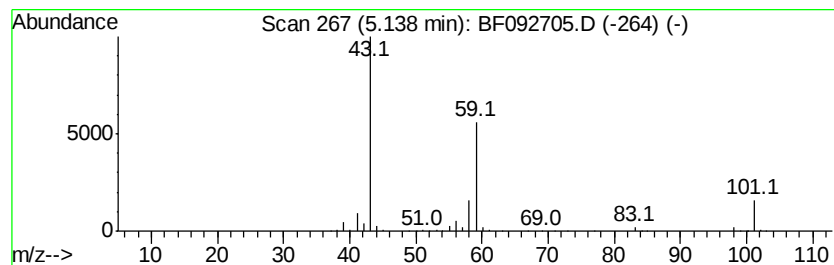

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020117\
Data File : BF092705.D
Acq On : 1 Feb 2017 15:41
Operator : SJ/MA
Sample : PB96625BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB96625BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.72 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.72	74.57 ng	3677510	1,4-Dichlorobenzene-d4	6.94

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

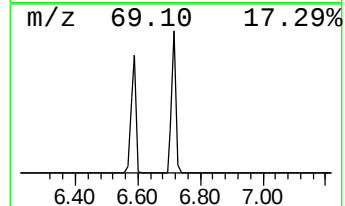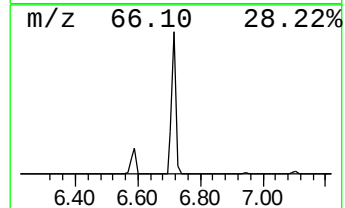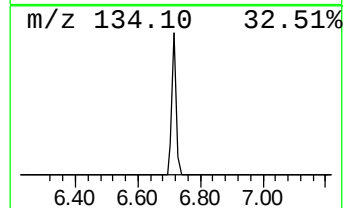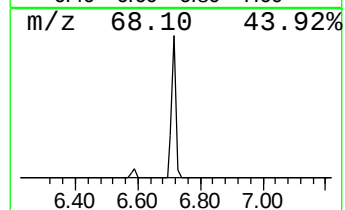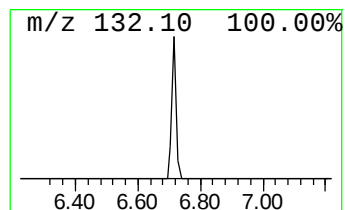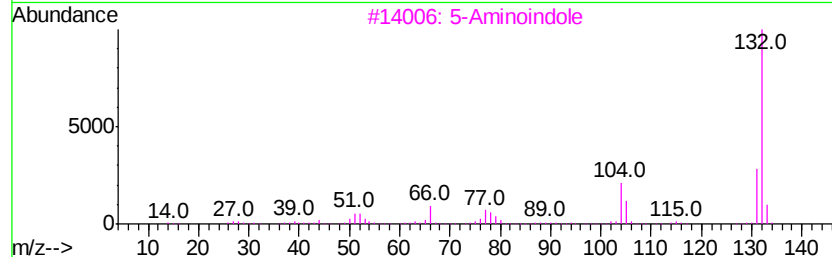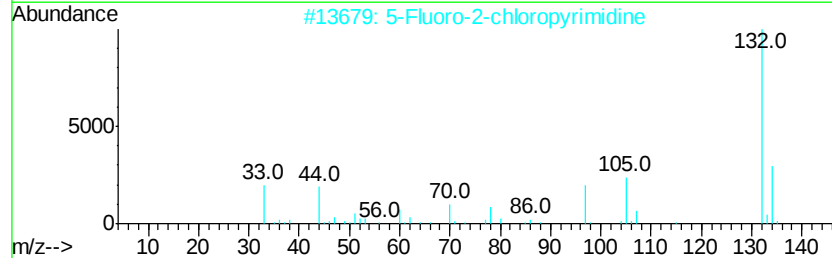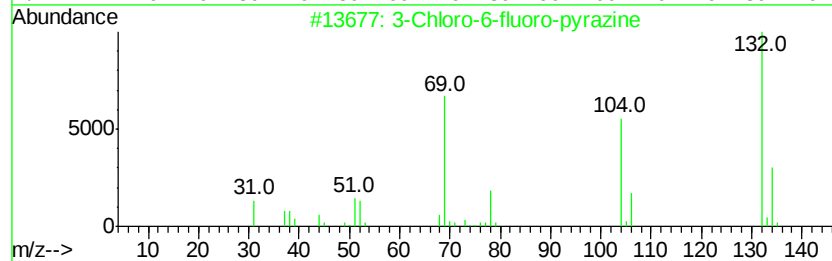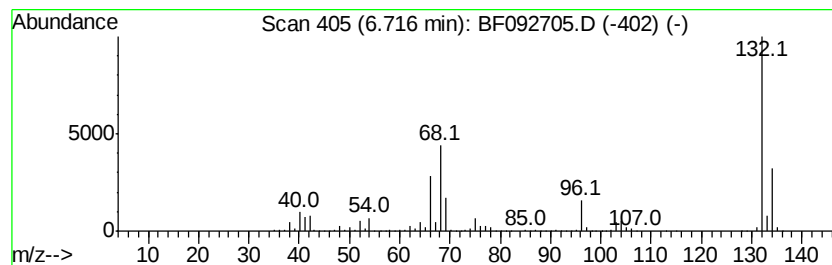

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020117\
Data File : BF092705.D
Acq On : 1 Feb 2017 15:41
Operator : SJ/MA
Sample : PB96625BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB96625BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.14	37.0	ng	1824550	1	6.94	986312	20.0
unknown6.72	6.72	74.6	ng	3677510	1	6.94	986312	20.0