


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020117\
 Data File : BF092701.D
 Acq On : 1 Feb 2017 13:36
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 30 14:50:05 2017

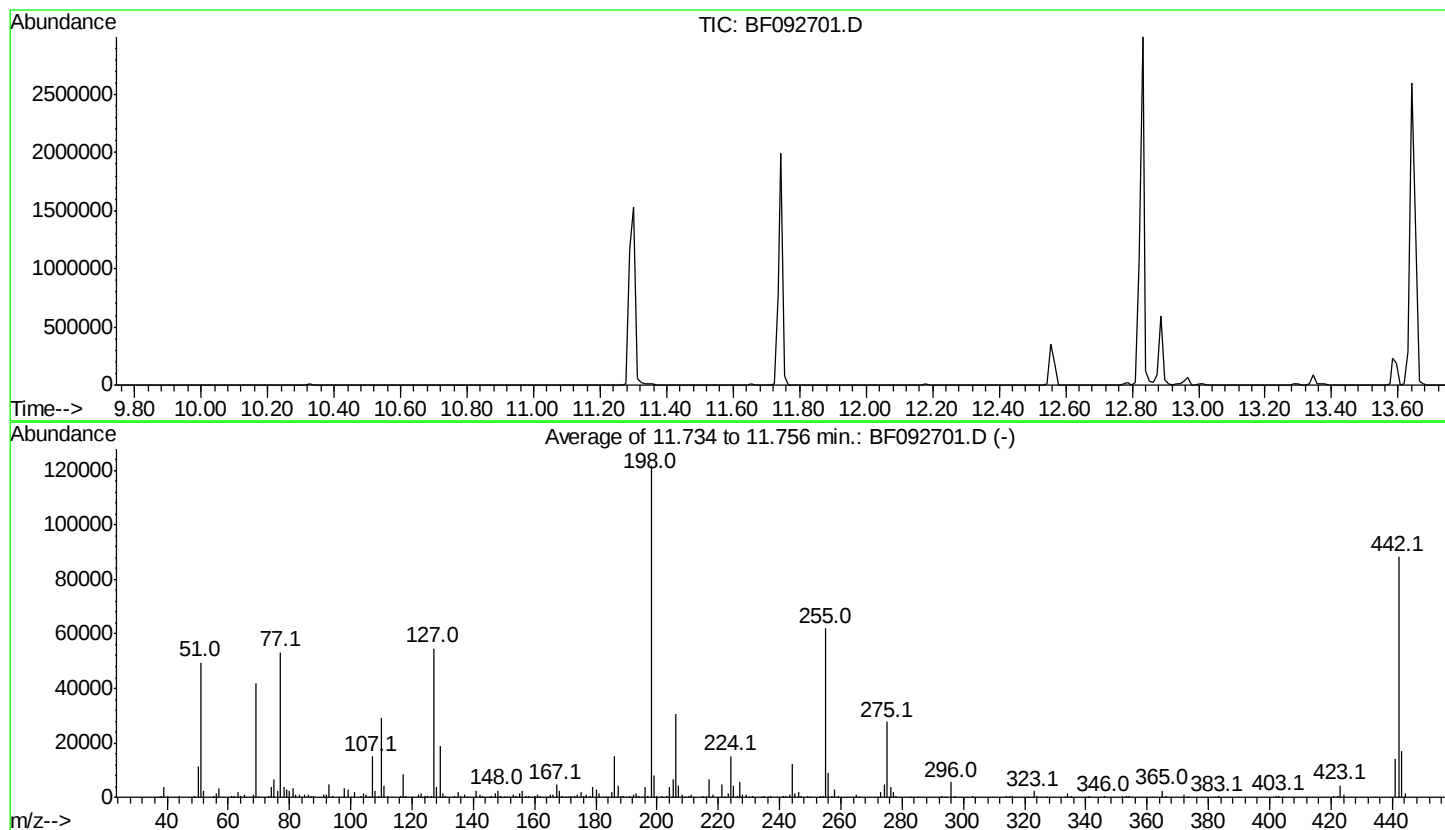

AutoFind: Scans 844, 845, 846; Background Corrected with Scan 840

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	49438	PASS
68	69	0.00	2	1.8	773	PASS
69	198	0.00	100	34.5	42005	PASS
70	69	0.00	2	0.5	227	PASS
127	198	10	80	44.9	54742	PASS
197	198	0.00	2	0.2	261	PASS
198	198	100	100	100.0	121868	PASS
199	198	5	9	6.5	7972	PASS
275	198	10	60	22.6	27592	PASS
365	198	1	100	2.0	2415	PASS
441	442	0.01	24	16.0	14117	PASS
442	198	50	100	72.5	88373	PASS
443	442	15	24	19.1	16900	PASS