


Data Path : Z:\HPCHEM1\BNA F\DATA\BF020117\
 Data File : BF092723.D
 Acq On : 2 Feb 2017 1:14
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 30 14:50:05 2017

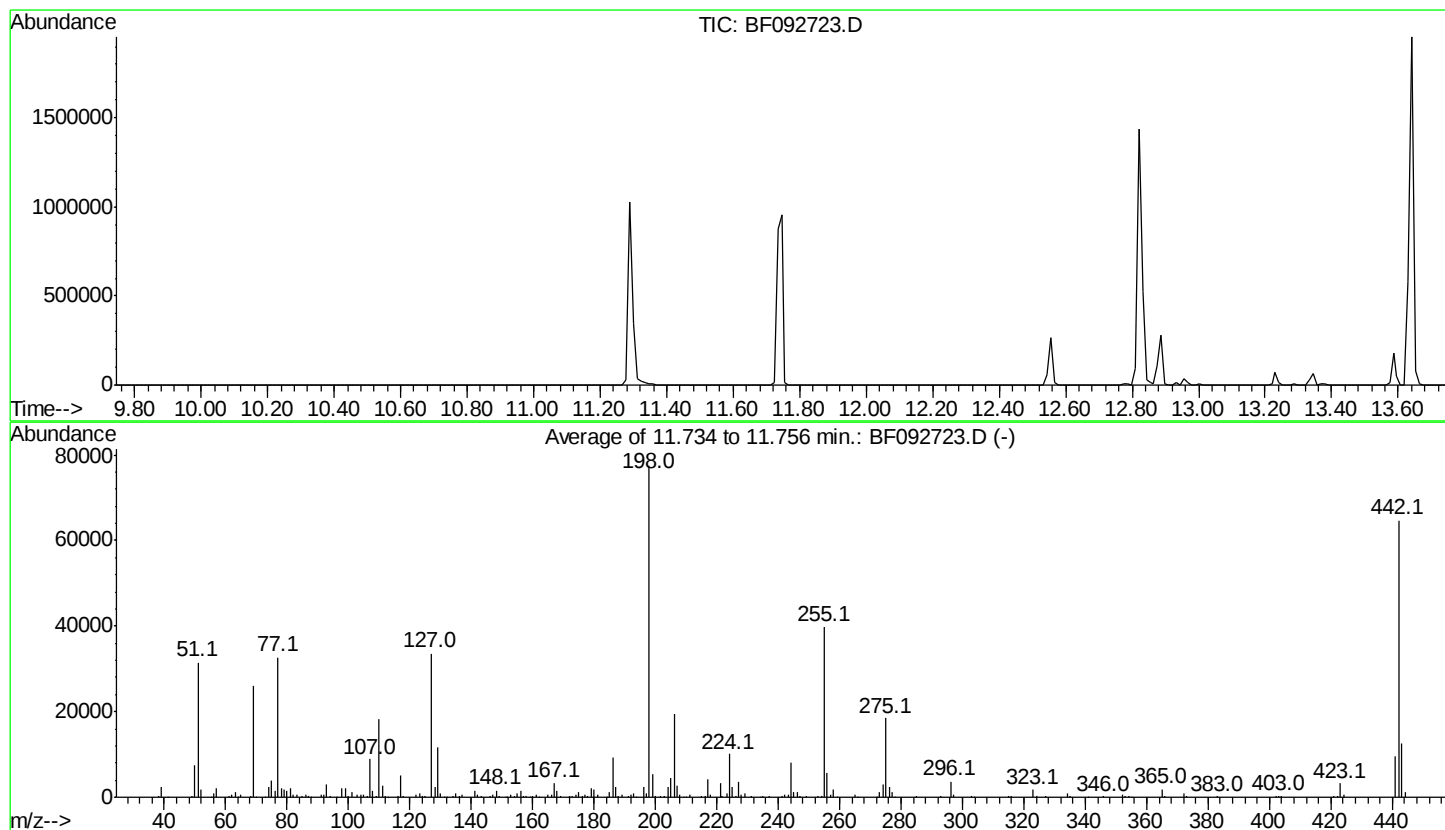

AutoFind: Scans 844, 845, 846; Background Corrected with Scan 840

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.5	31416	PASS
68	69	0.00	2	1.4	354	PASS
69	198	0.00	100	33.7	26117	PASS
70	69	0.00	2	0.4	104	PASS
127	198	10	80	43.4	33616	PASS
197	198	0.00	2	1.2	923	PASS
198	198	100	100	100.0	77508	PASS
199	198	5	9	6.8	5275	PASS
275	198	10	60	23.9	18531	PASS
365	198	1	100	2.5	1903	PASS
441	442	0.01	24	14.9	9661	PASS
442	198	50	100	83.5	64740	PASS
443	442	15	24	19.6	12701	PASS