


Data Path : Z:\HPCHEM1\BNA_F\Data\BF020118\
 Data File : BF102684.D
 Acq On : 1 Feb 2018 13:45
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 31 18:38:00 2018

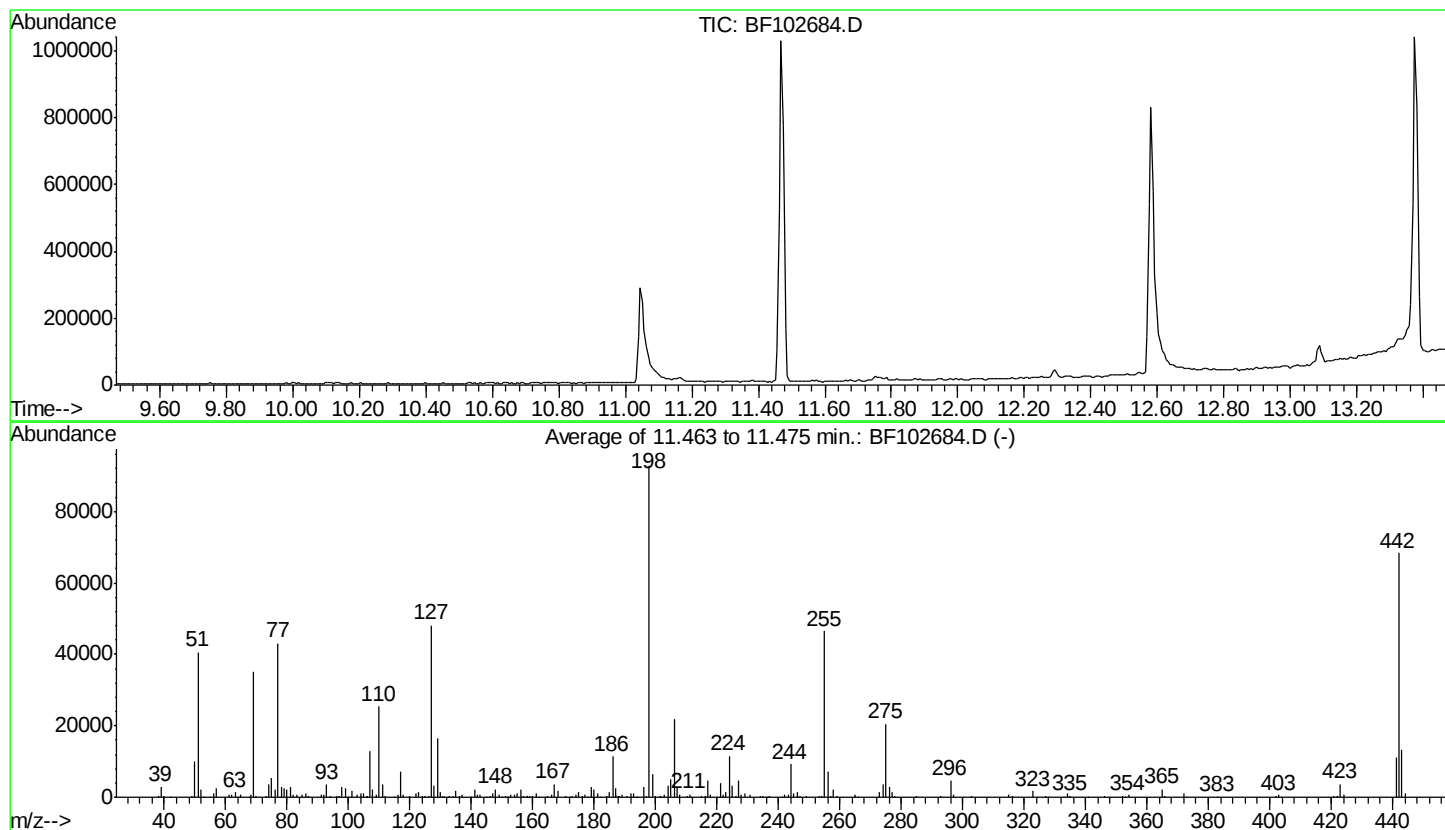

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.7	40581	PASS
68	69	0.00	2	1.6	580	PASS
69	198	0.00	100	38.0	35292	PASS
70	69	0.00	2	0.7	236	PASS
127	198	10	80	51.8	48101	PASS
197	198	0.00	2	0.3	238	PASS
198	198	100	100	100.0	92829	PASS
199	198	5	9	6.9	6380	PASS
275	198	10	60	22.1	20486	PASS
365	198	1	100	2.5	2290	PASS
441	443	0.01	100	85.1	11140	PASS
442	198	50	100	73.6	68304	PASS
443	442	15	24	19.2	13094	PASS