
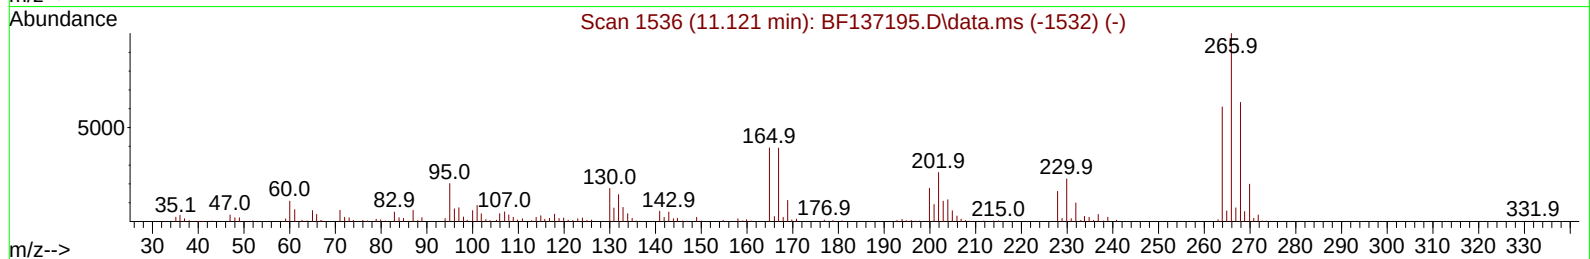
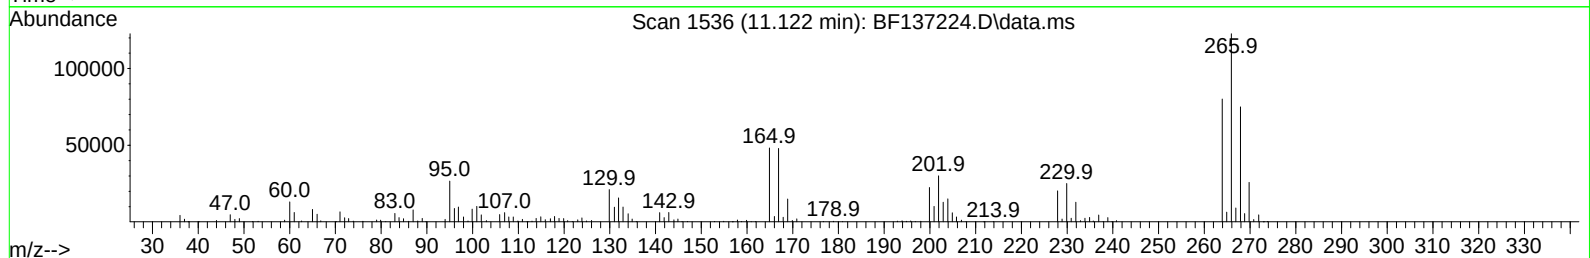


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF020124\  
Data File : BF137224.D  
Acq On : 01 Feb 2024 11:19  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 12:46:04 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF013024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jan 31 04:56:22 2024  
Response via : Initial Calibration

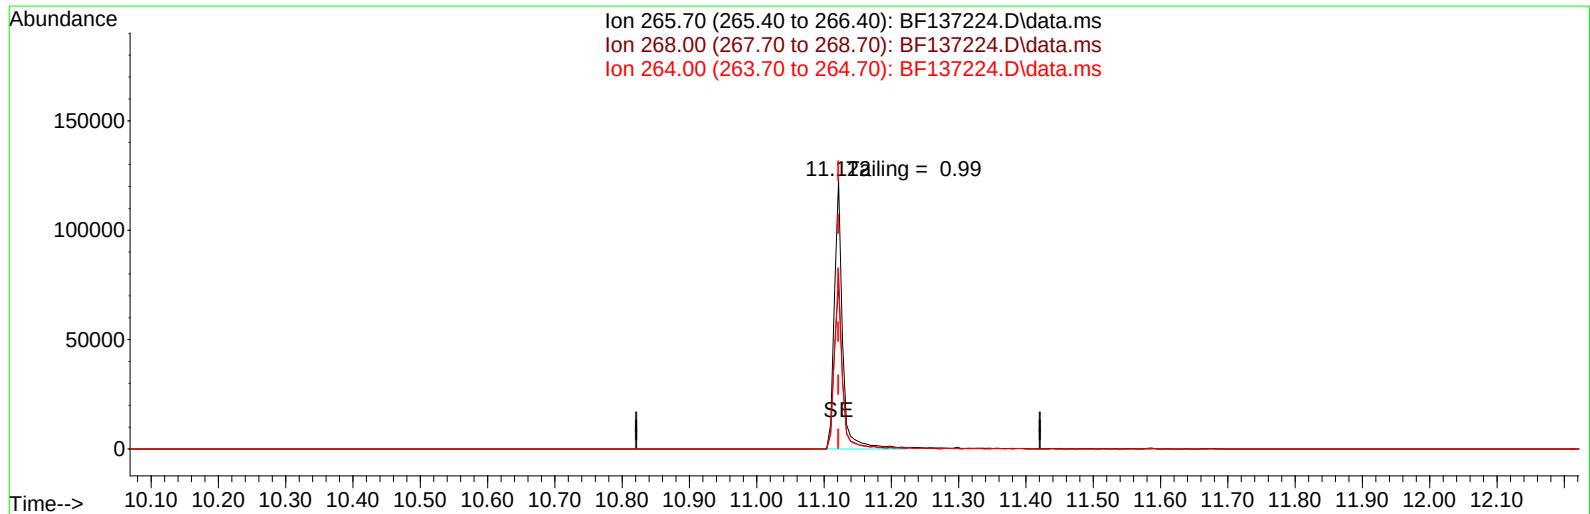

TIC: BF137224.D\data.ms

**(70) Pentachlorophenol (C)**




11.122min (+ 0.001) 30913.72 ng

response 104908

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.30  | 61.19  |
| 264.00 | 61.00  | 65.33  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF020124\  
Data File : BF137224.D  
Acq On : 01 Feb 2024 11:19  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 12:46:04 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF013024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jan 31 04:56:22 2024  
Response via : Initial Calibration

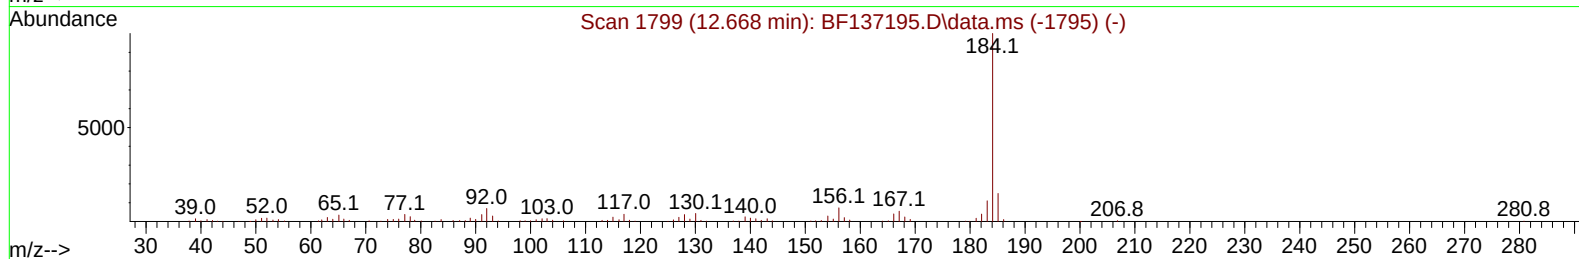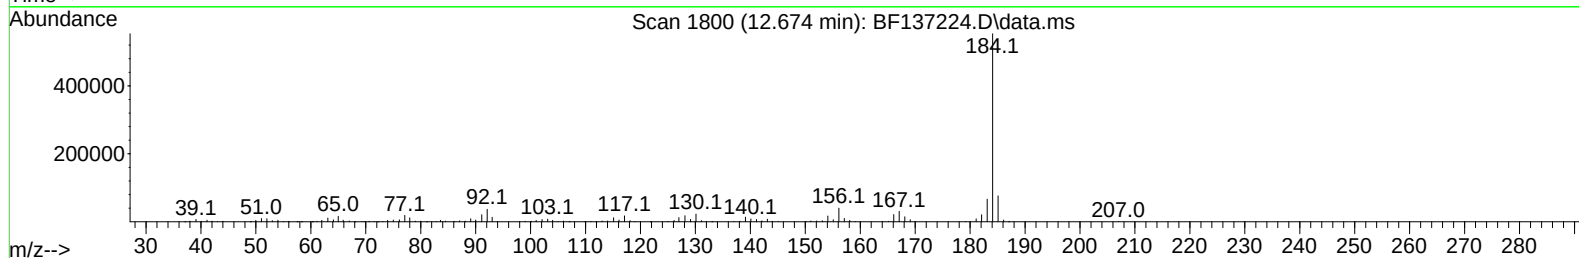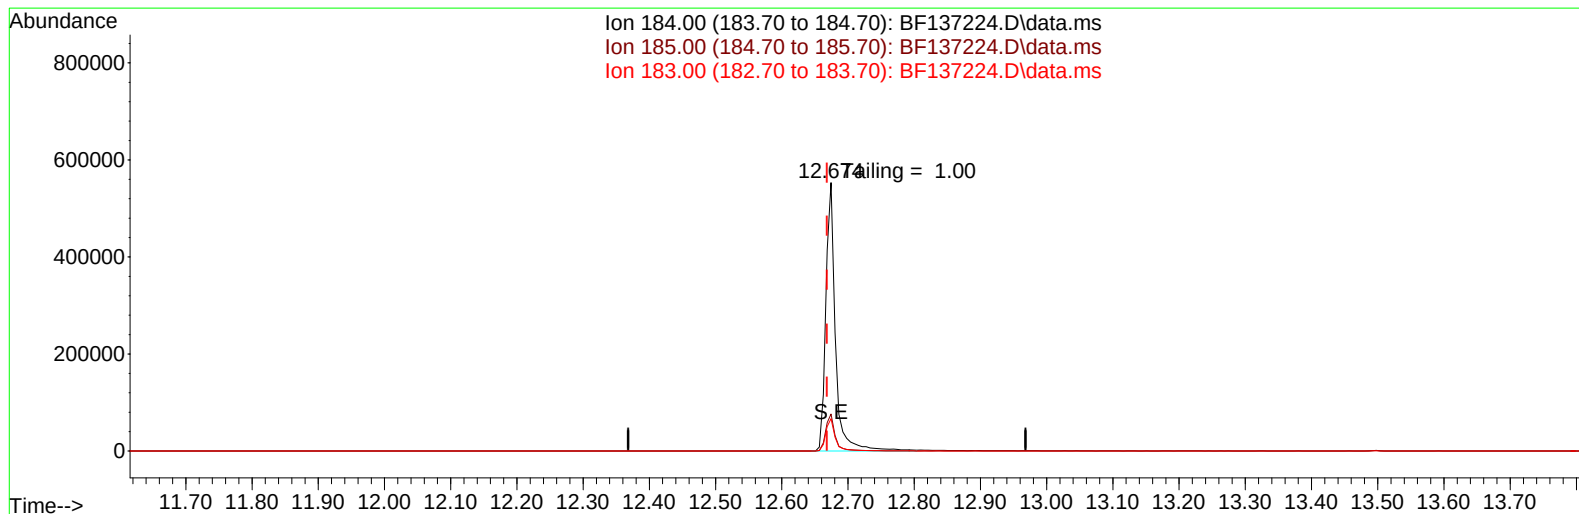

TIC: BF137224.D\data.ms

**(77) Benzidine**

12.674min (+ 0.006) 0.00 ng m

response 560770

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.90  | 13.81  |
| 183.00 | 11.00  | 12.05  |
| 0.00   | 0.00   | 0.00   |