


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020124\
Data File : BF137224.D
Acq On : 01 Feb 2024 11:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 31 04:56:22 2024

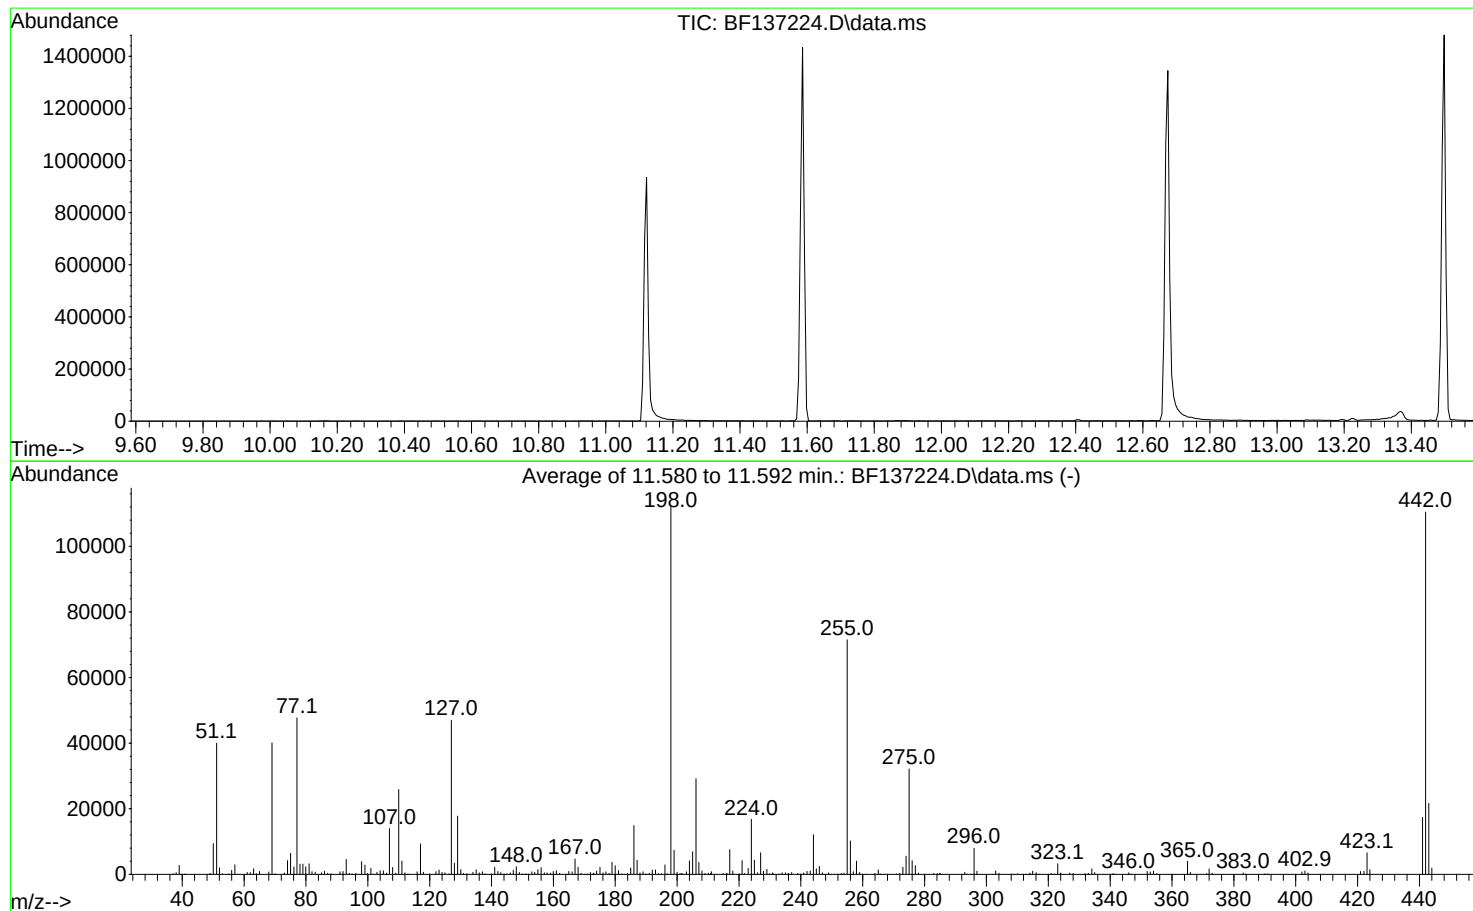




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	40020	PASS
68	69	0.00	2	1.8	718	PASS
69	198	0.00	100	35.8	40115	PASS
70	69	0.00	2	0.3	117	PASS
127	198	10	80	41.8	46925	PASS
197	198	0.00	2	0.2	201	PASS
198	198	100	100	100.0	112139	PASS
199	198	5	9	6.5	7337	PASS
275	198	10	60	28.7	32128	PASS
365	198	1	100	3.5	3933	PASS
441	198	0.01	100	15.5	17372	PASS
442	442	50	100	100.0	110419	PASS
443	442	15	24	19.6	21644	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020124\
Data File : BF137224.D
Acq On : 01 Feb 2024 11:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 01 12:46:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 04:56:22 2024
Response via : Initial Calibration

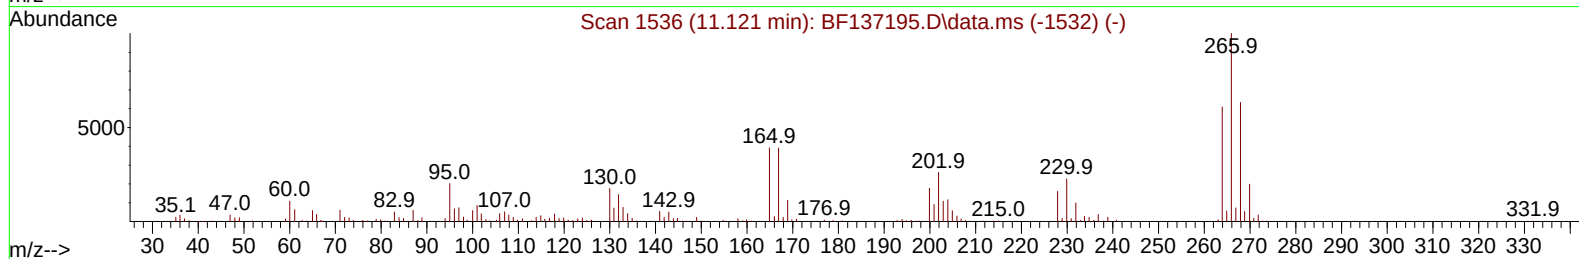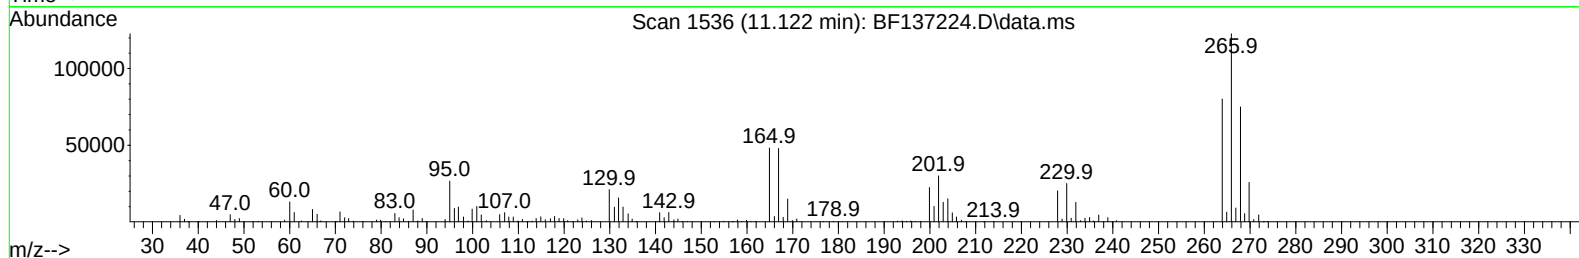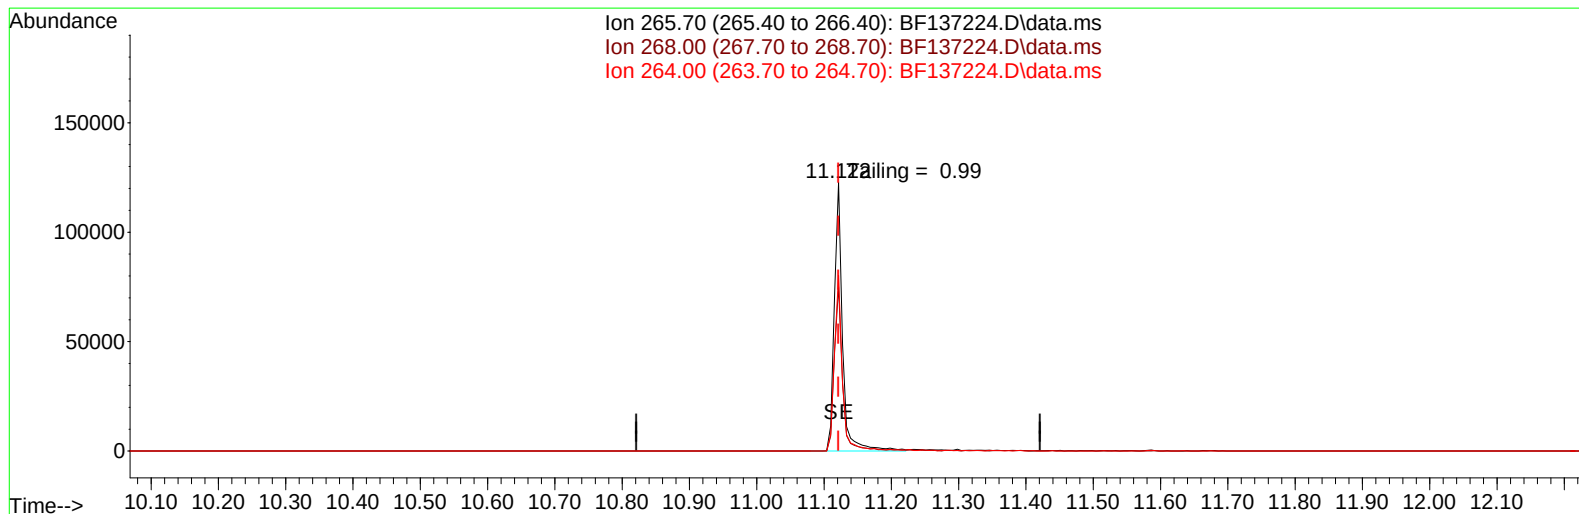

TIC: BF137224.D\data.ms

(70) Pentachlorophenol (C)

11.122min (+ 0.001) 30913.72 ng




response 104908

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	61.19
264.00	61.00	65.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020124\
Data File : BF137224.D
Acq On : 01 Feb 2024 11:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 01 12:46:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 04:56:22 2024
Response via : Initial Calibration

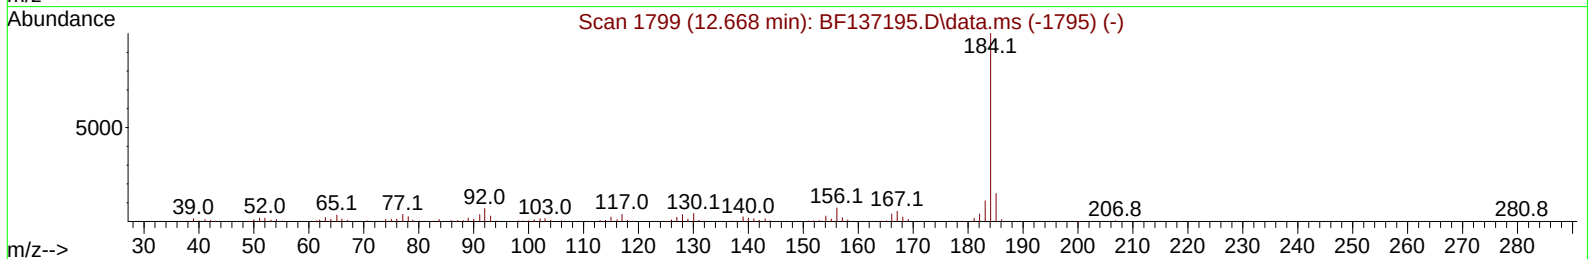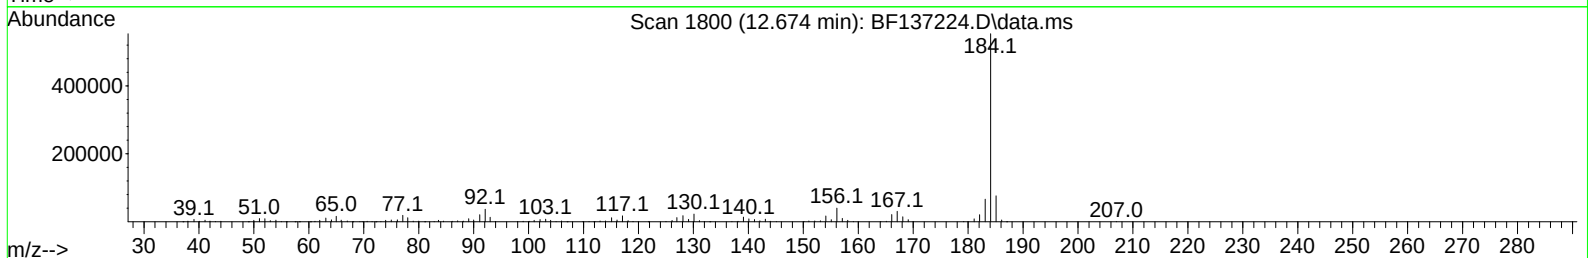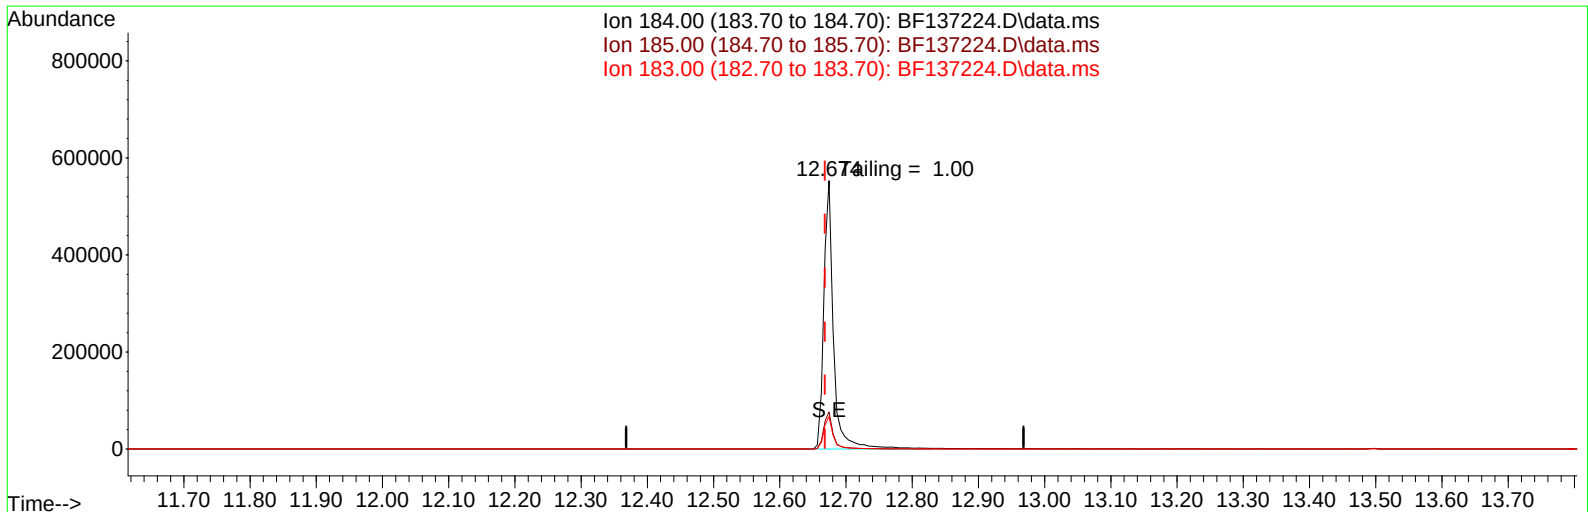

TIC: BF137224.D\data.ms

(77) Benzidine

12.674min (+ 0.006) 0.00 ng m

response 560770

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.81
183.00	11.00	12.05
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/1/2024	BNA_F	<u>BF137224.D</u>
Compound Name	Response	Retention Time
DDT	246113	13.498
DDD	3408	13.227
DDE	142	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3550	249663	1.42

Instrument :
BNA_F
ClientSampleId :
DFTPP