

Data Path : Z:\HPCHEM1\BNA F\Data\BF020216\
 Data File : BF084779.D
 Acq On : 3 Feb 2016 8:03
 Operator : SJ/IZ
 Sample : H1313-05
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HSR-WC-24-012916

Quant Time: Feb 03 09:46:26 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 01 14:55:11 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.69	152	180617	20.00	ng	-0.03
21) Naphthalene-d8	7.98	136	798410	20.00	ng	-0.03
38) Acenaphthene-d10	9.73	164	374784	20.00	ng	-0.03
63) Phenanthrene-d10	11.21	188	693379	20.00	ng	-0.03
75) Chrysene-d12	13.85	240	493439	20.00	ng	-0.02
86) Perylene-d12	15.22	264	364033	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.31	112	1451580	125.18	ng	0.00
7) Phenol-d6	6.35	99	1428943	99.40	ng	-0.02
23) Nitrobenzene-d5	7.26	82	1135634	80.13	ng	-0.03
41) 2,4,6-Tribromophenol	10.52	330	530501	135.70	ng	-0.03
44) 2-Fluorobiphenyl	9.07	172	2209265	110.17	ng	-0.02
78) Terphenyl-d14	12.81	244	2118160	97.27	ng	-0.02
Target Compounds						
9) Benzaldehyde	6.48	77	36684	4.32	ng	Qvalue 85
19) n-Nitroso-di-n-propylamine	7.26	70	154926	17.19	ng	# 72
25) Isophorone	7.26	82	951048	34.51	ng	# 66
31) Naphthalene	8.01	128	146455	3.66	ng	97
50) 2,6-Dinitrotoluene	9.73	165	49029	7.86	ng	# 37
56) 2,4-Dinitrotoluene	9.73	165	49029	6.16	ng	# 21
66) 4-Bromophenyl-phenylether	10.52	248	31862	4.16	ng	# 1
76) Benzidine	12.56	184	53929	8.96	ng	# 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\Data\BF020216\
Data File : BF084779.D
Acq On : 3 Feb 2016 8:03
Operator : SJ/IZ
Sample : H1313-05
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HSR-WC-24-012916

Quant Time: Feb 03 09:46:26 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 01 14:55:11 2016
Response via : Initial Calibration

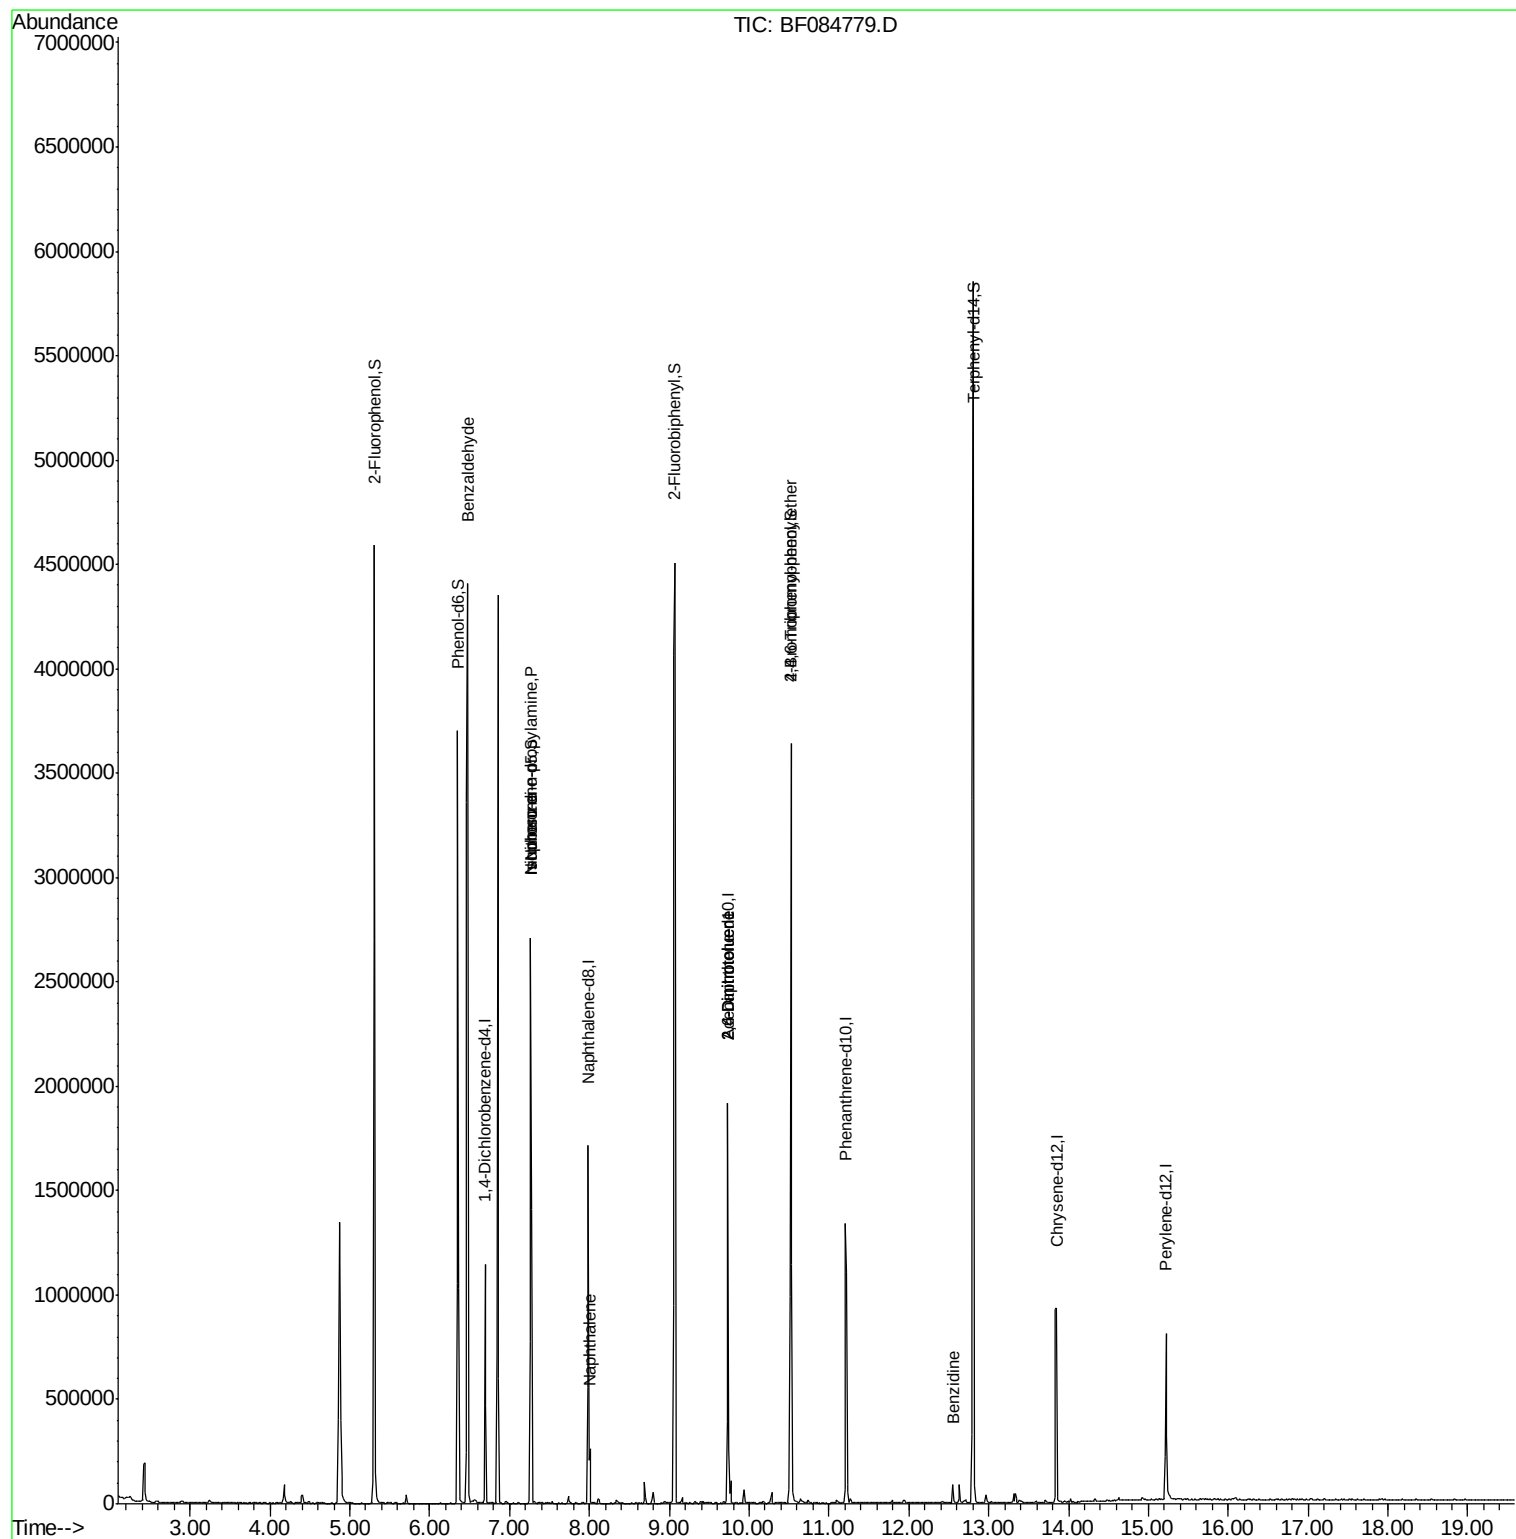

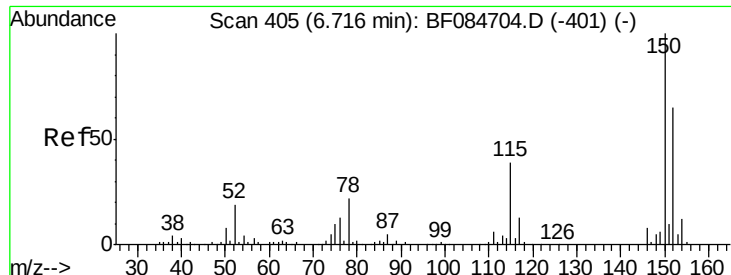

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.69 min Scan# 403

Delta R.T. -0.03 min

Lab File: BF084779.D

Acq: 3 Feb 2016 8:03

Instrument :

BNA_F

ClientSampleId :

HSR-WC-24-012916


Tot Ion:152 Resp: 180617

Ion Ratio Lower Upper

152 100

150 160.9 123.0 184.4




115 74.1 51.4 77.2

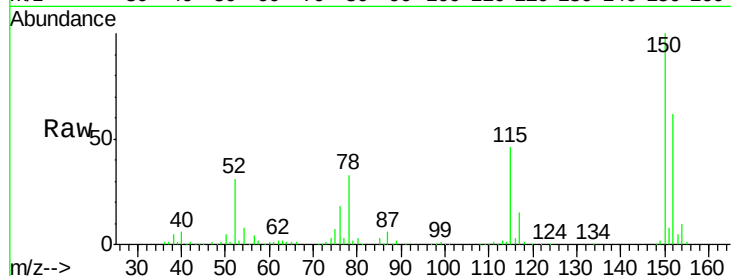

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

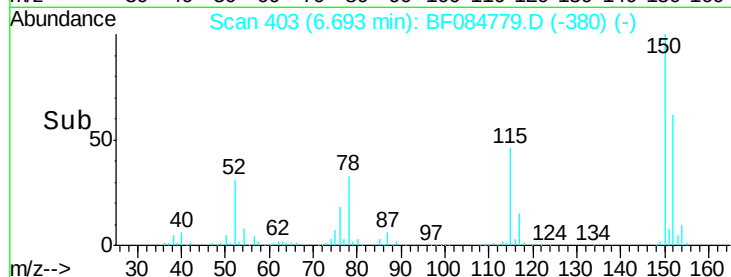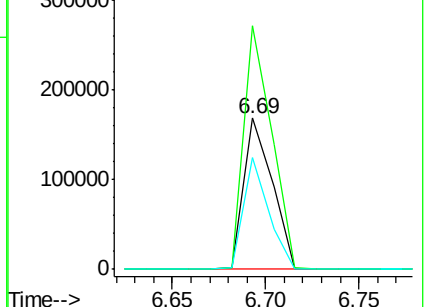

#5

2-Fluorophenol

Concen: 125.18 ng

RT: 5.31 min Scan# 282

Delta R.T. 0.00 min

Lab File: BF084779.D

Acq: 3 Feb 2016 8:03


Tgt Ion:112 Resp: 1451580

Ion Ratio Lower Upper

112 100

64 58.5 36.6 55.0#



63 30.8 19.4 29.0#




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

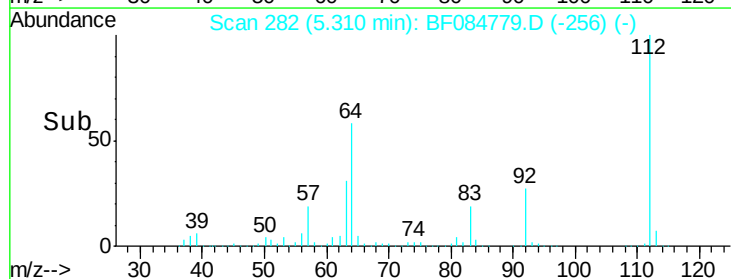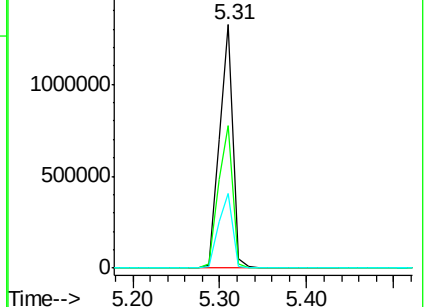

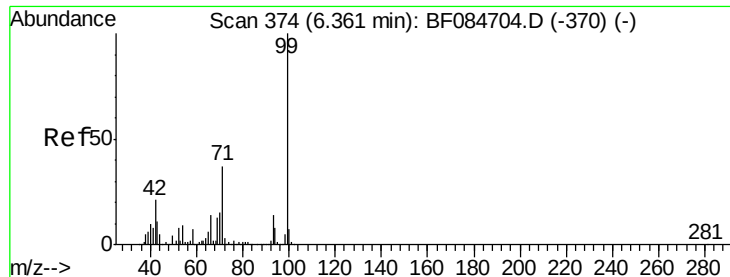

#7

Phenol-d6

Concen: 99.40 ng

RT: 6.35 min Scan# 373

Delta R.T. -0.02 min

Lab File: BF084779.D

Acq: 3 Feb 2016 8:03

Instrument :





BNA_F

ClientSampleId :

HSR-WC-24-012916

Tot Ion: 99 Resp: 1428943

Ion	Ratio	Lower	Upper
99	100		
42	20.9	12.8	19.2#
71	37.7	30.9	46.3

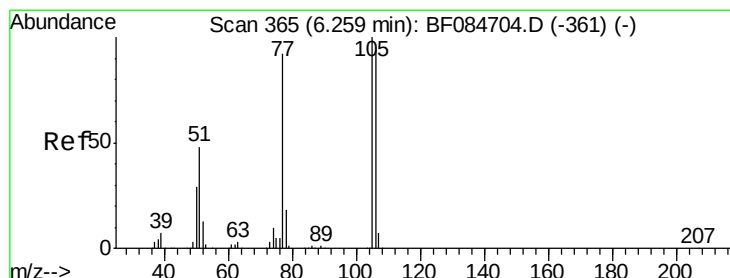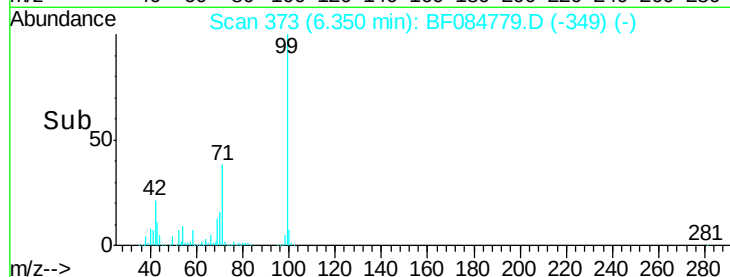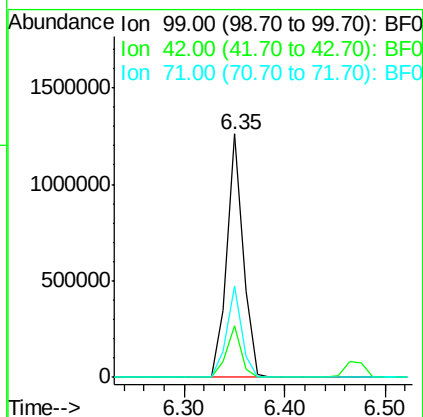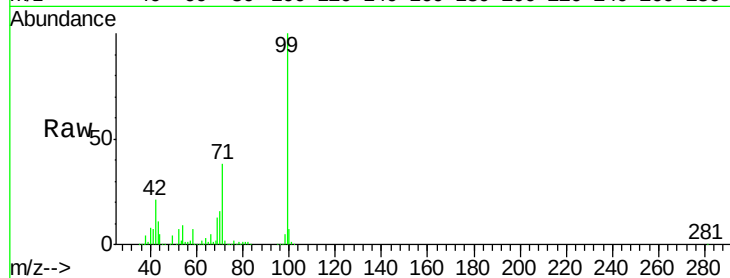

#9

Benzaldehyde

Concen: 4.32 ng

RT: 6.48 min Scan# 384




Delta R.T. 0.21 min




Lab File: BF084779.D

Acq: 3 Feb 2016 8:03

Tgt Ion: 77 Resp: 36684

Ion	Ratio	Lower	Upper
77	100		
105	88.1	83.0	123.0
106	79.0	74.6	114.6


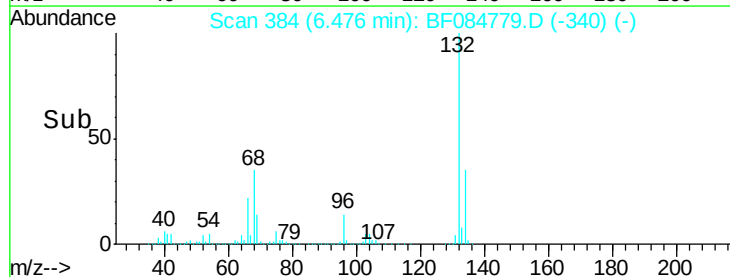
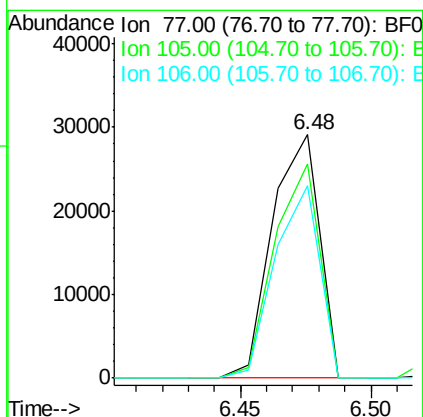
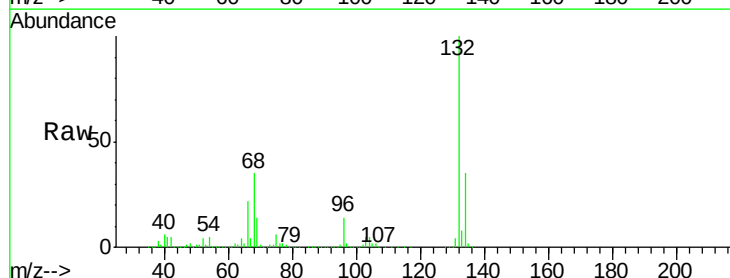


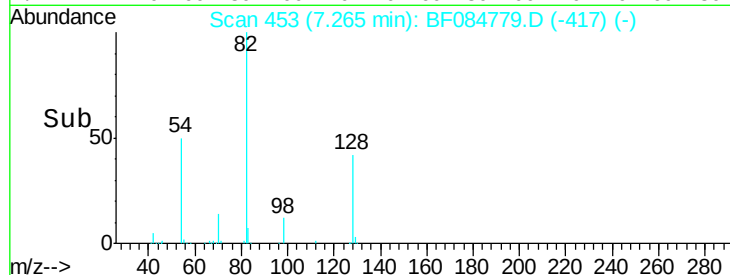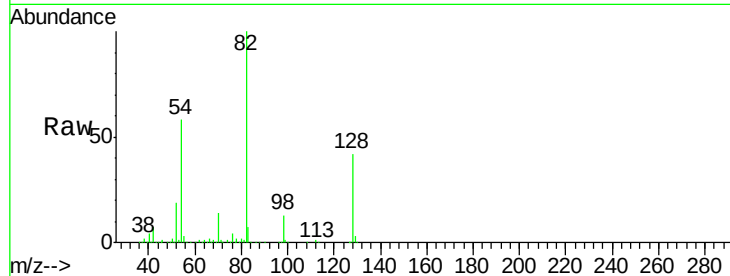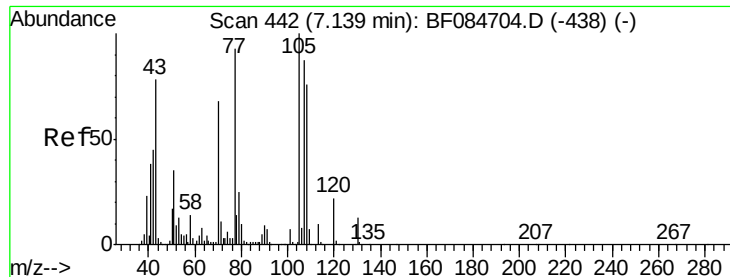

#19
n-Nitroso-di-n-propylamine
Concen: 17.19 ng
RT: 7.26 min Scan# 453
Delta R.T. 0.11 min
Lab File: BF084779.D
Acq: 3 Feb 2016 8:03


Instrument :
BNA_F
ClientSampleId :
HSR-WC-24-012916


Tot Ion:	70	Resp:	154926
Ion	Ratio	Lower	Upper
70	100		
42	49.4	33.3	49.9
101	0.0	9.3	13.9#
130	2.0	23.4	35.0#

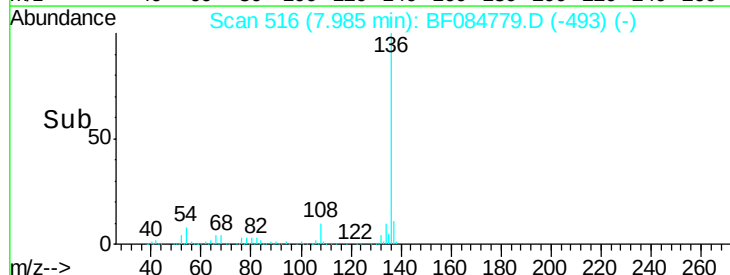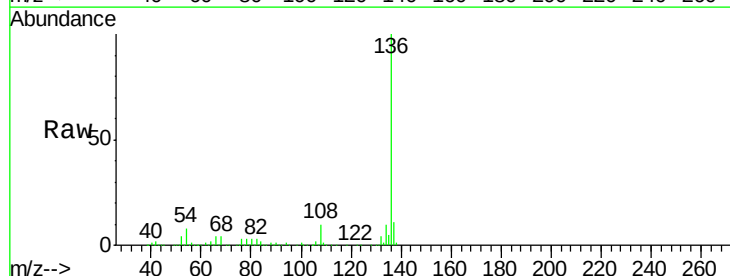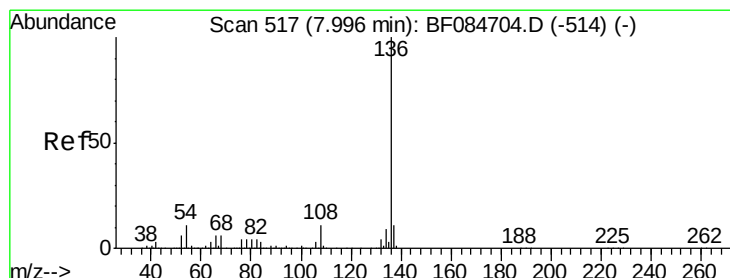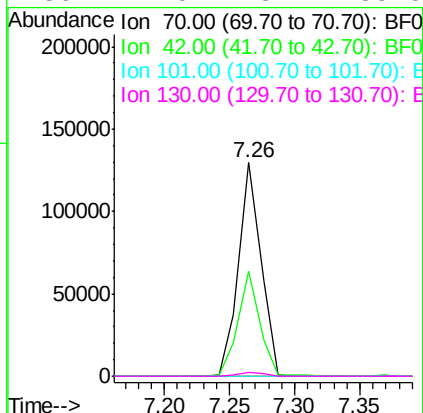

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.98 min Scan# 516
Delta R.T. -0.03 min
Lab File: BF084779.D
Acq: 3 Feb 2016 8:03

Tgt Ion:	136	Resp:	798410
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.7	13.1
54	7.6	5.8	8.8
68	4.3	4.2	6.2




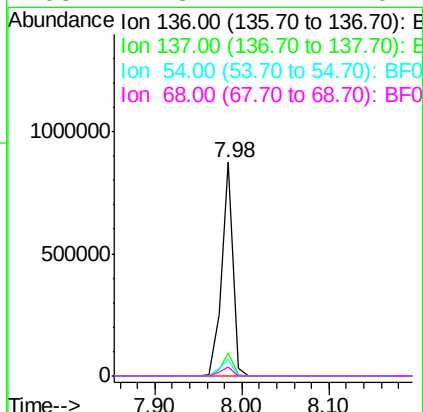


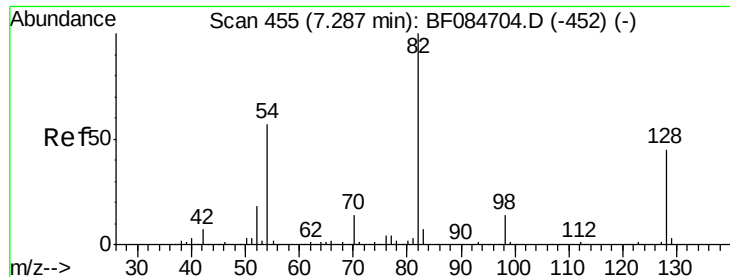

#23
 Nitrobenzene-d5
 Concen: 80.13 ng
 RT: 7.26 min Scan# 453
 Delta R.T. -0.03 min
 Lab File: BF084779.D
 Acq: 3 Feb 2016 8:03




Instrument :
 BNA_F
 ClientSampleId :
 HSR-WC-24-012916


Tot Ion: 82 Resp: 1135634
 Ion Ratio Lower Upper
 82 100
 128 41.8 34.6 51.8
 54 57.9 38.4 57.6#

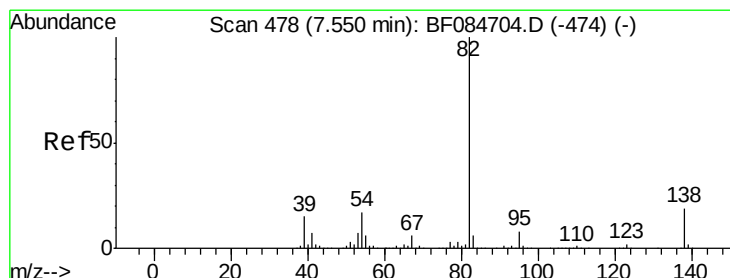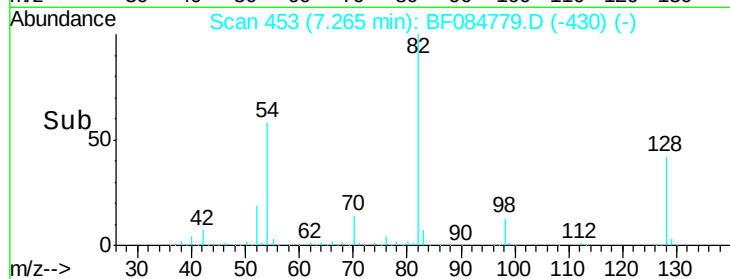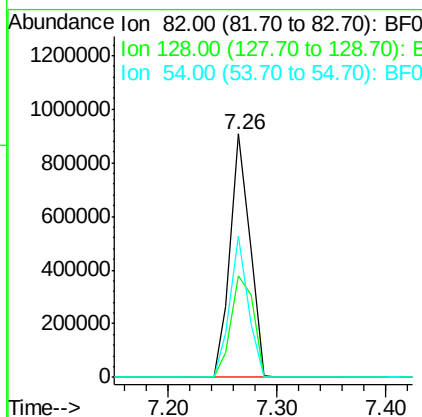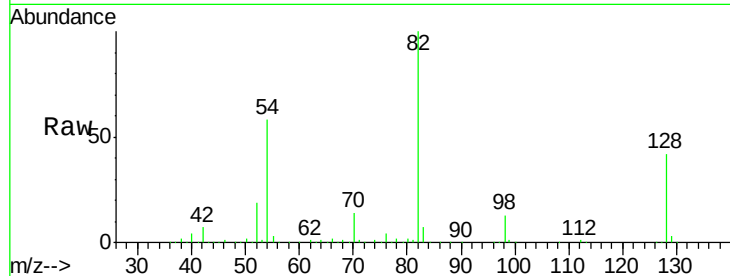

#25
 Isophorone
 Concen: 34.51 ng
 RT: 7.26 min Scan# 453
 Delta R.T. -0.30 min
 Lab File: BF084779.D
 Acq: 3 Feb 2016 8:03

Tgt Ion: 82 Resp: 951048
 Ion Ratio Lower Upper
 82 100
 95 0.0 6.6 10.0#
 138 0.0 13.6 20.4#

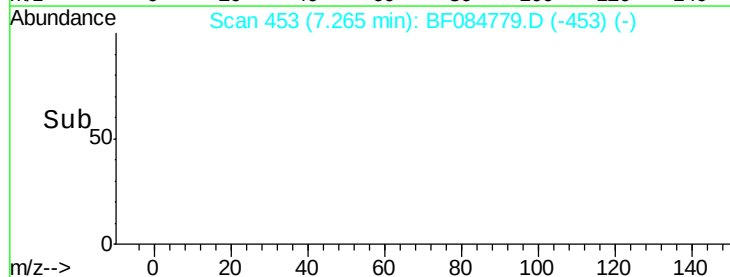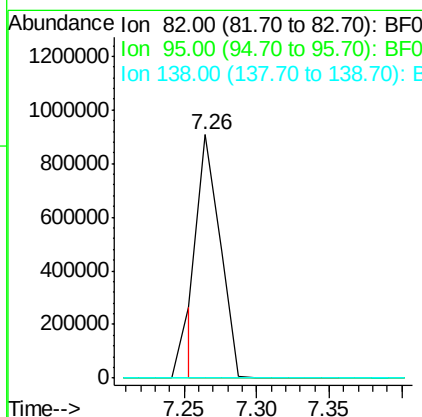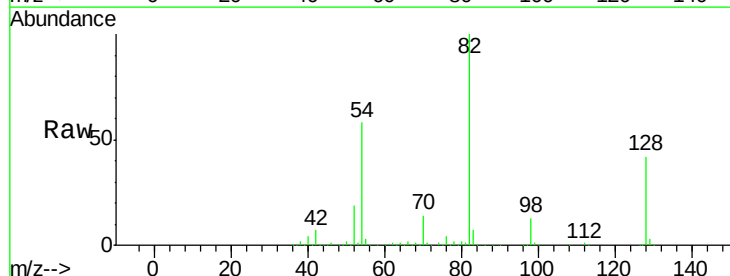

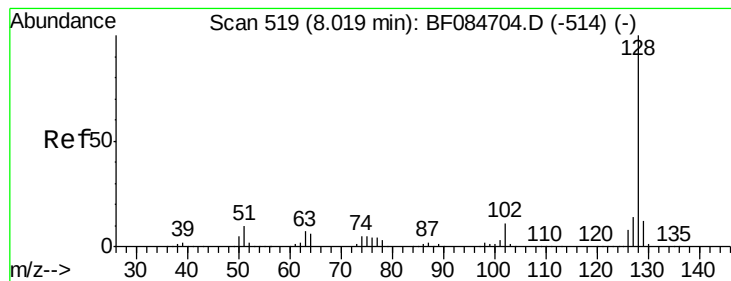

#31

Naphthalene

Concen: 3.66 ng

RT: 8.01 min Scan# 518

Delta R.T. -0.02 min

Lab File: BF084779.D

Acq: 3 Feb 2016 8:03

Instrument :

BNA_F

ClientSampleId :

HSR-WC-24-012916


Tot Ion:128 Resp: 146455

Ion Ratio Lower Upper

128 100

129 10.3 9.1 13.7




127 13.0 11.1 16.7



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

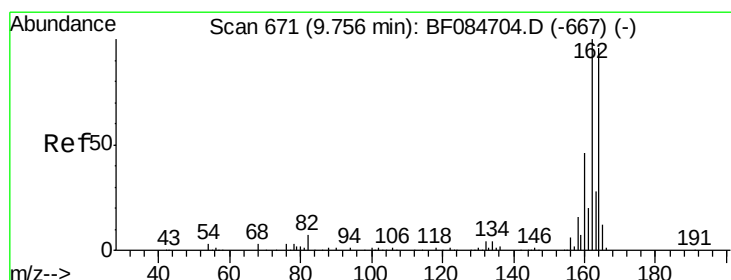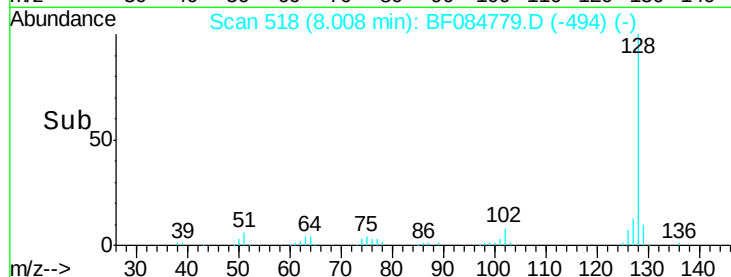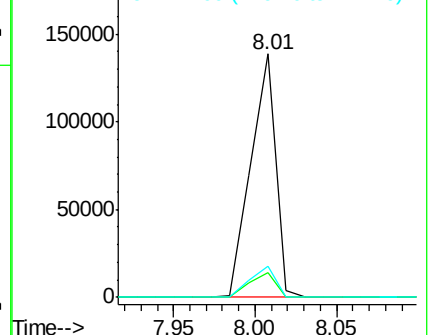

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.73 min Scan# 669

Delta R.T. -0.03 min

Lab File: BF084779.D

Acq: 3 Feb 2016 8:03


Tgt Ion:164 Resp: 374784

Ion Ratio Lower Upper

164 100

162 104.4 85.1 127.7



160 47.8 37.5 56.3




Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E



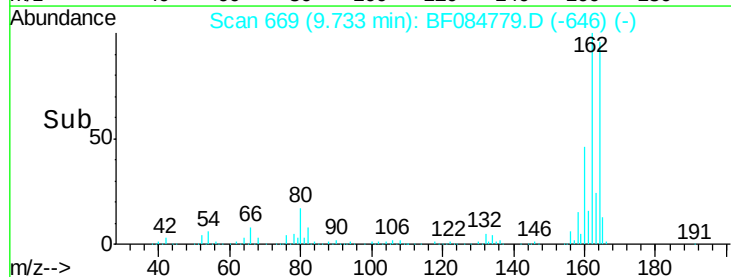
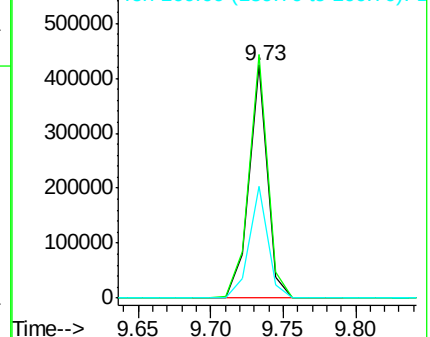


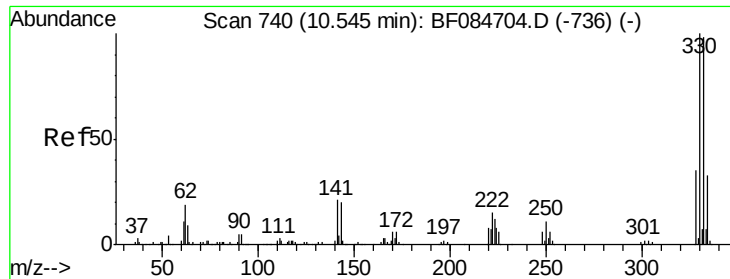

#41
 2,4,6-Tribromophenol
 Concen: 135.70 ng
 RT: 10.52 min Scan# 738
 Delta R.T. -0.03 min
 Lab File: BF084779.D
 Acq: 3 Feb 2016 8:03




Instrument :
 BNA_F
 ClientSampleId :
 HSR-WC-24-012916


Tot Ion	Ratio	Lower	Upper
330	100		
332	96.1	76.6	114.8
141	33.3	27.8	41.6

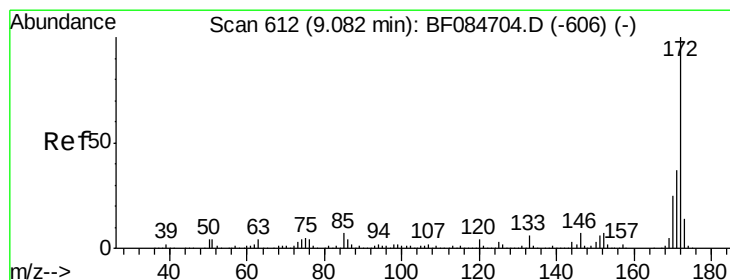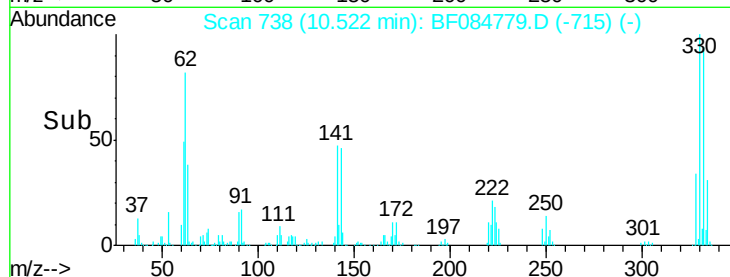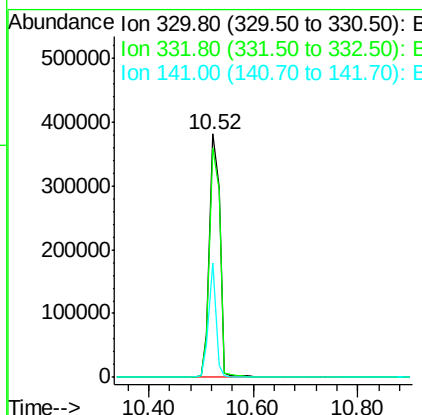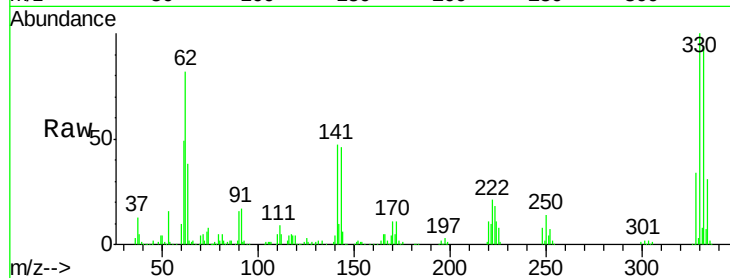

#44
 2-Fluorobiphenyl
 Concen: 110.17 ng
 RT: 9.07 min Scan# 611
 Delta R.T. -0.02 min
 Lab File: BF084779.D
 Acq: 3 Feb 2016 8:03

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.1	28.9	43.3
170	25.0	18.6	27.8

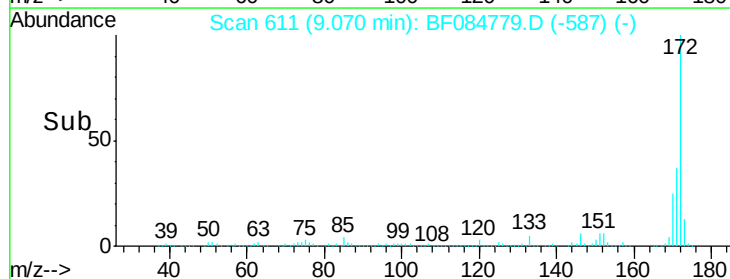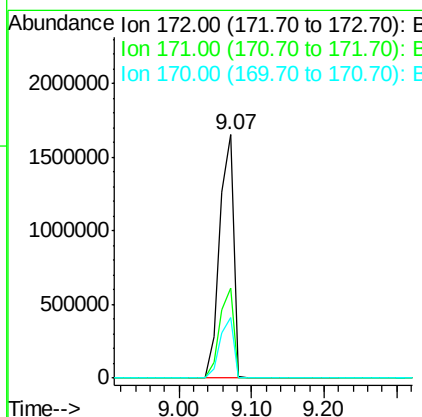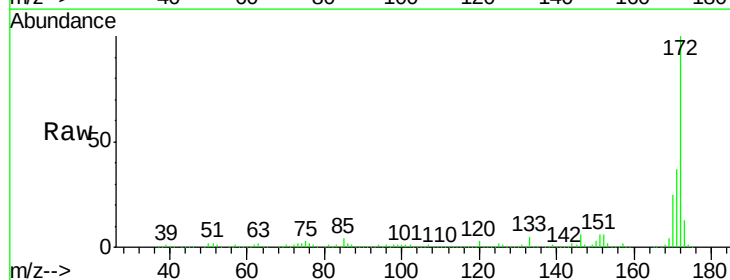


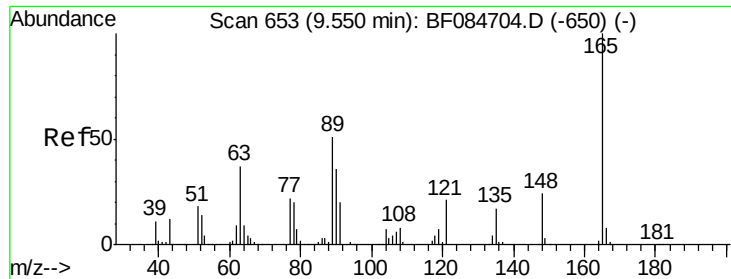

#50
 2,6-Dinitrotoluene
 Concen: 7.86 ng
 RT: 9.73 min Scan# 669
 Delta R.T. 0.17 min
 Lab File: BF084779.D
 Acq: 3 Feb 2016 8:03

Instrument :
 BNA_F
 ClientSampleId :
 HSR-WC-24-012916




Tot Ion	Ratio	Lower	Upper
165	100		
63	1.3	28.8	43.2#
89	1.3	35.1	52.7#

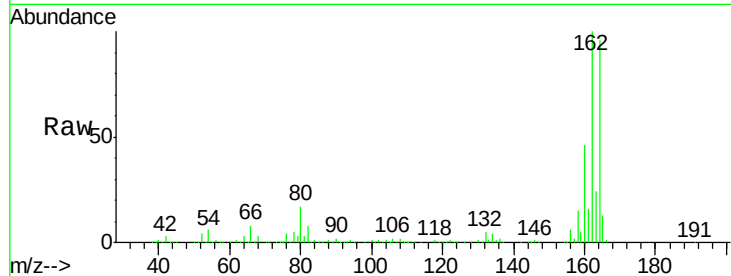

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

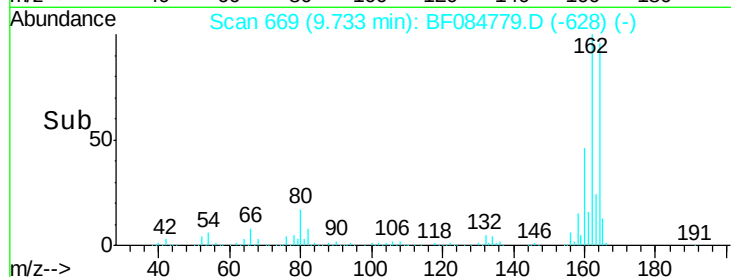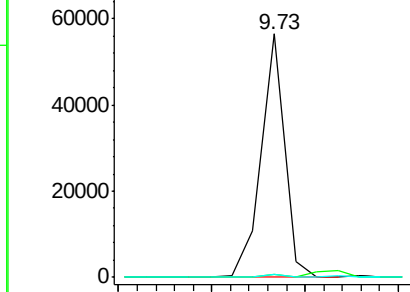

#56
 2,4-Dinitrotoluene
 Concen: 6.16 ng
 RT: 9.73 min Scan# 669
 Delta R.T. -0.23 min
 Lab File: BF084779.D
 Acq: 3 Feb 2016 8:03




Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.3	36.7	55.1#
89	1.3	61.9	92.9#
182	0.0	2.0	3.0#


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E

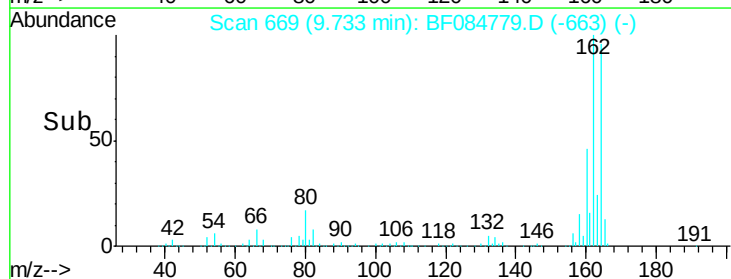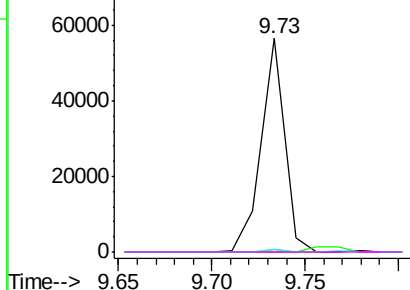

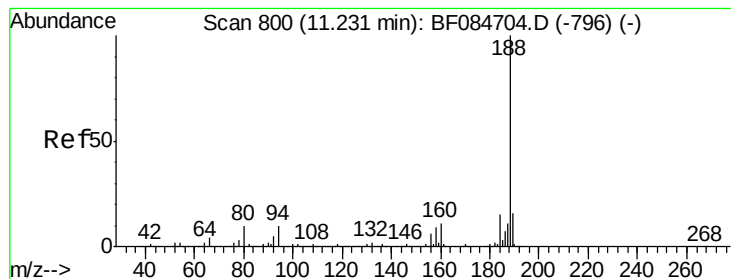

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.21 min Scan# 798

Delta R.T. -0.03 min

Lab File: BF084779.D

Acq: 3 Feb 2016 8:03

Instrument :

BNA_F

ClientSampleId :

HSR-WC-24-012916


Tot Ion:188 Resp: 693379

Ion Ratio Lower Upper

188 100

94 12.4 9.0 13.4




80 13.2 9.6 14.4



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

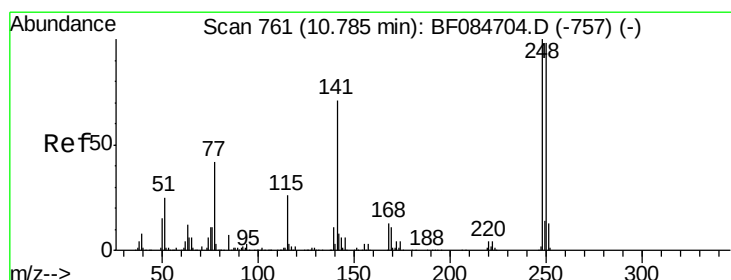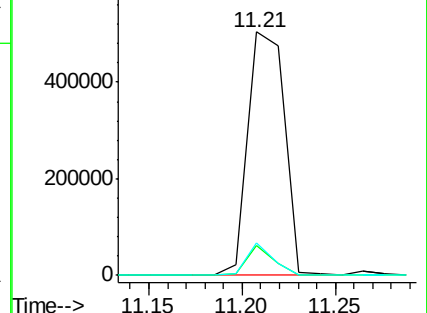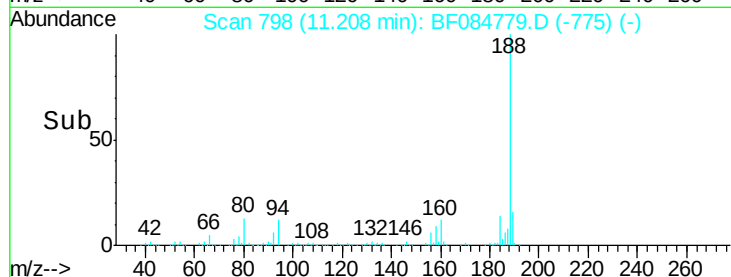

#66

4-Bromophenyl-phenylether

Concen: 4.16 ng

RT: 10.52 min Scan# 738

Delta R.T. -0.27 min

Lab File: BF084779.D

Acq: 3 Feb 2016 8:03


Tgt Ion:248 Resp: 31862

Ion Ratio Lower Upper

248 100

250 181.7 78.4 117.6#



141 602.1 44.0 66.0#




Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

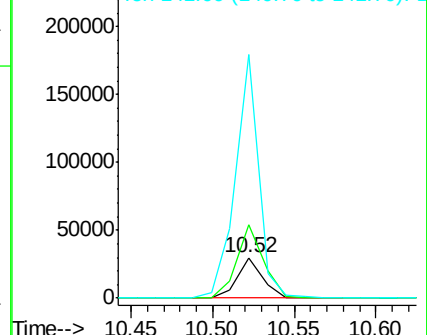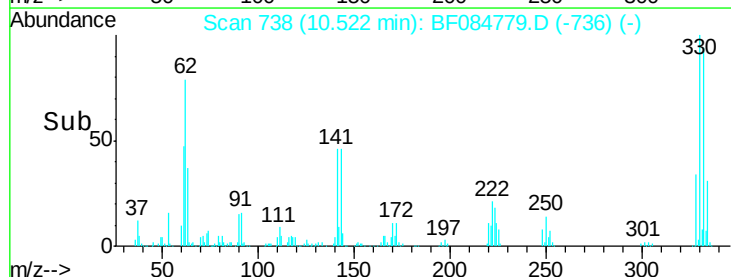

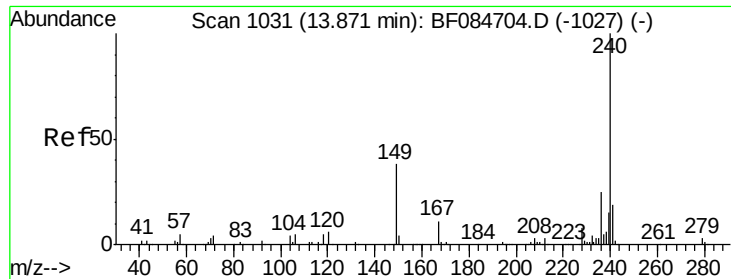

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.85 min Scan# 1029

Delta R.T. -0.02 min

Lab File: BF084779.D

Acq: 3 Feb 2016 8:03

Instrument :

BNA_F

ClientSampleId :

HSR-WC-24-012916


Tot Ion:240 Resp: 493439

Ion Ratio Lower Upper

240 100

120 6.3 9.5 14.3#




236 25.3 20.6 31.0

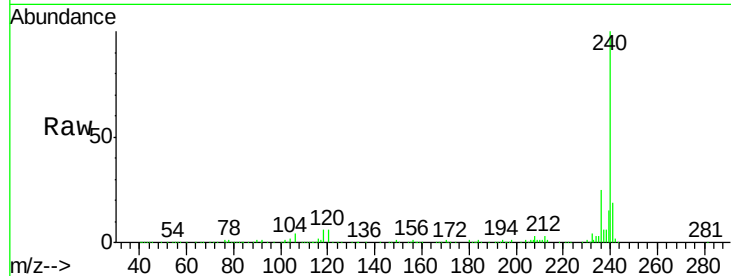

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

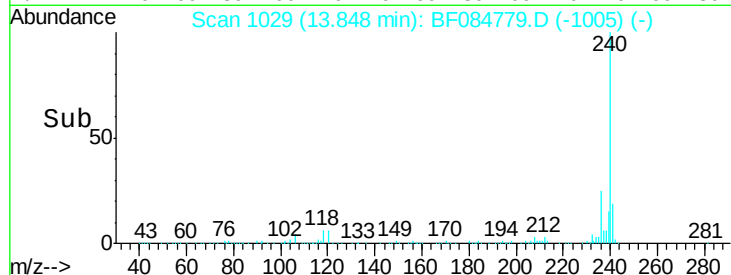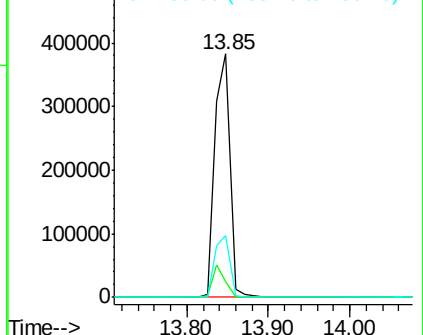

#76

Benzidine

Concen: 8.96 ng

RT: 12.56 min Scan# 916

Delta R.T. -0.02 min

Lab File: BF084779.D

Acq: 3 Feb 2016 8:03


Tgt Ion:184 Resp: 53929

Ion Ratio Lower Upper

184 100

185 12.1 12.2 18.2#



183 9.7 9.8 14.8#




Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

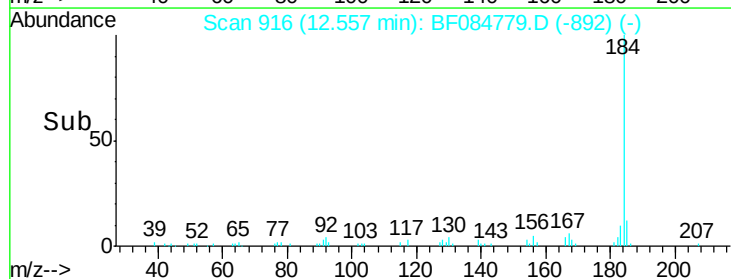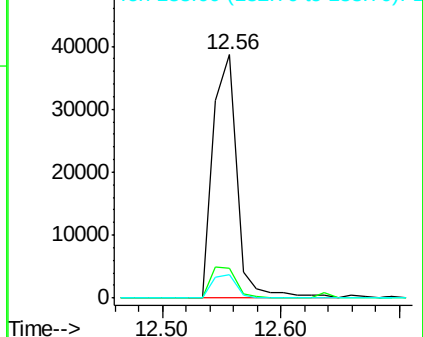

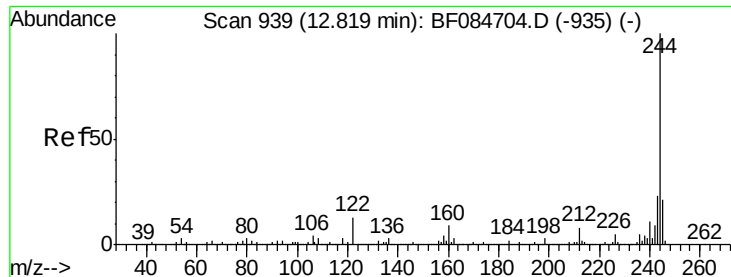

#78

Terphenyl-d14

Concen: 97.27 ng

RT: 12.81 min Scan# 938

Delta R.T. -0.02 min

Lab File: BF084779.D

Acq: 3 Feb 2016 8:03

Instrument :

BNA_F

ClientSampleId :

HSR-WC-24-012916


Tot Ion:244 Resp: 2118160

Ion Ratio Lower Upper

244 100

212 7.6 5.7 8.5




122 11.3 7.4 11.0#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

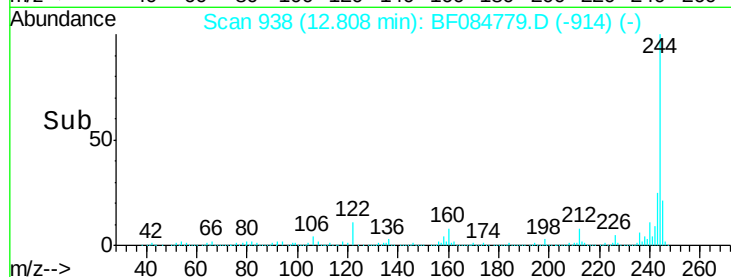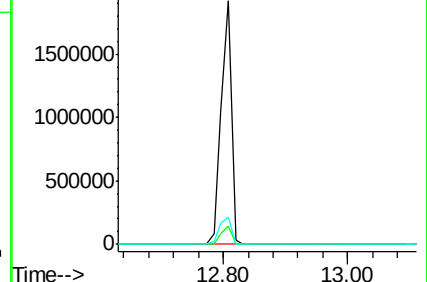

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.22 min Scan# 1149

Delta R.T. -0.03 min

Lab File: BF084779.D

Acq: 3 Feb 2016 8:03


Tgt Ion:264 Resp: 364033

Ion Ratio Lower Upper

264 100

260 23.5 19.4 29.2

265 21.6 17.8 26.6



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

