

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020216\
 Data File : BF084763.D
 Acq On : 3 Feb 2016 00:41
 Operator : SJ/IZ
 Sample : PB88115BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB88115BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.144	177	180	187	rVB	36471	51179	2.99%	0.365%
2	4.830	238	240	246	rBV	527142	563060	32.92%	4.011%
3	5.287	277	280	282	rBV	424390	614391	35.92%	4.377%
4	5.687	314	315	318	rBV	22657	30903	1.81%	0.220%
5	6.339	369	372	374	rBV	647852	607885	35.54%	4.330%
6	6.464	380	383	385	rBV	543701	640790	37.46%	4.565%
7	6.693	401	403	406	rVB	1375696	1147593	67.09%	8.175%
8	6.853	415	417	419	rBV	485231	507909	29.69%	3.618%
9	7.264	450	453	455	rBV	338038	380860	22.27%	2.713%
10	7.984	513	516	518	rBV	1757924	1608438	94.03%	11.458%
11	9.059	608	610	613	rBV	905887	765390	44.75%	5.452%
12	9.733	666	669	672	rBV	1895297	1710481	100.00%	12.185%
13	10.522	735	738	740	rBV	343343	410432	24.00%	2.924%
14	11.208	796	798	801	rBV	1383785	1662533	97.20%	11.843%
15	12.796	935	937	939	rBV	926629	771722	45.12%	5.497%
16	13.848	1026	1029	1031	rBV	1063717	1497103	87.53%	10.665%
17	15.219	1146	1149	1152	rBV	914491	1042769	60.96%	7.428%
18	15.265	1152	1153	1160	rVB7	14820	24269	1.42%	0.173%




Sum of corrected areas: 14037707

Data Path : Z:\HPCHEM1\BNA F\DATA\BF020216\
Data File : BF084763.D
Acq On : 3 Feb 2016 00:41
Operator : SJ/IZ
Sample : PB88115BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB88115BL

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

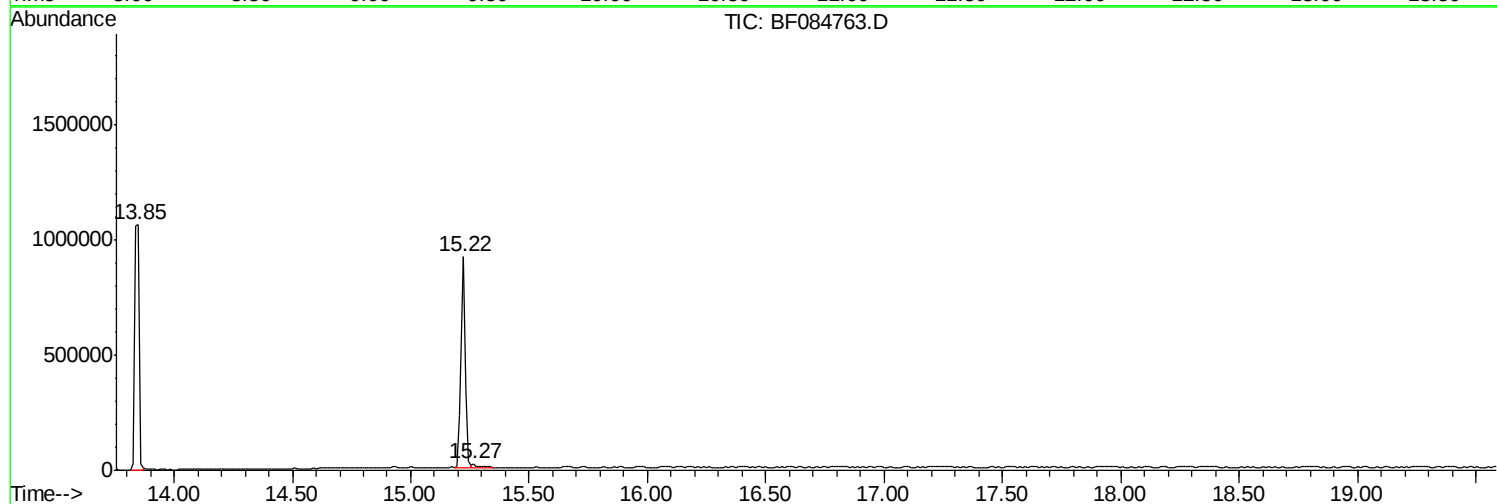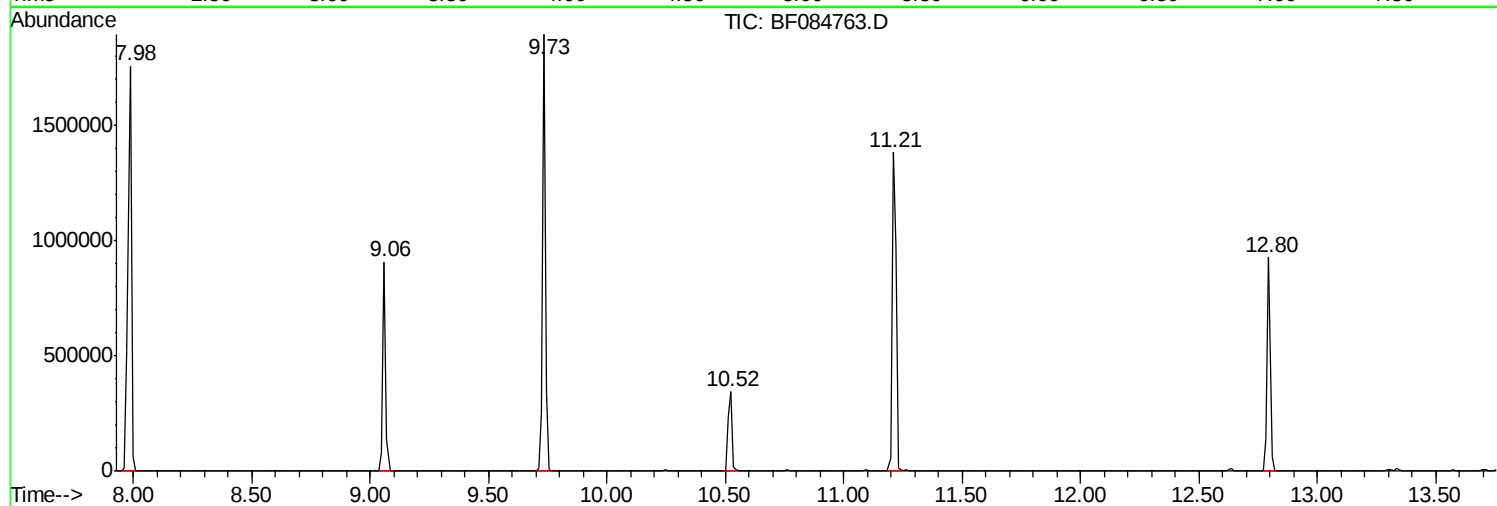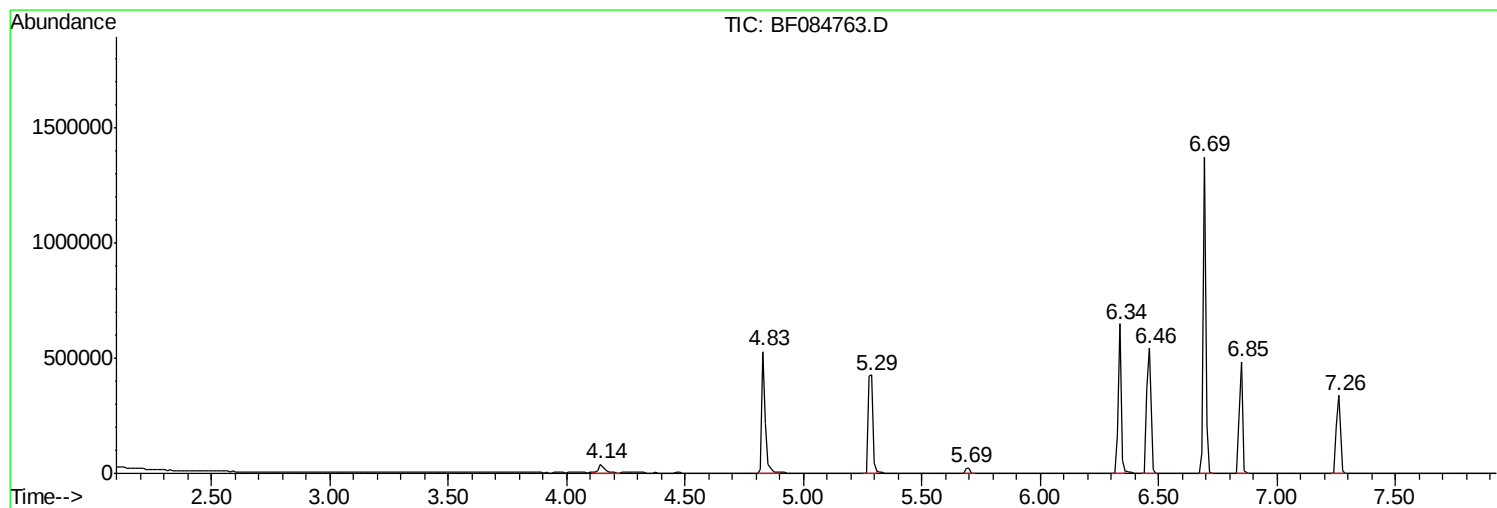

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020216\
Data File : BF084763.D
Acq On : 3 Feb 2016 00:41
Operator : SJ/IZ
Sample : PB88115BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB88115BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.83	9.81 ng	563060	1,4-Dichlorobenzene-d4	6.69

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
2			Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	42
3			2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	33
4			3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33
5			3-Hexanol	102	C6H14O	000623-37-0	33

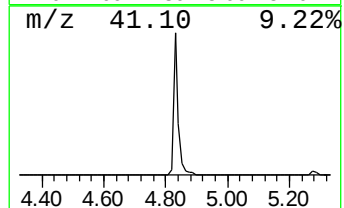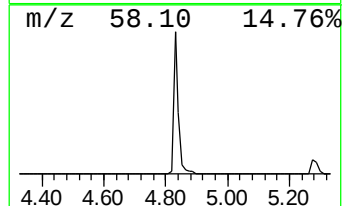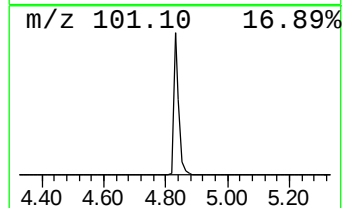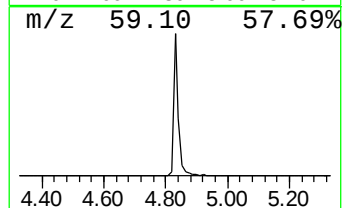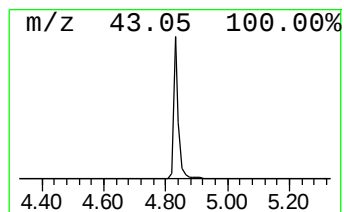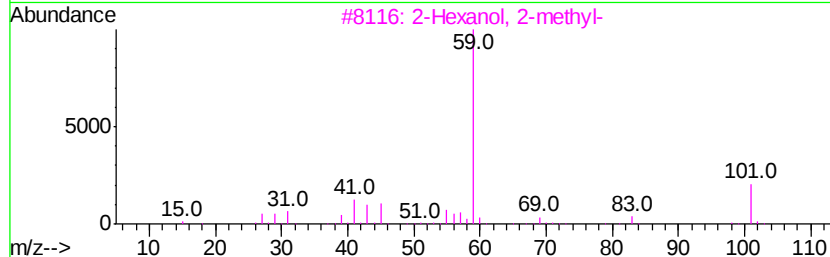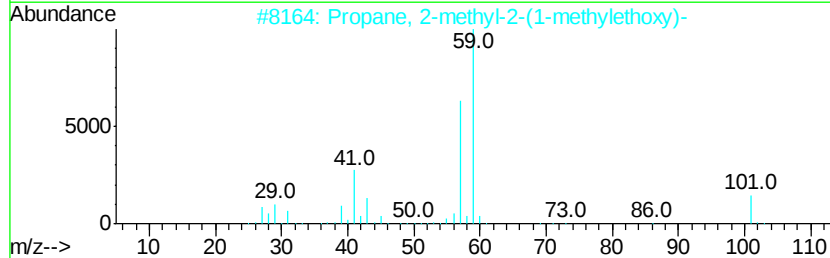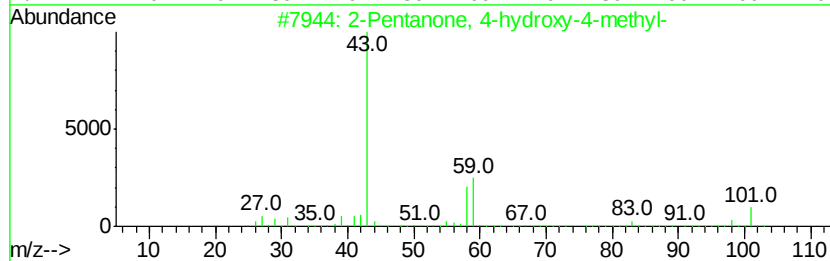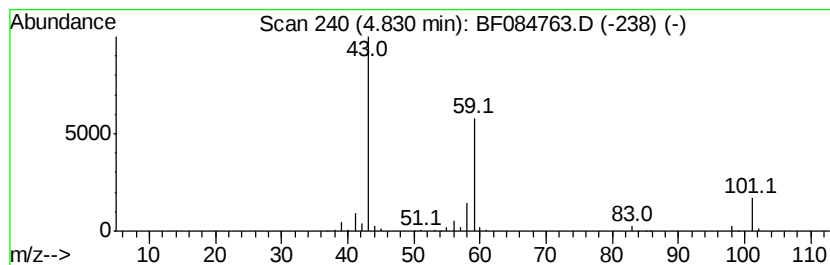

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020216\
Data File : BF084763.D
Acq On : 3 Feb 2016 00:41
Operator : SJ/IZ
Sample : PB88115BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB88115BL









Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.46 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.46	11.17 ng	640790	1,4-Dichlorobenzene-d4	6.69

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Chloro-6-fluoro-pyrazine			132	C4H2ClFN2	1000146-10-7	38
2	(E)-3-Chloro-2-methyl-2-pentenal			132	C6H9ClO	031357-76-3	17
3	5-Aminoindole			132	C8H8N2	005192-03-0	10
4	Benzene, 1,3,5-trifluoro-			132	C6H3F3	000372-38-3	9
5	Xenon			132	Xe	007440-63-3	9

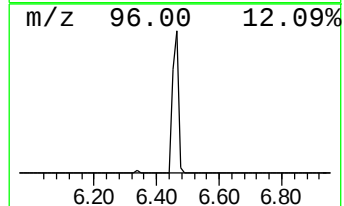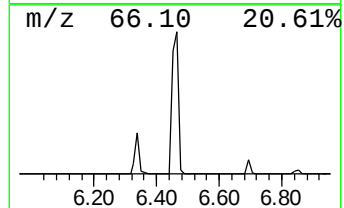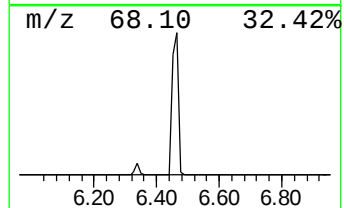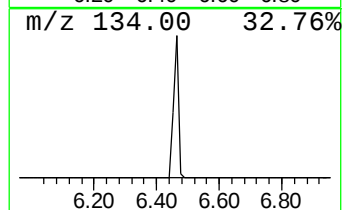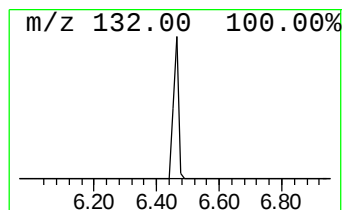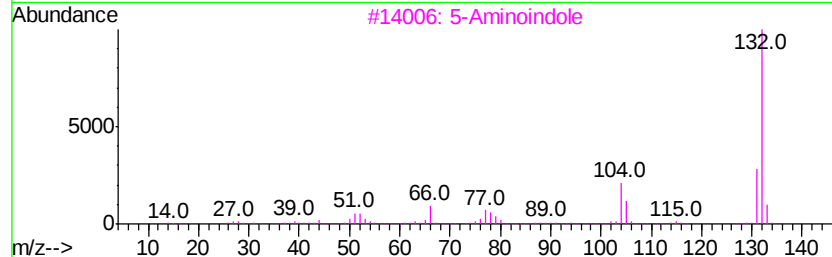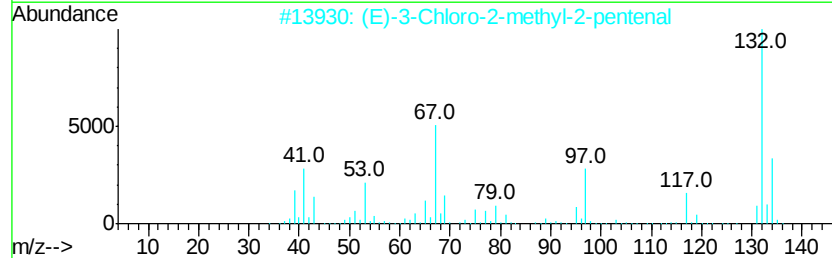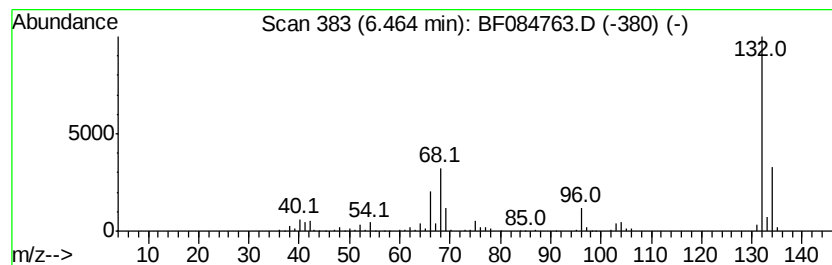

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020216\
Data File : BF084763.D
Acq On : 3 Feb 2016 00:41
Operator : SJ/IZ
Sample : PB88115BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB88115BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.83	9.8	ng	563060	1	6.69	1147590	20.0
unknown6.46	6.46	11.2	ng	640790	1	6.69	1147590	20.0