


Data Path : Z:\HPCHEM1\BNA_F\Data\BF020216\
 Data File : BF084746.D
 Acq On : 2 Feb 2016 10:16
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 01 14:55:11 2016

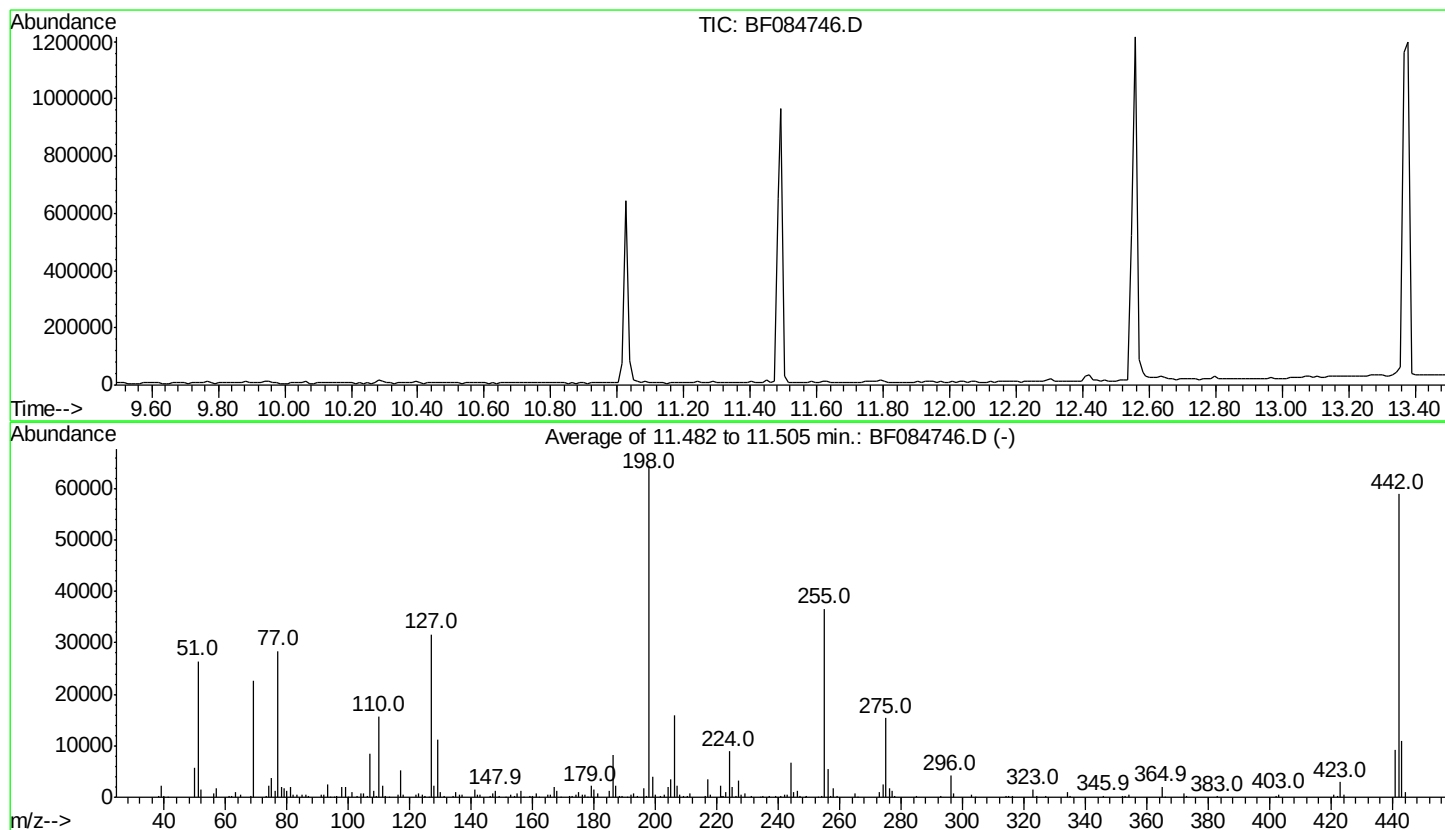

AutoFind: Scans 822, 823, 824; Background Corrected with Scan 818

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.9	26385	PASS
68	69	0.00	2	1.5	347	PASS
69	198	0.00	100	35.3	22754	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.0	31600	PASS
197	198	0.00	2	0.5	301	PASS
198	198	100	100	100.0	64453	PASS
199	198	5	9	6.3	4088	PASS
275	198	10	60	23.8	15348	PASS
365	198	1	100	3.2	2034	PASS
441	442	0.01	24	15.5	9145	PASS
442	198	50	100	91.3	58863	PASS
443	442	15	24	18.8	11060	PASS