


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020216\
 Data File : BF084761.D
 Acq On : 2 Feb 2016 23:46
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 01 14:55:11 2016

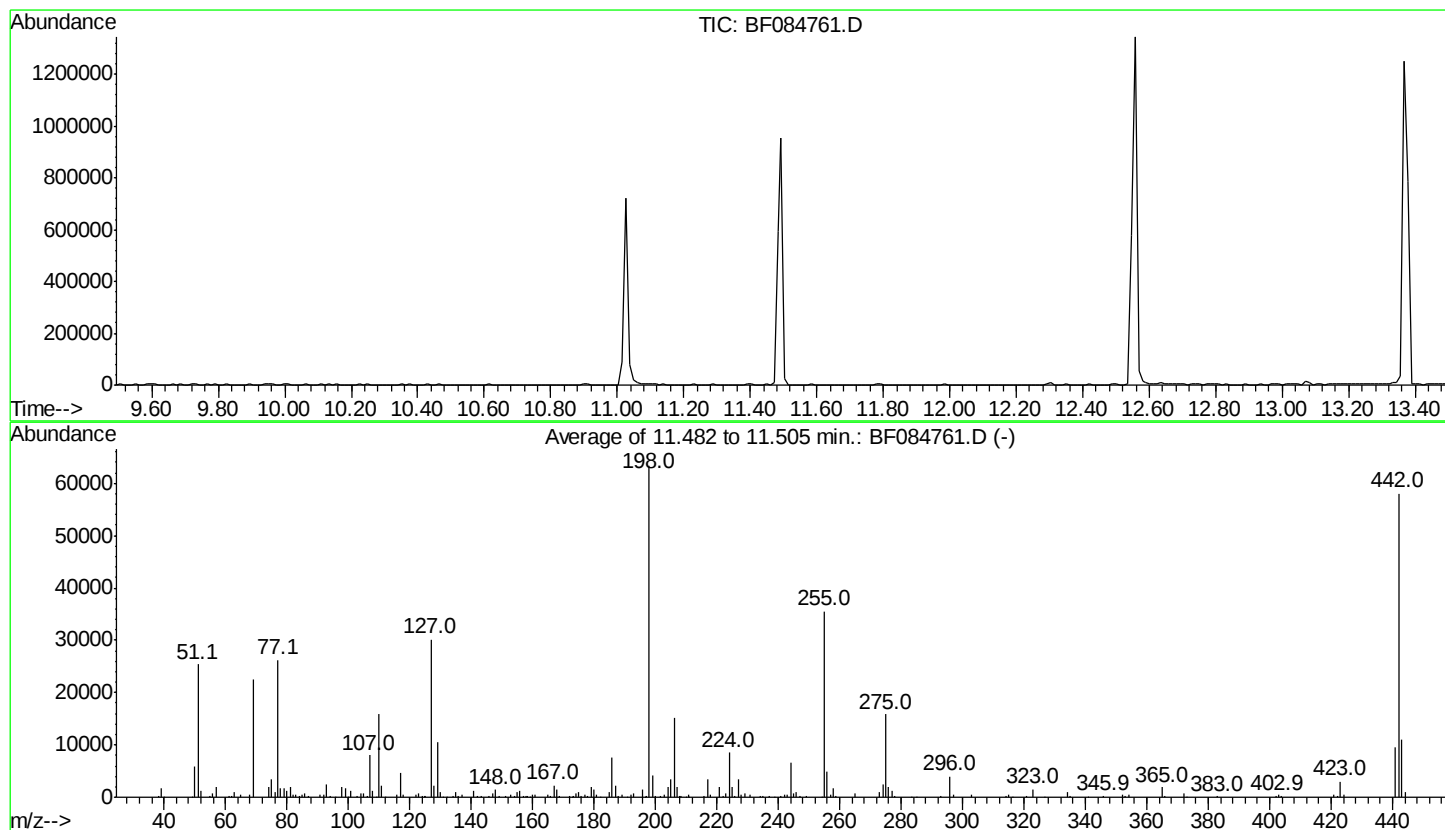

AutoFind: Scans 822, 823, 824; Background Corrected with Scan 818

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	25402	PASS
68	69	0.00	2	1.7	390	PASS
69	198	0.00	100	35.5	22496	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.5	30120	PASS
197	198	0.00	2	0.3	187	PASS
198	198	100	100	100.0	63371	PASS
199	198	5	9	6.5	4110	PASS
275	198	10	60	25.0	15830	PASS
365	198	1	100	2.9	1845	PASS
441	442	0.01	24	16.4	9528	PASS
442	198	50	100	91.5	57984	PASS
443	442	15	24	18.8	10910	PASS