

Data Path : Z:\HPCHEM1\BNA F\Data\BF020217\
 Data File : BF092772.D
 Acq On : 3 Feb 2017 11:36
 Operator : SJ/MA
 Sample : PB96683BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Feb 03 12:20:21 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 30 14:50:05 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.93	152	142611	20.00	ng	-0.03
21) Naphthalene-d8	8.22	136	553791	20.00	ng	-0.03
38) Acenaphthene-d10	9.98	164	282311	20.00	ng	-0.02
63) Phenanthrene-d10	11.46	188	404845	20.00	ng	-0.03
75) Chrysene-d12	14.10	240	328796	20.00	ng	-0.05
86) Perylene-d12	15.56	264	293439	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.55	112	956574	115.08	ng	-0.02
7) Phenol-d6	6.57	99	1156703	108.15	ng	-0.03
23) Nitrobenzene-d5	7.50	82	696410	70.03	ng	-0.03
41) 2,4,6-Tribromophenol	10.77	330	207887	101.81	ng	-0.03
44) 2-Fluorobiphenyl	9.30	172	1243335	79.79	ng	-0.03
78) Terphenyl-d14	13.05	244	987771	70.59	ng	-0.03
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.49	70	90062	13.23	ng	# 83
25) Isophorone	7.50	82	657398	35.48	ng	# 65
50) 2,6-Dinitrotoluene	9.98	165	35663	8.68	ng	# 29
56) 2,4-Dinitrotoluene	9.98	165	35664	6.52	ng	# 18
64) 4,6-Dinitro-2-methylphenol	10.76	198	222	2.75	ng	# 1
66) 4-Bromophenyl-phenylether	10.77	248	14328	3.39	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\Data\BF020217\
Data File : BF092772.D
Acq On : 3 Feb 2017 11:36
Operator : SJ/MA
Sample : PB96683BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Feb 03 12:20:21 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 30 14:50:05 2017
Response via : Initial Calibration

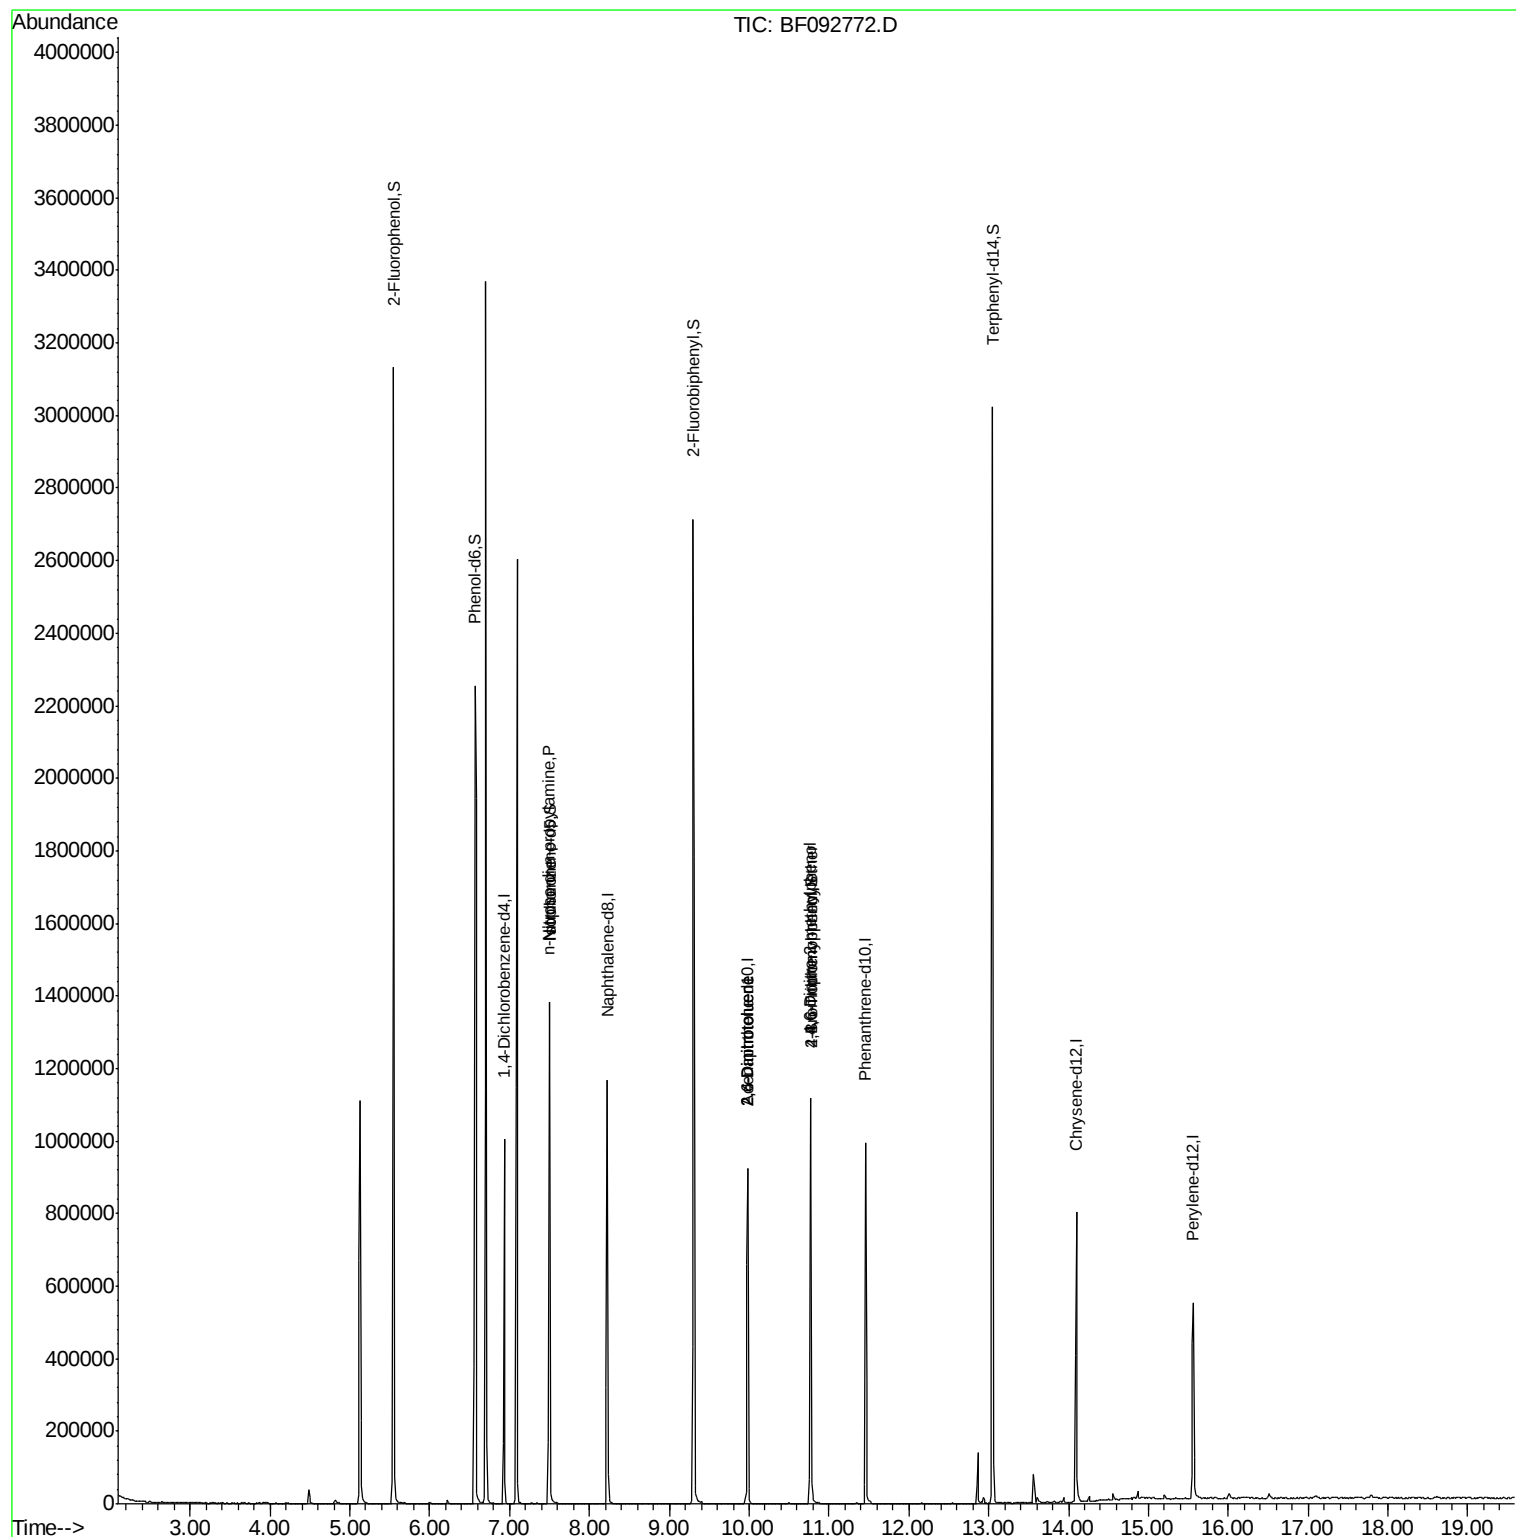



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.93 min Scan# 424

Delta R.T. -0.03 min

Lab File: BF092772.D

Acq: 3 Feb 2017 11:36

Instrument :

BNA_F

ClientSampleId :


Tot Ion:152 Resp: 142611

Ion Ratio Lower Upper

152 100

150 157.1 124.9 187.3




115 58.1 46.0 69.0



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

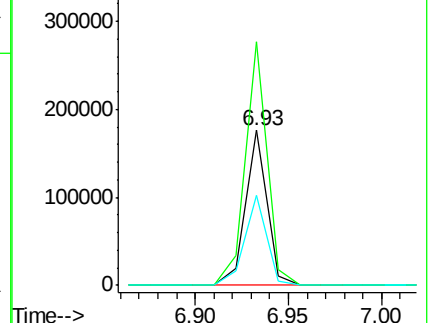

#5

2-Fluorophenol

Concen: 115.08 ng

RT: 5.55 min Scan# 303

Delta R.T. -0.02 min

Lab File: BF092772.D

Acq: 3 Feb 2017 11:36


Tgt Ion:112 Resp: 956574

Ion Ratio Lower Upper

112 100

64 60.9 46.1 69.1



63 30.4 23.8 35.6




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

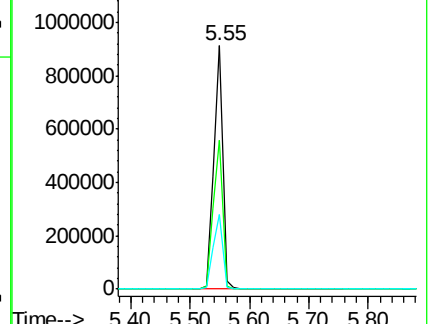

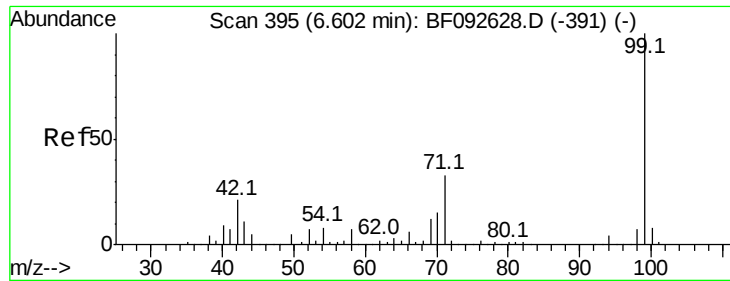

#7

Phenol-d6

Concen: 108.15 ng

RT: 6.57 min Scan# 392

Delta R.T. -0.03 min

Lab File: BF092772.D

Acq: 3 Feb 2017 11:36

Instrument :

BNA_F

ClientSampled :


Tot Ion: 99 Resp: 1156703

Ion Ratio Lower Upper

99 100

42 21.0 15.6 23.4




71 34.0 27.5 41.3

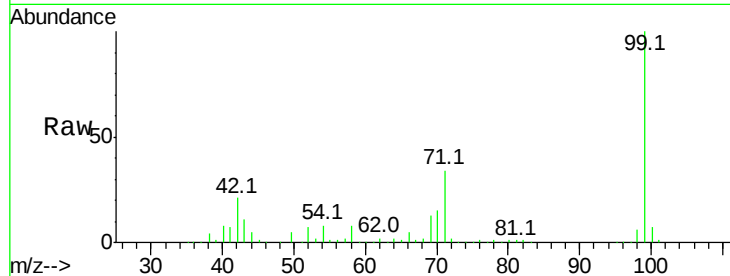

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

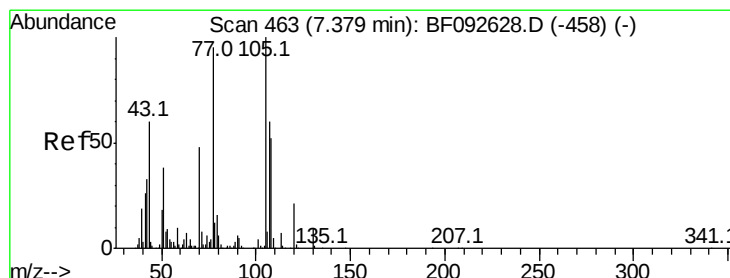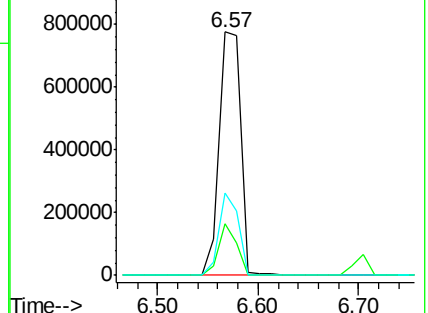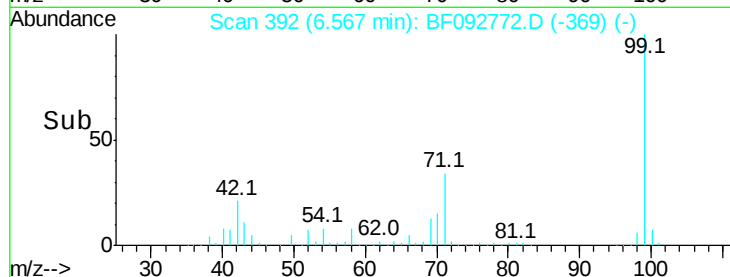

#19

n-Nitroso-di-n-propylamine

Concen: 13.23 ng

RT: 7.49 min Scan# 473

Delta R.T. 0.11 min

Lab File: BF092772.D

Acq: 3 Feb 2017 11:36

Tgt Ion: 70 Resp: 90062


Ion Ratio Lower Upper

70 100

42 54.1 49.4 74.0

101 0.0 7.4 11.2#

130 1.9 14.2 21.4#


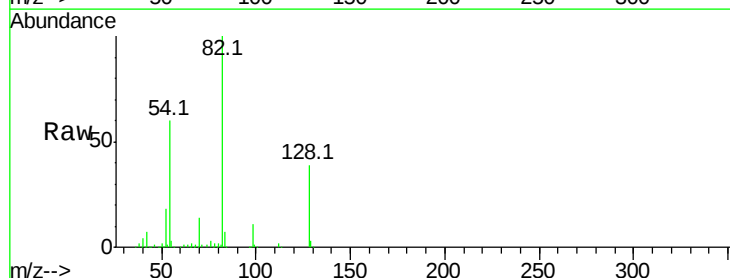


Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0

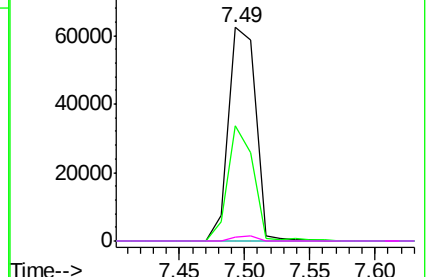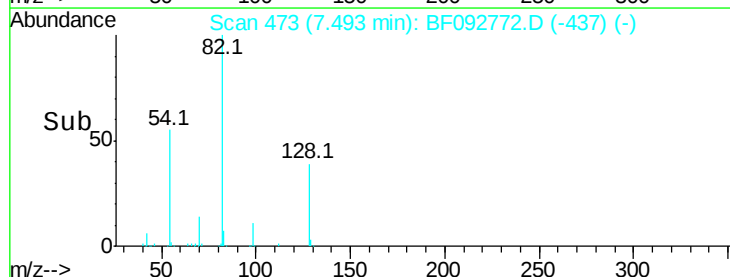






#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.22 min Scan# 537
Delta R.T. -0.03 min
Lab File: BF092772.D
Acq: 3 Feb 2017 11:36

Instrument :
BNA_F
ClientSampleId :

Tot Ion:136	Resp:	553791
Ion	Ratio	Lower Upper
136	100	
137	10.4	8.4 12.6
54	9.0	4.5 6.7#
68	6.2	3.6 5.4#




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

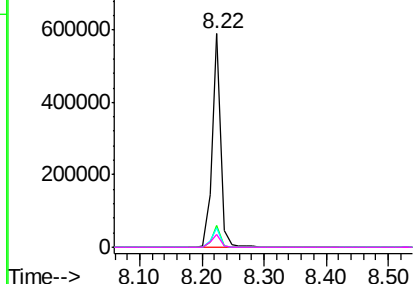




#23
Nitrobenzene-d5
Concen: 70.03 ng
RT: 7.50 min Scan# 474
Delta R.T. -0.03 min
Lab File: BF092772.D
Acq: 3 Feb 2017 11:36

Tgt Ion: 82	Resp:	696410
Ion	Ratio	Lower Upper
82	100	
128	54.6	34.6 52.0#
54	49.2	39.5 59.3



Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

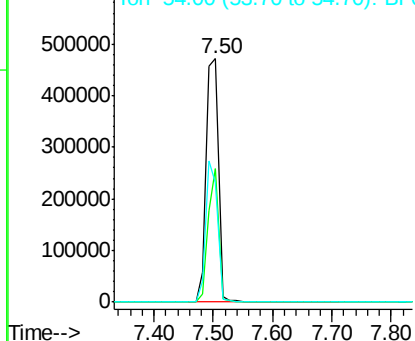

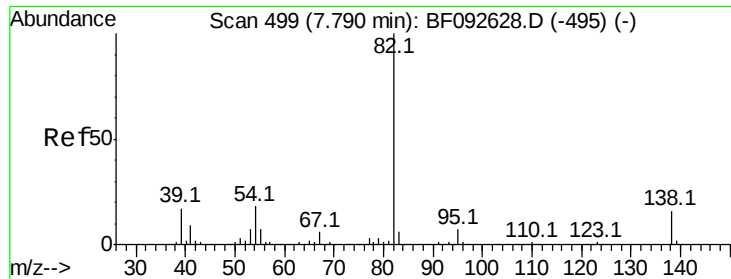

#25

Isophorone

Concen: 35.48 ng

RT: 7.50 min Scan# 474

Delta R.T. -0.29 min

Lab File: BF092772.D

Acq: 3 Feb 2017 11:36

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 657398

Ion Ratio Lower Upper




82 100

95 0.0 5.6 8.4#

138 0.0 14.6 22.0#



Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 95.00 (94.70 to 95.70): BF0
Ion 138.00 (137.70 to 138.70): E

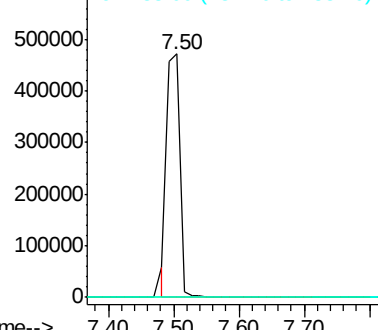

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.98 min Scan# 691

Delta R.T. -0.02 min

Lab File: BF092772.D

Acq: 3 Feb 2017 11:36


Tgt Ion:164 Resp: 282311

Ion Ratio Lower Upper



164 100

162 101.5 80.2 120.2

160 42.8 36.9 55.3



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

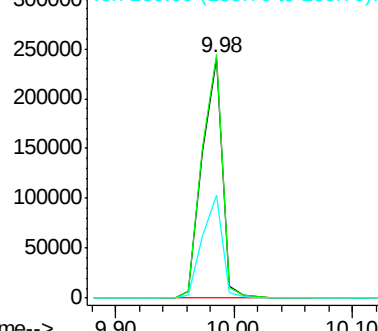







#41
 2,4,6-Tribromophenol
 Concen: 101.81 ng
 RT: 10.77 min Scan# 760
 Delta R.T. -0.03 min
 Lab File: BF092772.D
 Acq: 3 Feb 2017 11:36

Instrument :
 BNA_F
 ClientSampled :

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.9	77.4	116.2
141	32.6	34.1	51.1#




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


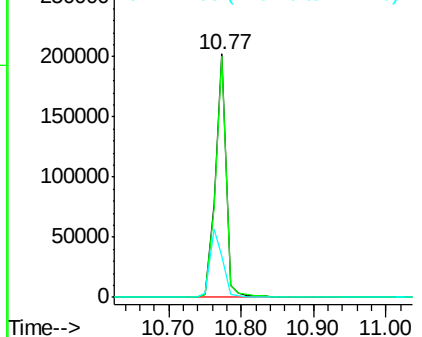



#44
 2-Fluorobiphenyl
 Concen: 79.79 ng
 RT: 9.30 min Scan# 631
 Delta R.T. -0.03 min
 Lab File: BF092772.D
 Acq: 3 Feb 2017 11:36

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.2	29.4	44.0
170	23.8	20.2	30.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E




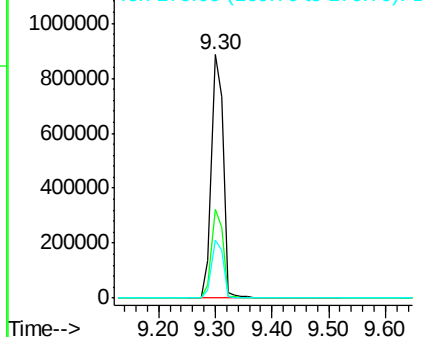




#50
 2,6-Dinitrotoluene
 Concen: 8.68 ng
 RT: 9.98 min Scan# 691
 Delta R.T. 0.19 min
 Lab File: BF092772.D
 Acq: 3 Feb 2017 11:36




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:165 Resp: 35663
 Ion Ratio Lower Upper
 165 100
 63 0.0 36.2 54.4#
 89 0.0 40.2 60.4#

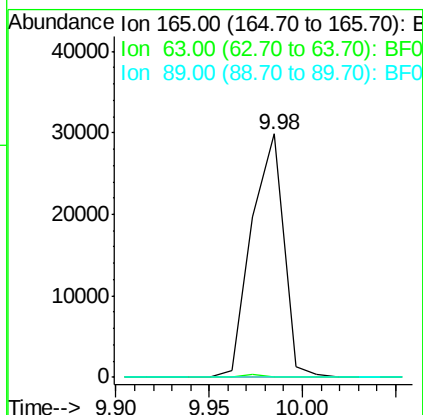

#56
 2,4-Dinitrotoluene
 Concen: 6.52 ng
 RT: 9.98 min Scan# 691
 Delta R.T. -0.22 min
 Lab File: BF092772.D
 Acq: 3 Feb 2017 11:36

Tgt Ion:165 Resp: 35664
 Ion Ratio Lower Upper
 165 100
 63 0.0 40.2 60.4#
 89 0.0 62.5 93.7#
 182 0.0 1.8 2.8#

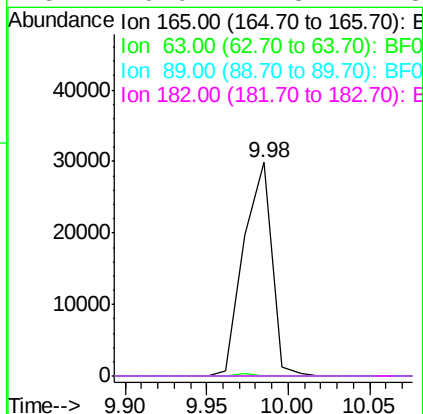


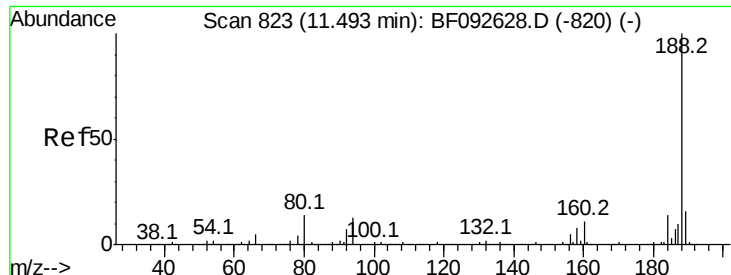




#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.46 min Scan# 820
 Delta R.T. -0.03 min
 Lab File: BF092772.D
 Acq: 3 Feb 2017 11:36

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:188 Resp: 404845
 Ion Ratio Lower Upper
 188 100
 94 12.6 10.0 15.0
 80 13.2 11.2 16.8




Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0

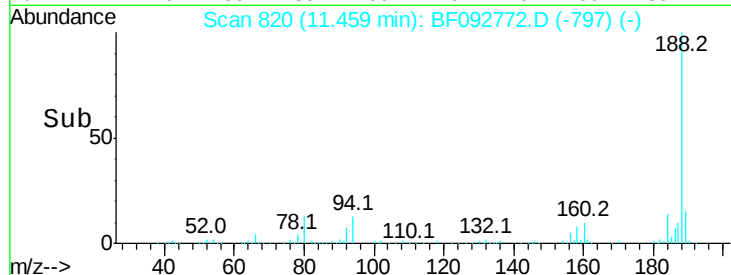
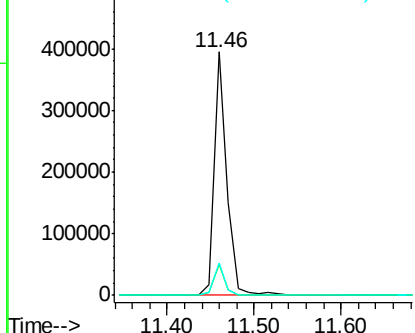



#64
 4,6-Dinitro-2-methylphenol
 Concen: 2.75 ng
 RT: 10.76 min Scan# 759
 Delta R.T. 0.15 min
 Lab File: BF092772.D
 Acq: 3 Feb 2017 11:36

Tgt Ion:198 Resp: 222
 Ion Ratio Lower Upper
 198 100
 51 356.7 6.7 46.7#
 105 242.4 16.6 56.6#



Abundance Ion 198.00 (197.70 to 198.70): E
 Ion 51.00 (50.70 to 51.70): BF0
 Ion 105.00 (104.70 to 105.70): E

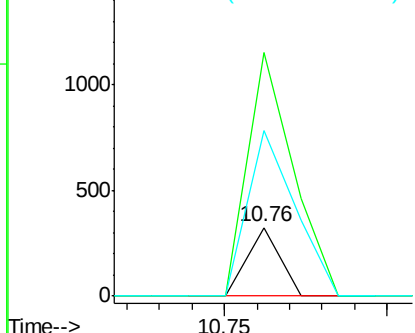


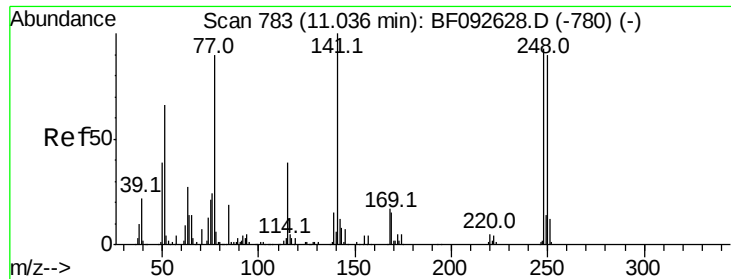




#66
 4-Bromophenyl-phenylether
 Concen: 3.39 ng
 RT: 10.77 min Scan# 760
 Delta R.T. -0.26 min
 Lab File: BF092772.D
 Acq: 3 Feb 2017 11:36

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:248 Resp: 14328
 Ion Ratio Lower Upper
 248 100
 250 203.3 76.9 115.3#
 141 293.9 68.2 102.4#

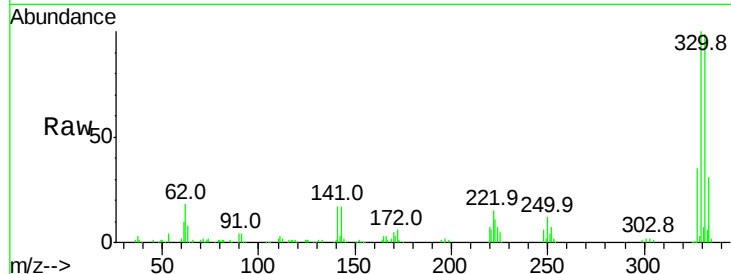


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E


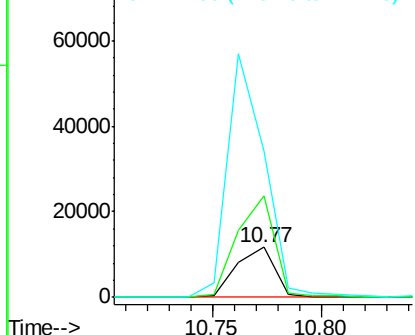



#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 14.10 min Scan# 1051
 Delta R.T. -0.05 min
 Lab File: BF092772.D
 Acq: 3 Feb 2017 11:36

Tgt Ion:240 Resp: 328796
 Ion Ratio Lower Upper
 240 100
 120 10.7 12.9 19.3#
 236 25.5 20.9 31.3



Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

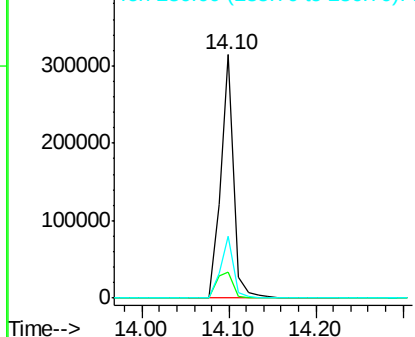


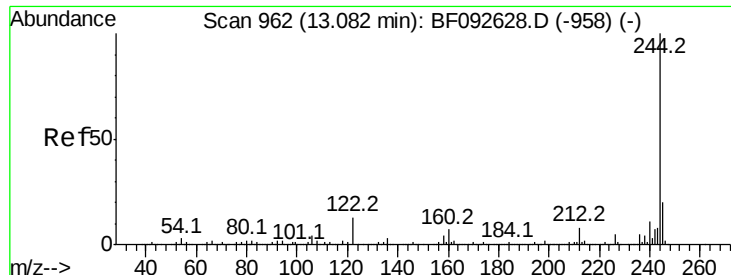




#78
 Terphenyl-d14
 Concen: 70.59 ng
 RT: 13.05 min Scan# 959
 Delta R.T. -0.03 min
 Lab File: BF092772.D
 Acq: 3 Feb 2017 11:36

Instrument :
 BNA_F
 ClientSampled :

Tot Ion:244 Resp: 987771
 Ion Ratio Lower Upper
 244 100
 212 7.4 6.2 9.2
 122 11.2 11.4 17.2#




Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

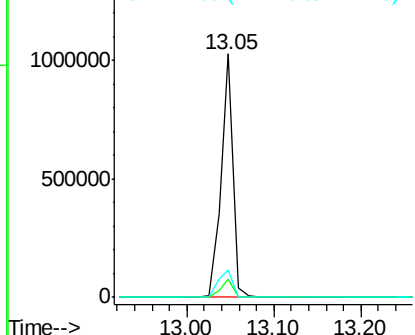

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.56 min Scan# 1179
 Delta R.T. -0.05 min
 Lab File: BF092772.D
 Acq: 3 Feb 2017 11:36

Tgt Ion:264 Resp: 293439
 Ion Ratio Lower Upper
 264 100
 260 24.0 19.2 28.8
 265 21.3 17.4 26.0



Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

