
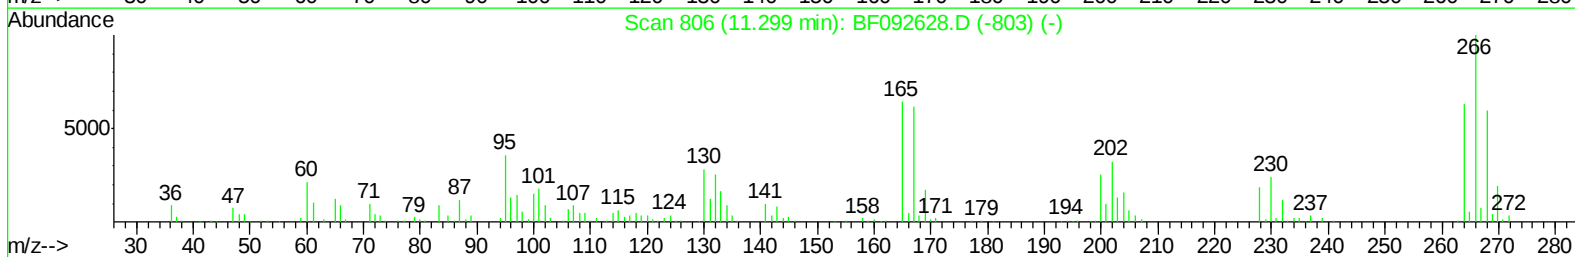
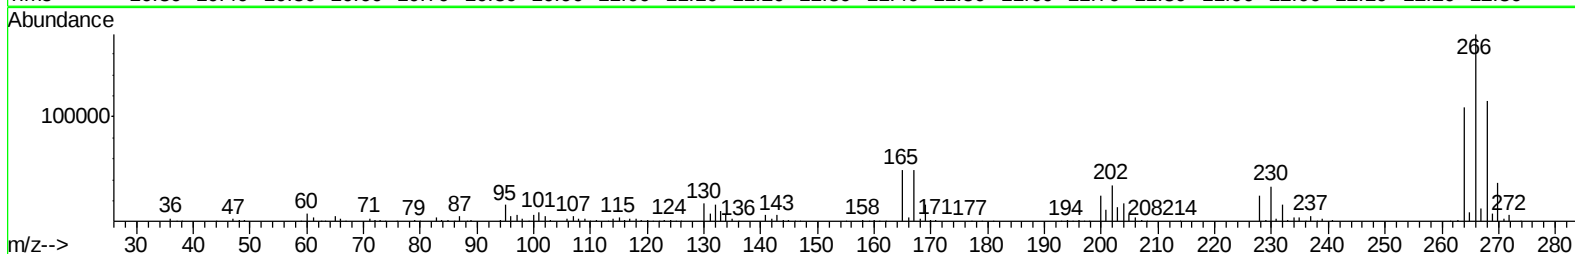


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020217\
Data File : BF092735.D
Acq On : 2 Feb 2017 15:00
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 06:44:38 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 30 14:50:05 2017
Response via : Initial Calibration

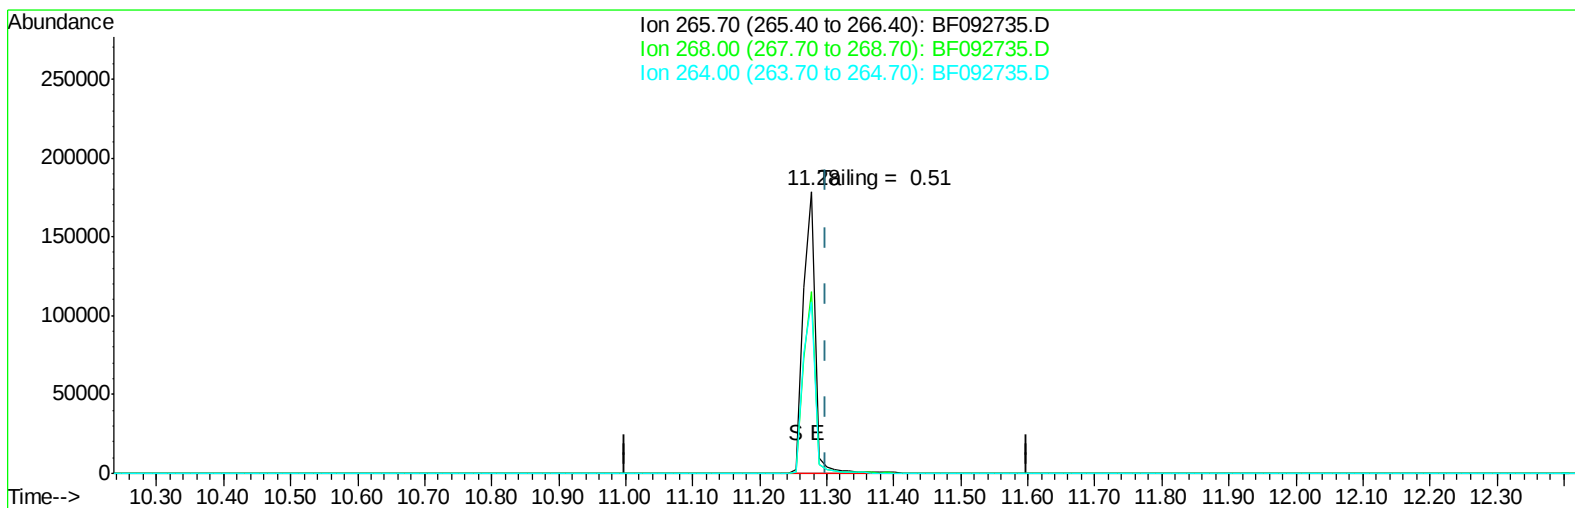

TIC: BF092735.D

(69) Pentachlorophenol (C)




11.276min (-0.023) 100183.45ng

response 220610

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	64.40
264.00	62.90	61.09
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020217\
Data File : BF092735.D
Acq On : 2 Feb 2017 15:00
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 06:44:38 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 30 14:50:05 2017
Response via : Initial Calibration

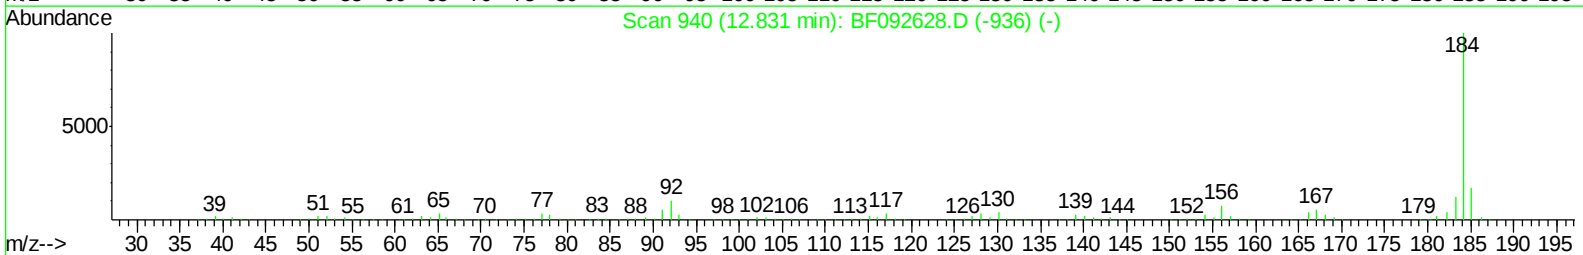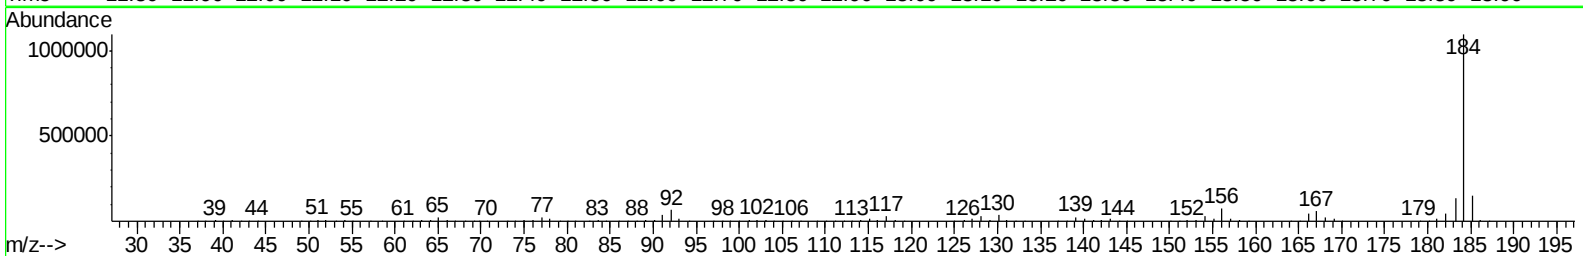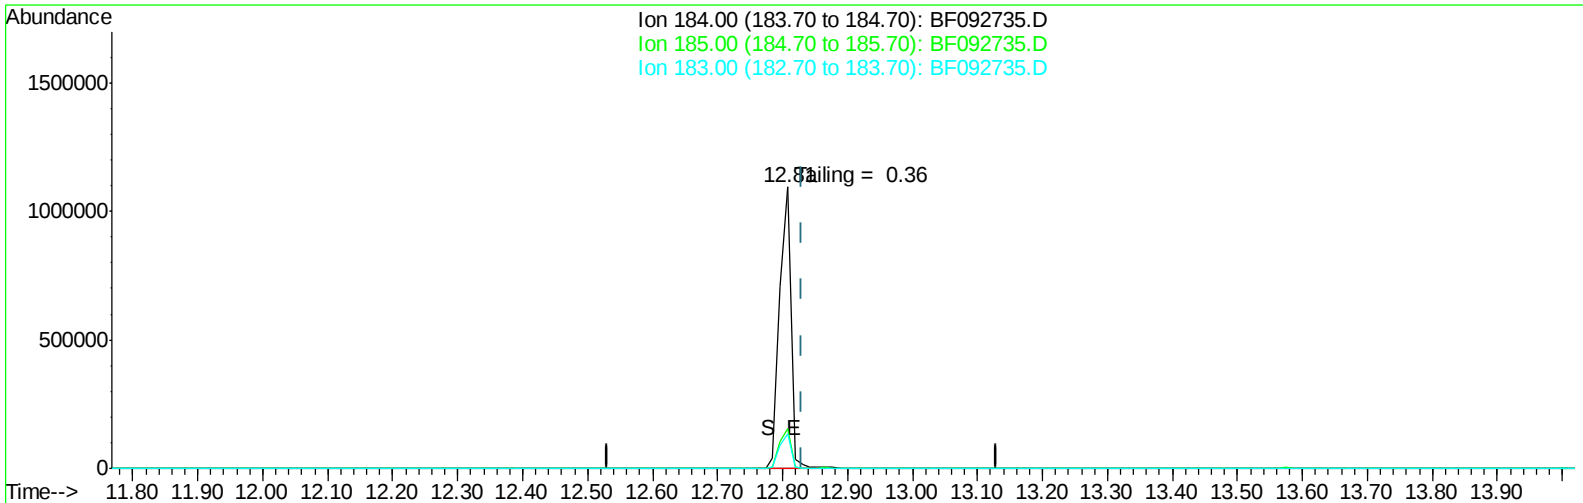

TIC: BF092735.D

(76) Benzidine

12.808min (-0.023) 30796.30ng m

response 1308377

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.08
183.00	11.50	12.26
0.00	0.00	0.00