

Data Path : Z:\HPCHEM1\BNA F\DATA\BF020217\
 Data File : BF092739.D
 Acq On : 2 Feb 2017 17:10
 Operator : SJ/MA
 Sample : I1664-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 ROLL-OFF-275032-COMP-0-2FT

Quant Time: Feb 03 00:13:58 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 30 14:50:05 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.93	152	162702	20.00	ng	-0.03
21) Naphthalene-d8	8.22	136	563106	20.00	ng	-0.03
38) Acenaphthene-d10	9.97	164	295322	20.00	ng	-0.03
63) Phenanthrene-d10	11.46	188	509219	20.00	ng	-0.03
75) Chrysene-d12	14.10	240	494720	20.00	ng	-0.05
86) Perylene-d12	15.56	264	426020	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.54	112	595605	62.80	ng	-0.03
7) Phenol-d6	6.57	99	754937	61.87	ng	-0.03
23) Nitrobenzene-d5	7.49	82	445805	44.09	ng	-0.05
41) 2,4,6-Tribromophenol	10.76	330	182614	85.50	ng	-0.05
44) 2-Fluorobiphenyl	9.30	172	863043	52.94	ng	-0.03
78) Terphenyl-d14	13.05	244	989418	46.99	ng	-0.03
Target Compounds						
10) Phenol	6.58	94	31006	2.17	ng	Qvalue 92
49) Dimethylphthalate	9.69	163	94794	4.77	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF020217\
Data File : BF092739.D
Acq On : 2 Feb 2017 17:10
Operator : SJ/MA
Sample : I1664-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ROLL-OFF-275032-COMP-0-2FT

Quant Time: Feb 03 00:13:58 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 30 14:50:05 2017
Response via : Initial Calibration

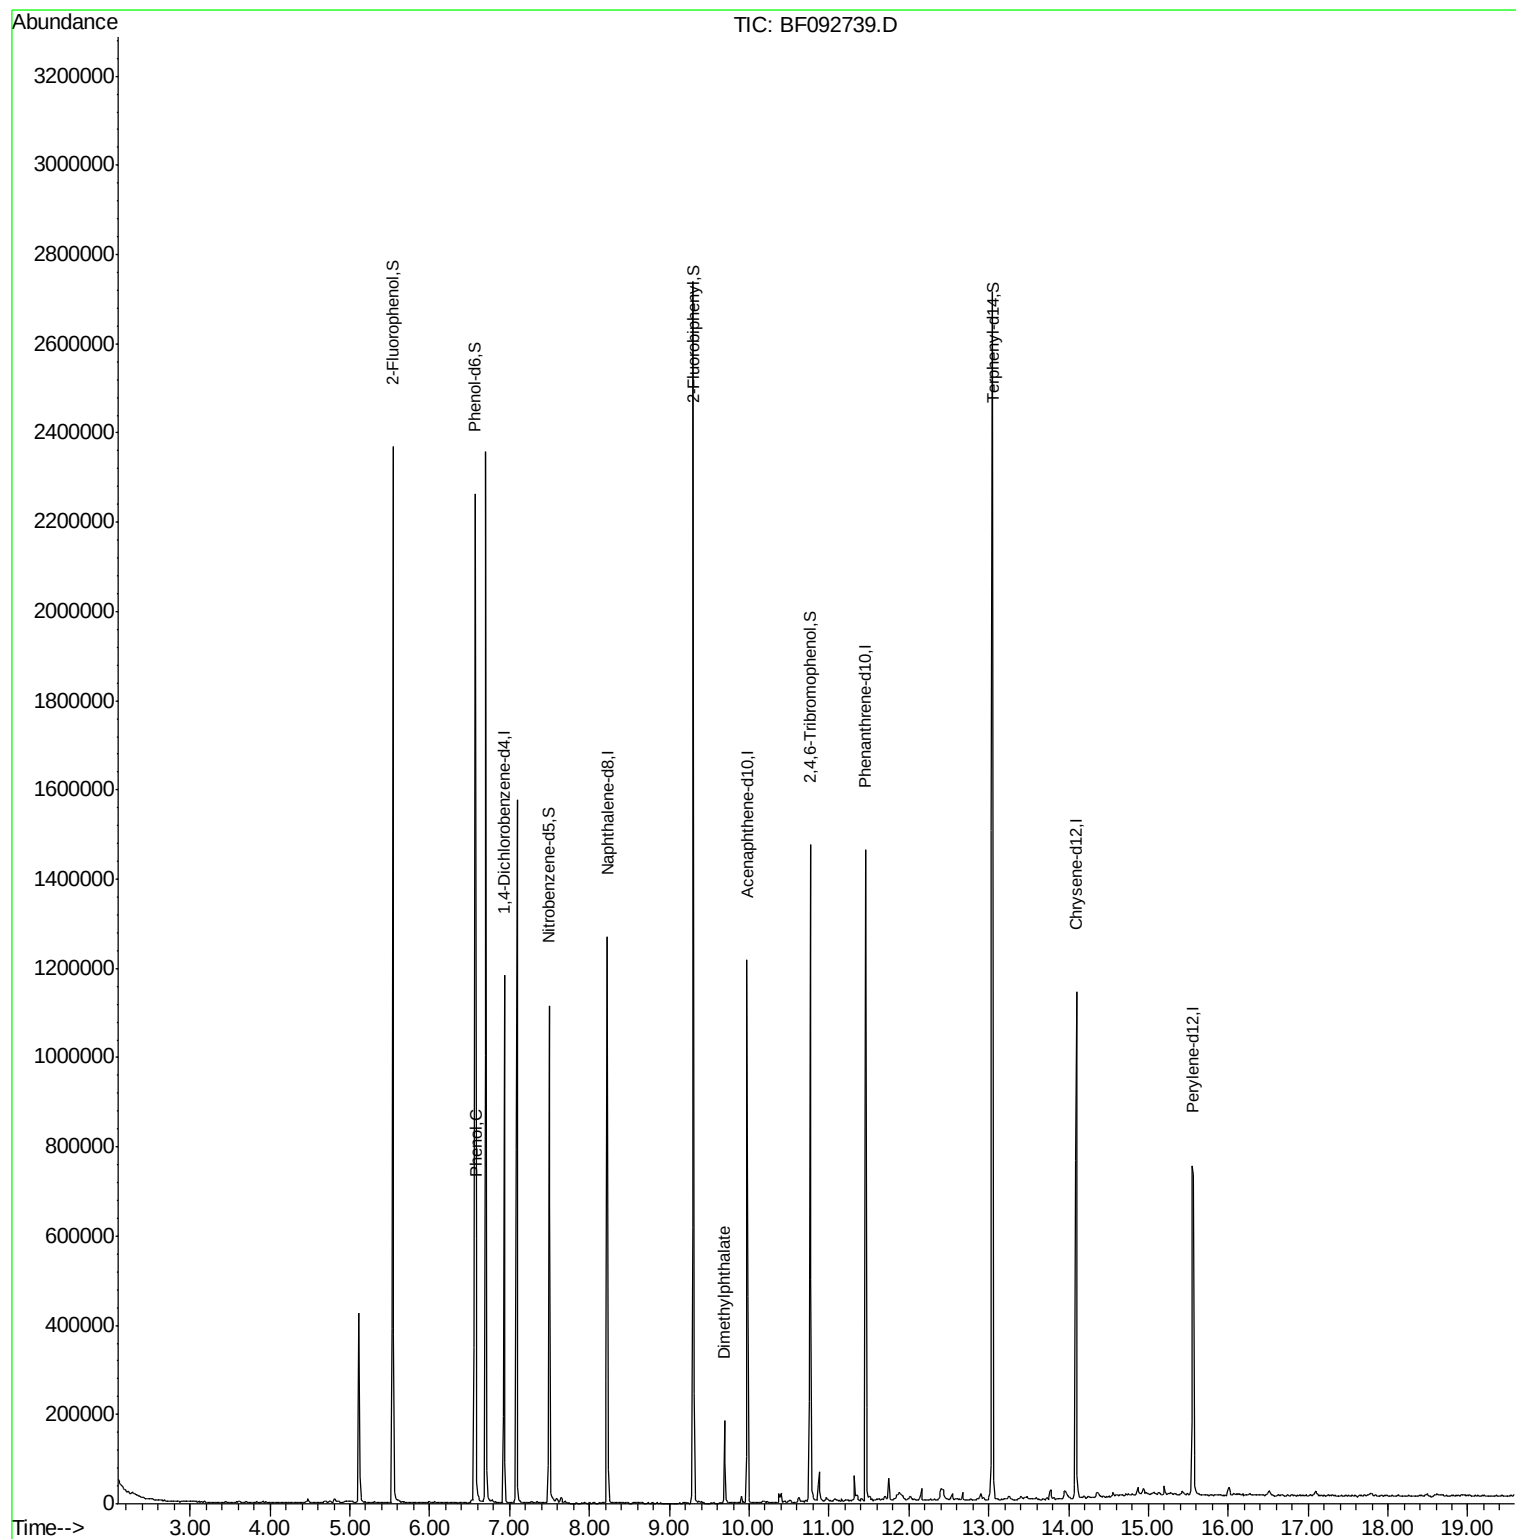

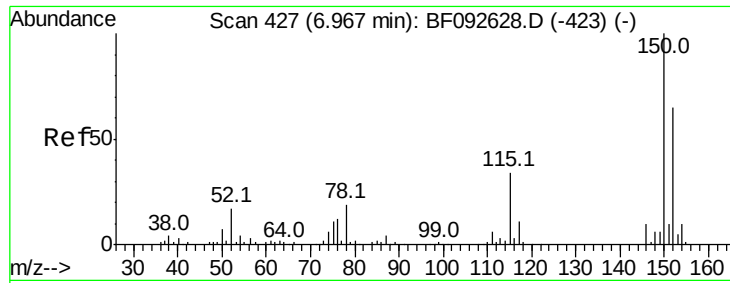

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.93 min Scan# 424

Delta R.T. -0.03 min

Lab File: BF092739.D

Acq: 2 Feb 2017 17:10

Instrument :

BNA_F

ClientSampleId :

ROLL-OFF-275032-COMP-0-2FT


Tot Ion:152 Resp: 162702

Ion Ratio Lower Upper

152 100

150 154.6 124.9 187.3




115 59.3 46.0 69.0

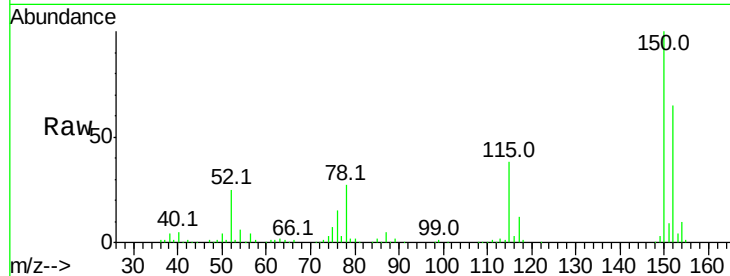

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

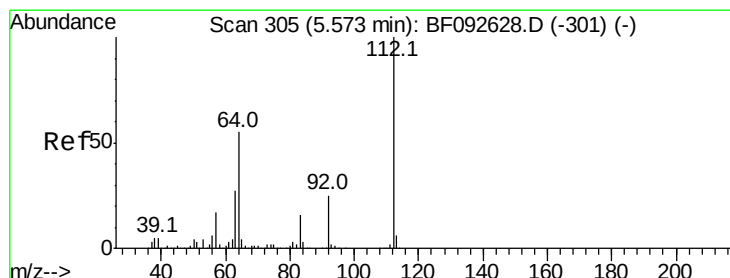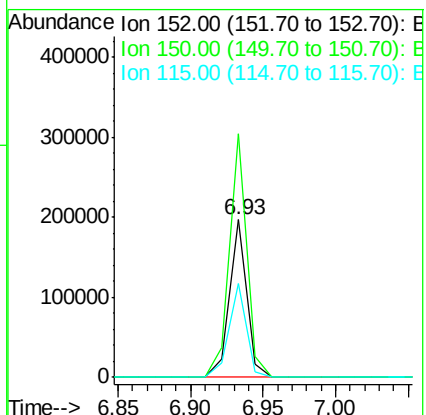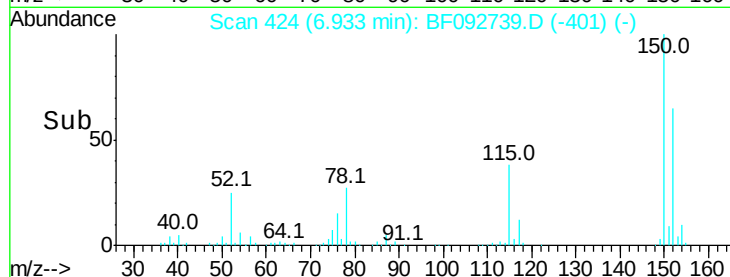

#5

2-Fluorophenol

Concen: 62.80 ng

RT: 5.54 min Scan# 302

Delta R.T. -0.03 min

Lab File: BF092739.D

Acq: 2 Feb 2017 17:10


Tgt Ion:112 Resp: 595605

Ion Ratio Lower Upper

112 100

64 68.1 46.1 69.1



63 33.8 23.8 35.6

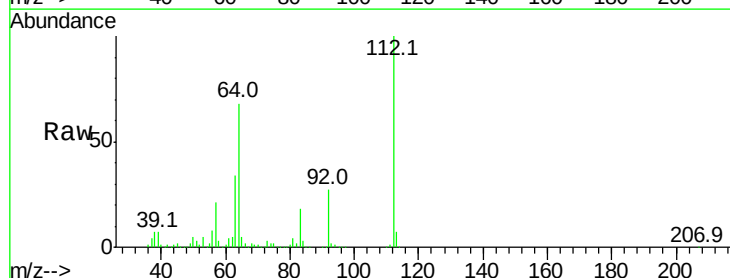


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

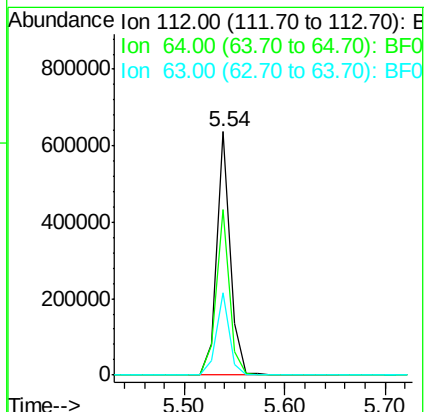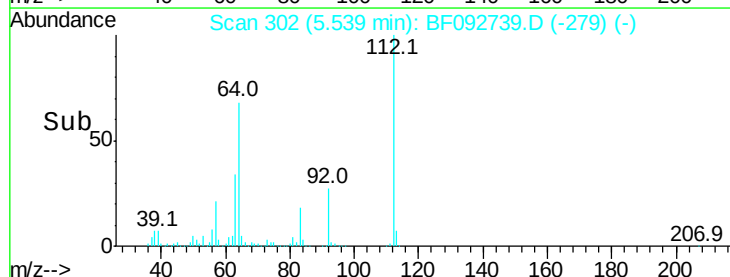

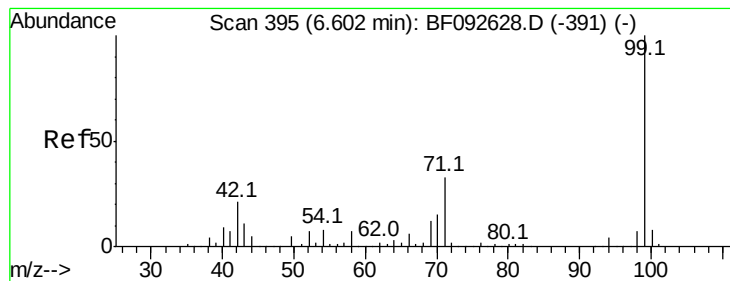

#7

Phenol-d6

Concen: 61.87 ng

RT: 6.57 min Scan# 392

Delta R.T. -0.03 min

Lab File: BF092739.D

Acq: 2 Feb 2017 17:10

Instrument :

BNA_F

ClientSampleId :

ROLL-OFF-275032-COMP-0-2FT


Tot Ion: 99 Resp: 754937

Ion Ratio Lower Upper




99 100

42 21.8 15.6 23.4

71 32.5 27.5 41.3

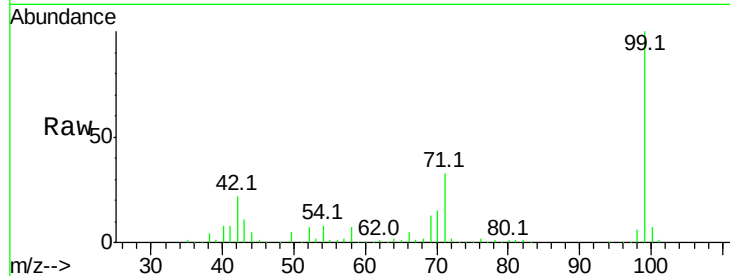

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

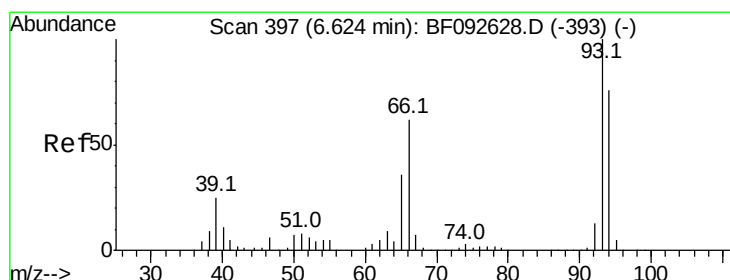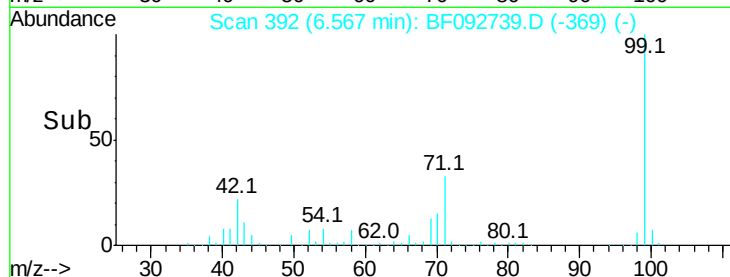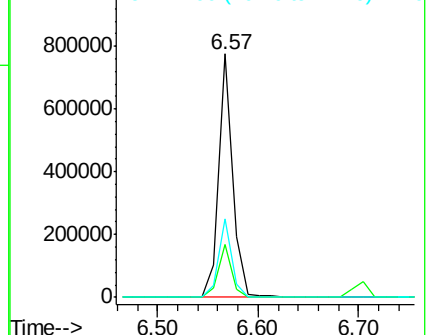

#10

Phenol

Concen: 2.17 ng

RT: 6.58 min Scan# 393

Delta R.T. -0.05 min

Lab File: BF092739.D

Acq: 2 Feb 2017 17:10


Tgt Ion: 94 Resp: 31006

Ion Ratio Lower Upper



94 100


65 34.5 21.4 61.4

66 59.4 44.0 84.0

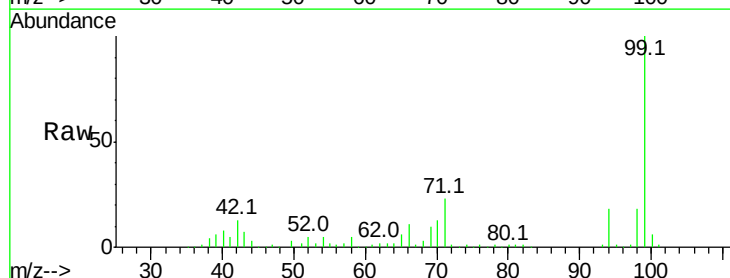

Abundance Ion 94.00 (93.70 to 94.70): BF0
Ion 65.00 (64.70 to 65.70): BF0
Ion 66.00 (65.70 to 66.70): BF0

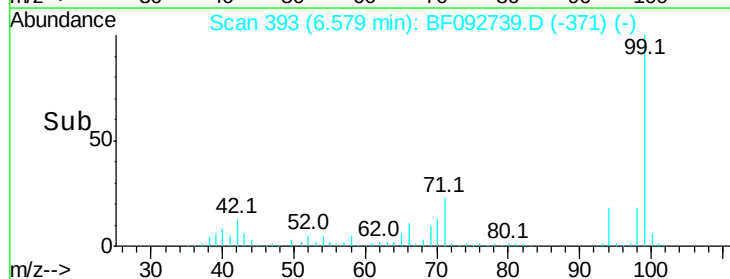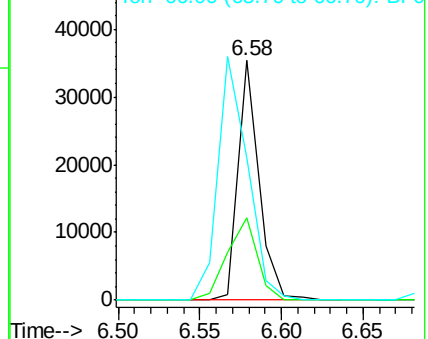


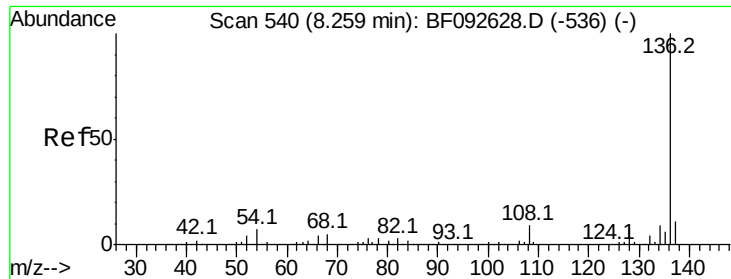




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.22 min Scan# 537
Delta R.T. -0.03 min
Lab File: BF092739.D
Acq: 2 Feb 2017 17:10

Instrument :
BNA_F
ClientSampleId :
ROLL-OFF-275032-COMP-0-2FT

Tot Ion:	136	Resp:	563106
Ion	Ratio	Lower	Upper
136	100		
137	11.2	8.4	12.6
54	9.0	4.5	6.7#
68	6.3	3.6	5.4#

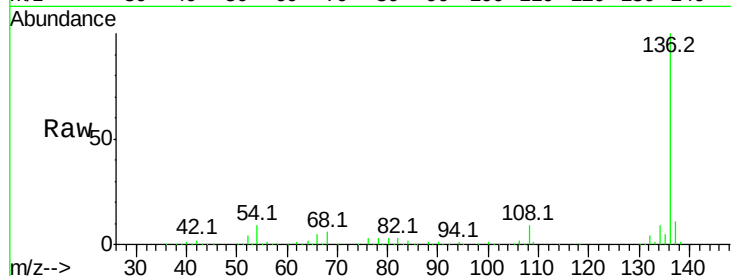


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

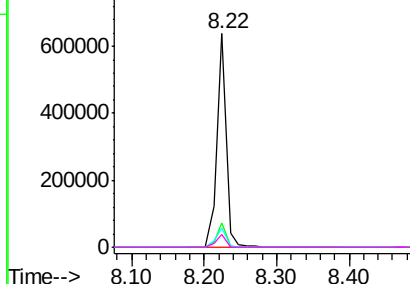




#23
Nitrobenzene-d5
Concen: 44.09 ng
RT: 7.49 min Scan# 473
Delta R.T. -0.05 min
Lab File: BF092739.D
Acq: 2 Feb 2017 17:10

Tgt Ion:	82	Resp:	445805
Ion	Ratio	Lower	Upper
82	100		
128	36.9	34.6	52.0
54	61.5	39.5	59.3#



Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

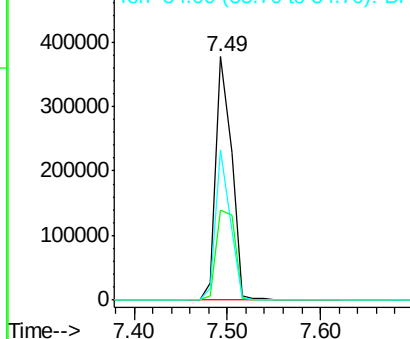







#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.97 min Scan# 690
 Delta R.T. -0.03 min
 Lab File: BF092739.D
 Acq: 2 Feb 2017 17:10

Instrument :
 BNA_F
 ClientSampleId :
 ROLL-OFF-275032-COMP-0-2FT

Tot Ion:164 Resp: 295322
 Ion Ratio Lower Upper
 164 100
 162 103.5 80.2 120.2
 160 44.5 36.9 55.3

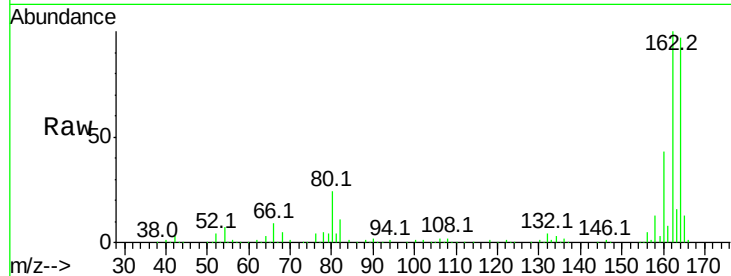


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

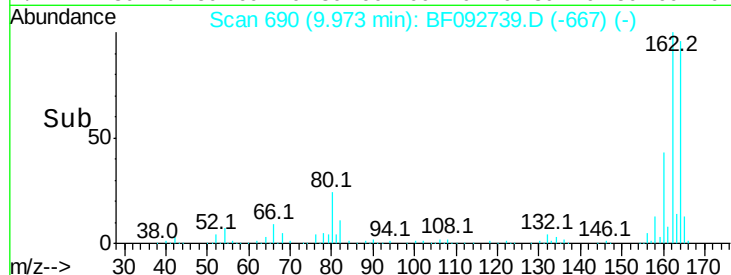
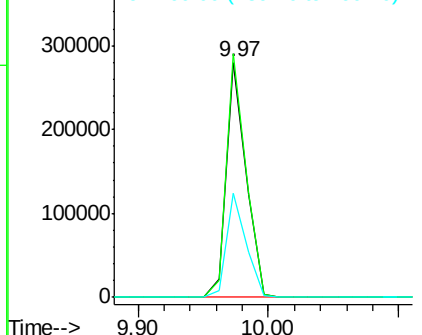



#41
 2,4,6-Tribromophenol
 Concen: 85.50 ng
 RT: 10.76 min Scan# 759
 Delta R.T. -0.05 min
 Lab File: BF092739.D
 Acq: 2 Feb 2017 17:10

Tgt Ion:330 Resp: 182614
 Ion Ratio Lower Upper
 330 100
 332 97.1 77.4 116.2
 141 36.1 34.1 51.1

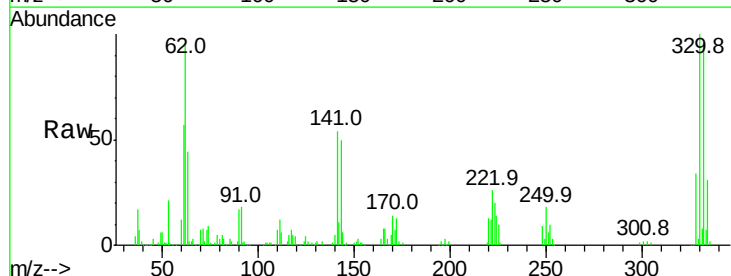

Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

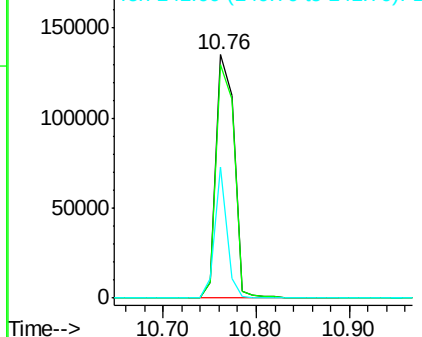



#44

2-Fluorobiphenyl

Concen: 52.94 ng

RT: 9.30 min Scan# 631

Delta R.T. -0.03 min

Lab File: BF092739.D

Acq: 2 Feb 2017 17:10

Instrument :

BNA_F

ClientSampleId :

ROLL-OFF-275032-COMP-0-2FT


Tot Ion:172 Resp: 863043

Ion Ratio Lower Upper

172 100

171 36.2 29.4 44.0




170 23.9 20.2 30.4



Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

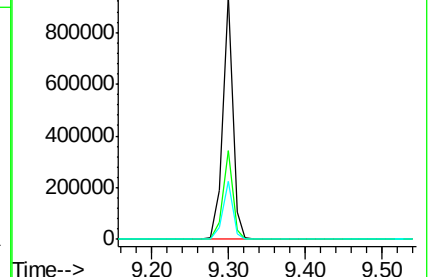

#49

Dimethylphthalate

Concen: 4.77 ng

RT: 9.69 min Scan# 665

Delta R.T. -0.05 min

Lab File: BF092739.D

Acq: 2 Feb 2017 17:10


Tgt Ion:163 Resp: 94794

Ion Ratio Lower Upper

163 100

194 3.4 3.0 4.4



164 9.9 8.0 12.0




Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

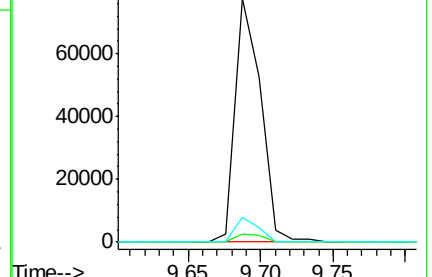


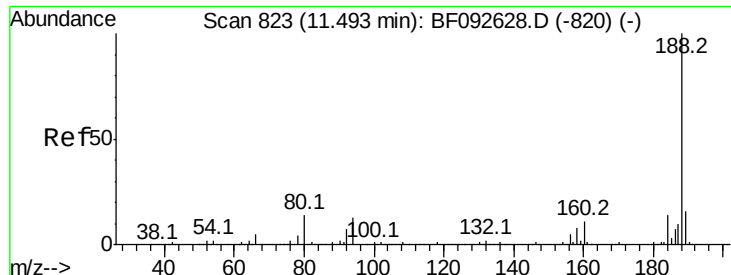




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.46 min Scan# 820
Delta R.T. -0.03 min
Lab File: BF092739.D
Acq: 2 Feb 2017 17:10

Instrument :
BNA_F
ClientSampleId :
ROLL-OFF-275032-COMP-0-2FT

Tot Ion:188 Resp: 509219
Ion Ratio Lower Upper
188 100
94 11.3 10.0 15.0
80 12.2 11.2 16.8

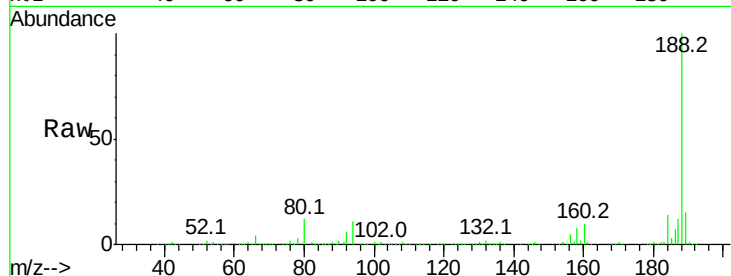


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

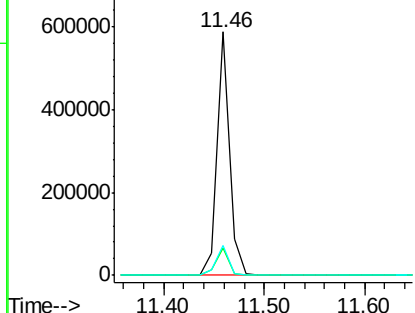




#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.10 min Scan# 1051
Delta R.T. -0.05 min
Lab File: BF092739.D
Acq: 2 Feb 2017 17:10

Tgt Ion:240 Resp: 494720
Ion Ratio Lower Upper
240 100
120 9.1 12.9 19.3#
236 26.2 20.9 31.3



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

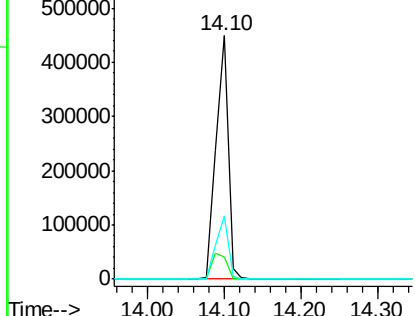



#78

Terphenyl-d14

Concen: 46.99 ng

RT: 13.05 min Scan# 959

Delta R.T. -0.03 min

Lab File: BF092739.D

Acq: 2 Feb 2017 17:10

Instrument :

BNA_F

ClientSampleId :

ROLL-OFF-275032-COMP-0-2FT


Tot Ion:244 Resp: 989418

Ion Ratio Lower Upper

244 100

212 7.0 6.2 9.2




122 9.1 11.4 17.2#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

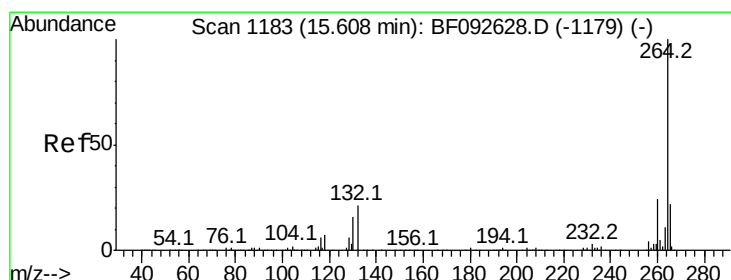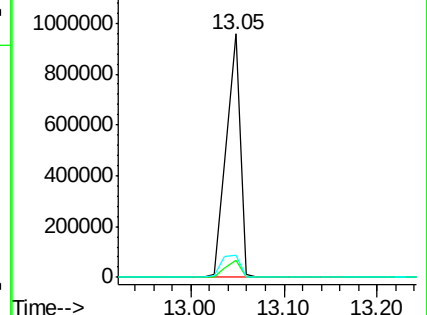

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.56 min Scan# 1179

Delta R.T. -0.05 min

Lab File: BF092739.D

Acq: 2 Feb 2017 17:10


Tgt Ion:264 Resp: 426020

Ion Ratio Lower Upper

264 100

260 23.7 19.2 28.8

265 20.9 17.4 26.0



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

