


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF020217\  
 Data File : BF092735.D  
 Acq On : 2 Feb 2017 15:00  
 Operator : SJ/MA  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF013017.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Jan 30 14:50:05 2017

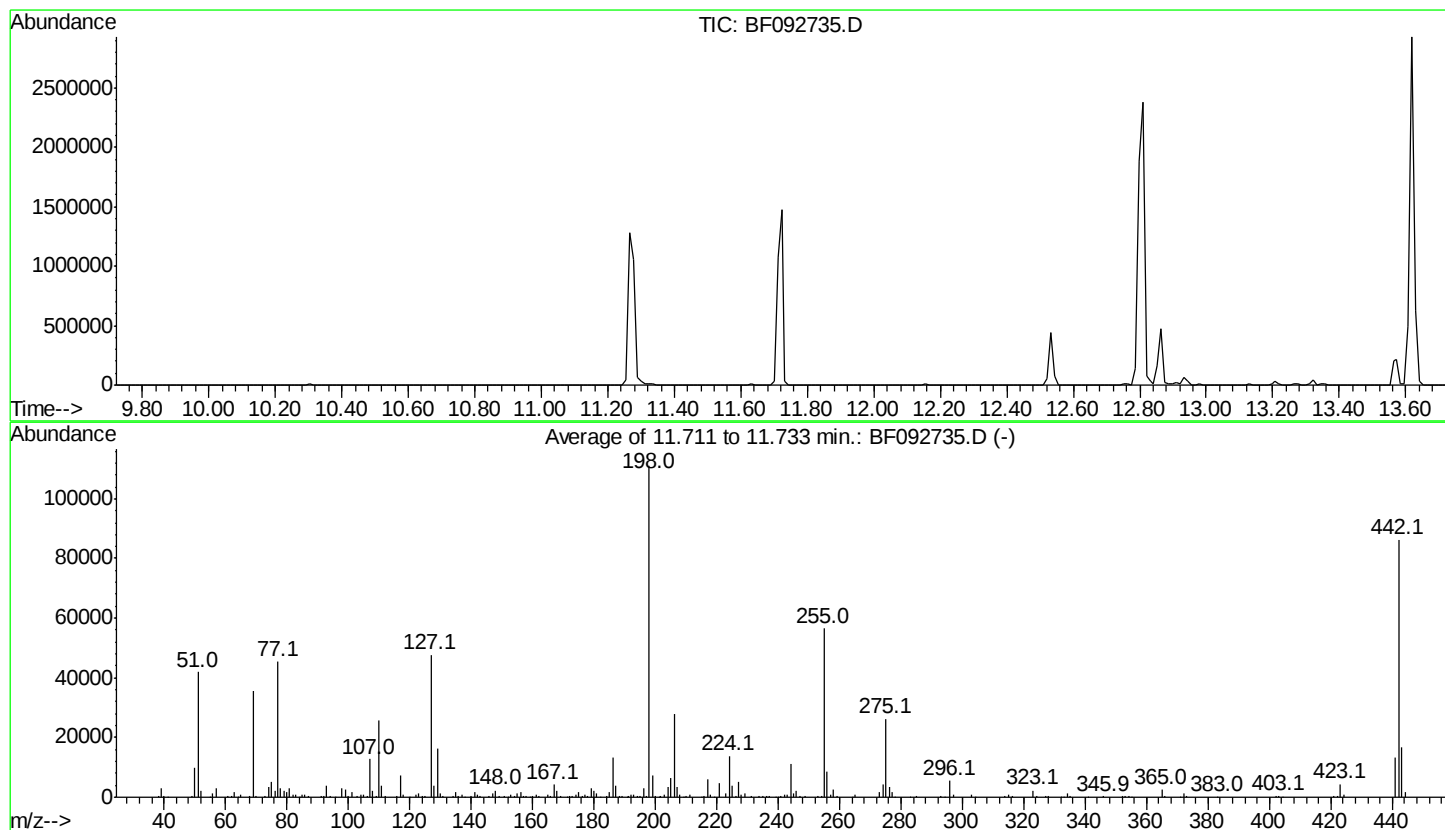

AutoFind: Scans 842, 843, 844; Background Corrected with Scan 838

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 37.7      | 41929   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.8       | 640     | PASS             |
| 69          | 198          | 0.00         | 100          | 32.0      | 35510   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.7       | 251     | PASS             |
| 127         | 198          | 10           | 80           | 43.0      | 47766   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.4       | 478     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 111095  | PASS             |
| 199         | 198          | 5            | 9            | 6.6       | 7364    | PASS             |
| 275         | 198          | 10           | 60           | 23.6      | 26261   | PASS             |
| 365         | 198          | 1            | 100          | 2.2       | 2406    | PASS             |
| 441         | 442          | 0.01         | 24           | 15.5      | 13380   | PASS             |
| 442         | 198          | 50           | 100          | 77.8      | 86403   | PASS             |
| 443         | 442          | 15           | 24           | 19.2      | 16613   | PASS             |