


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020217\
 Data File : BF092761.D
 Acq On : 3 Feb 2017 4:34
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 30 14:50:05 2017

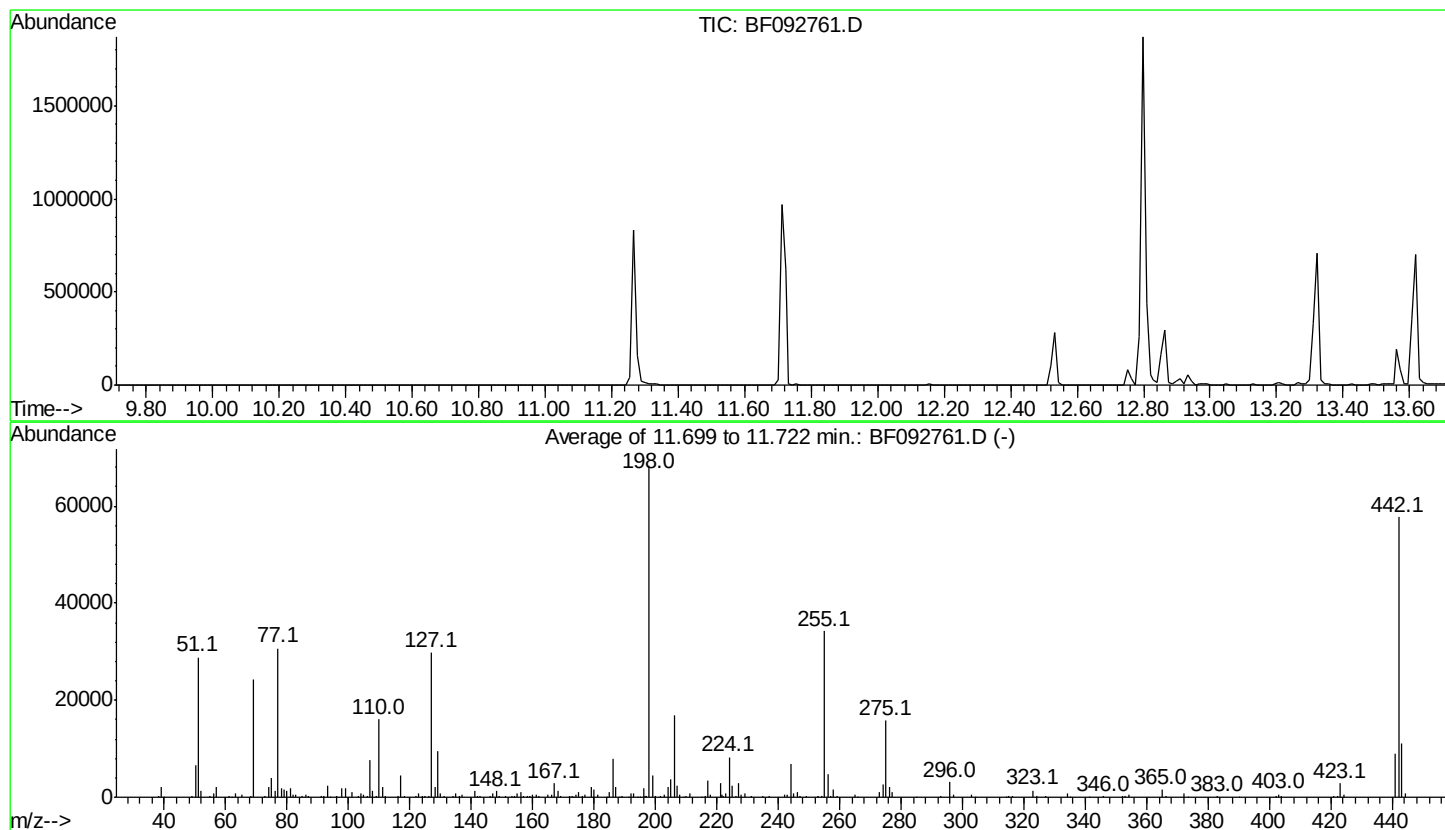

AutoFind: Scans 841, 842, 843; Background Corrected with Scan 838

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.3	28882	PASS
68	69	0.00	2	1.5	371	PASS
69	198	0.00	100	35.4	24153	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.5	29697	PASS
197	198	0.00	2	0.5	374	PASS
198	198	100	100	100.0	68313	PASS
199	198	5	9	6.6	4479	PASS
275	198	10	60	23.1	15800	PASS
365	198	1	100	2.2	1522	PASS
441	442	0.01	24	15.7	9052	PASS
442	198	50	100	84.4	57640	PASS
443	442	15	24	19.3	11113	PASS