
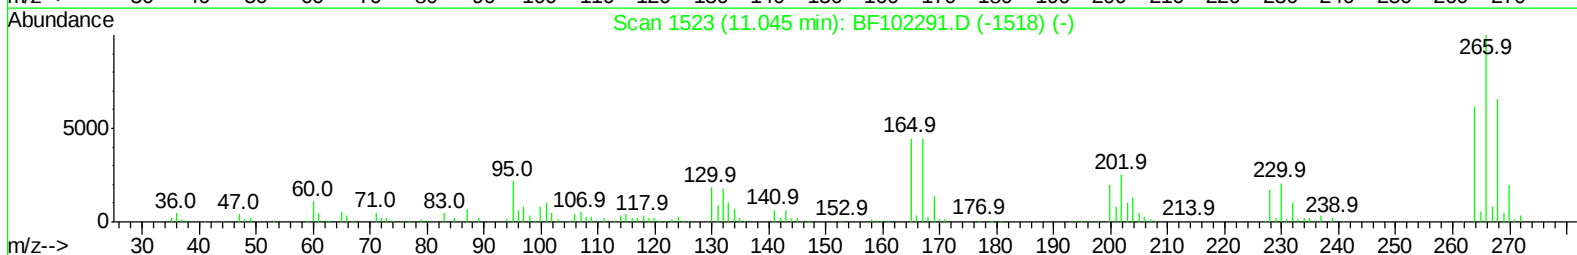
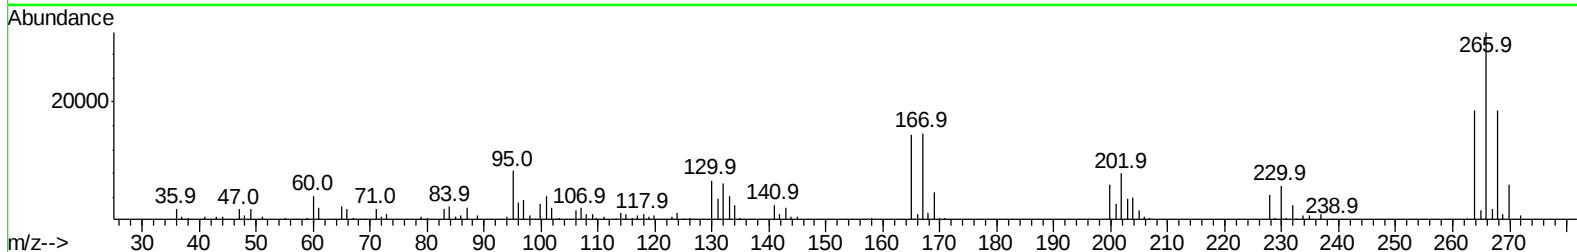


Data Path : U:\HPCHEM1\BNA F\Data\BF020218\
Data File : BF102700.D
Acq On : 2 Feb 2018 11:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 02 23:21:45 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 18:38:00 2018
Response via : Initial Calibration

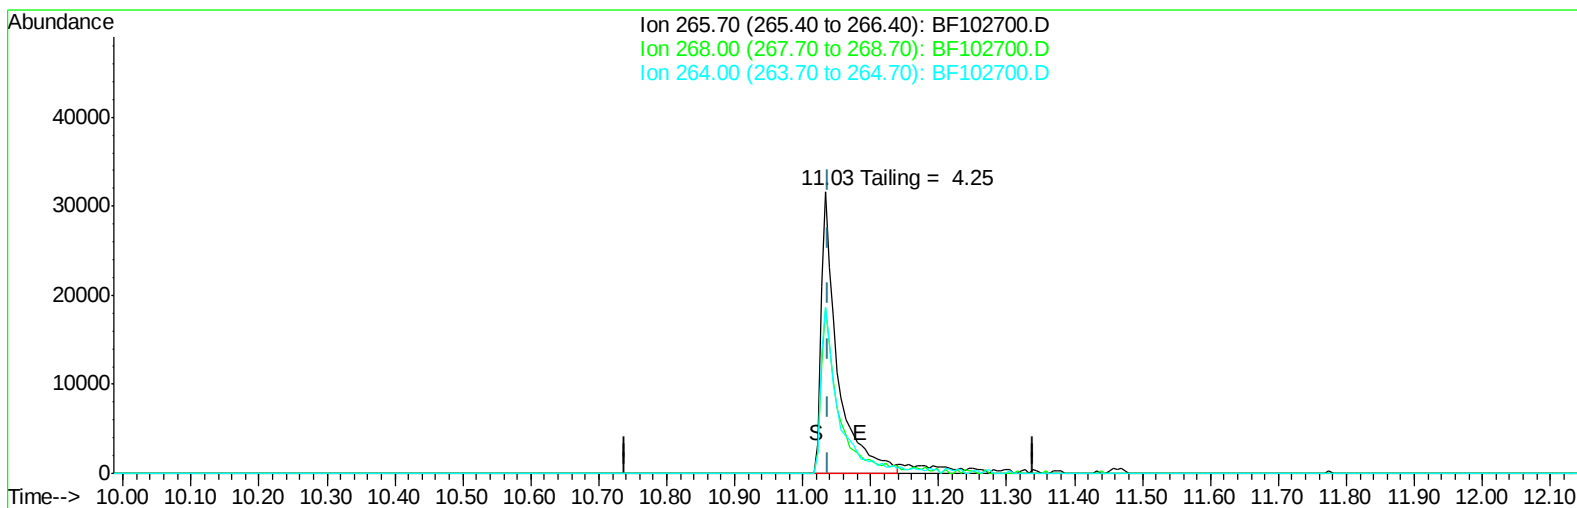

TIC: BF102700.D

(69) Pentachlorophenol (C)




11.033min (-0.006) 56591.83ng

response 54045

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	58.82
264.00	61.90	58.92
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\Data\BF020218\
Data File : BF102700.D
Acq On : 2 Feb 2018 11:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 02 23:21:45 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 18:38:00 2018
Response via : Initial Calibration

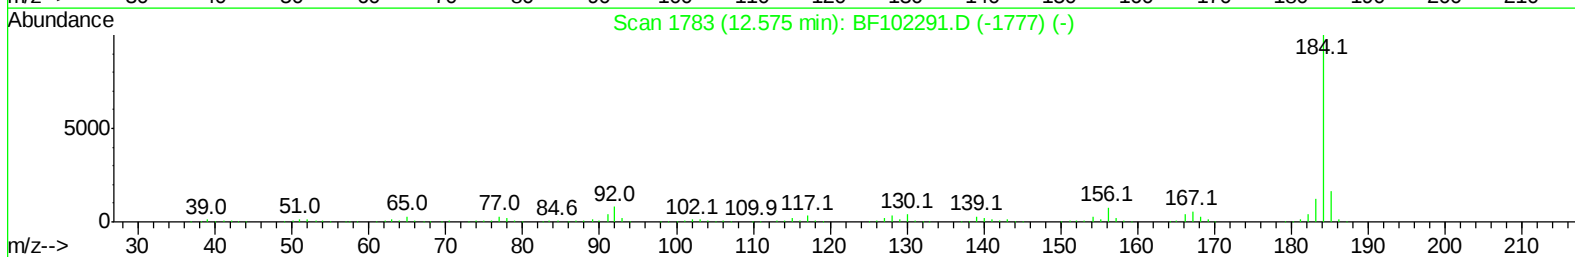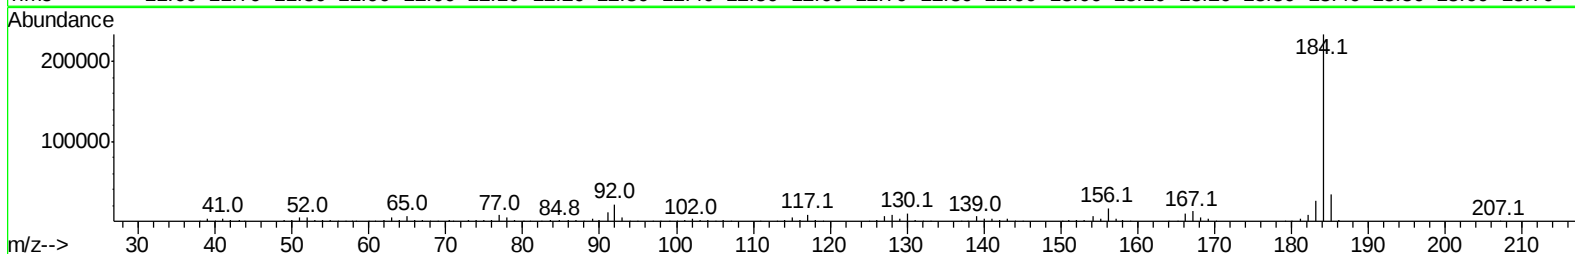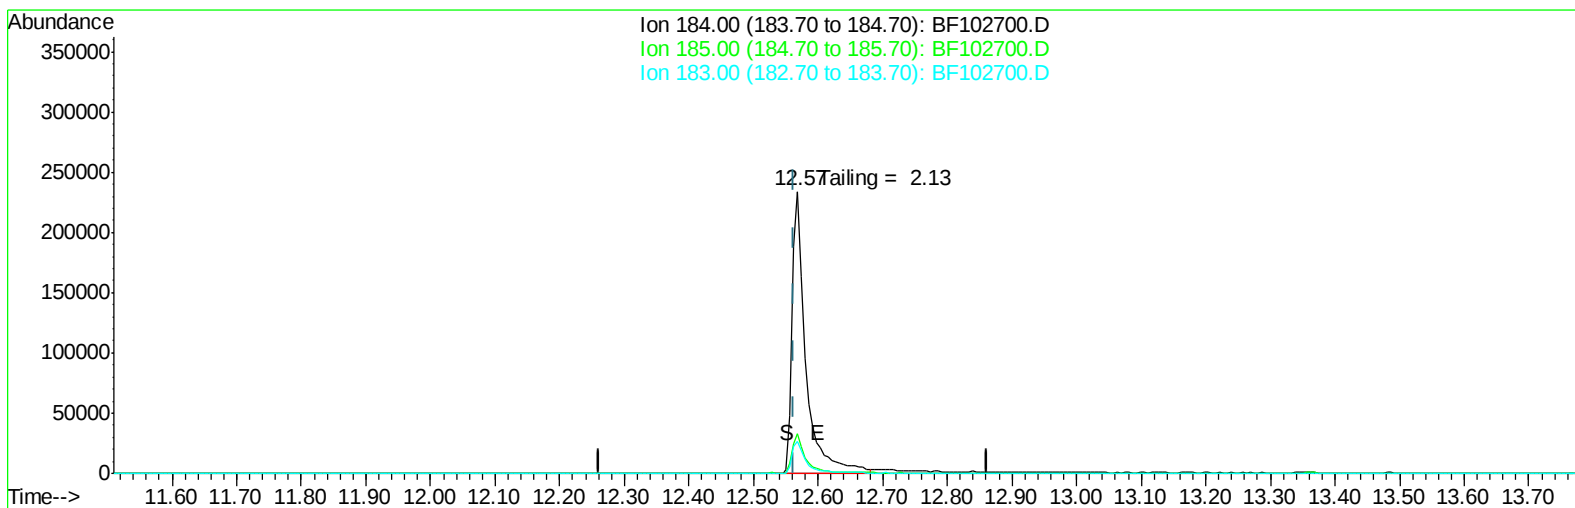

TIC: BF102700.D

(76) Benzidine

12.569min (+0.006) 0.00ng

response 359051

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.19
183.00	11.60	11.23
0.00	0.00	0.00