


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020218\
 Data File : BF102700.D
 Acq On : 2 Feb 2018 11:10
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 31 18:38:00 2018

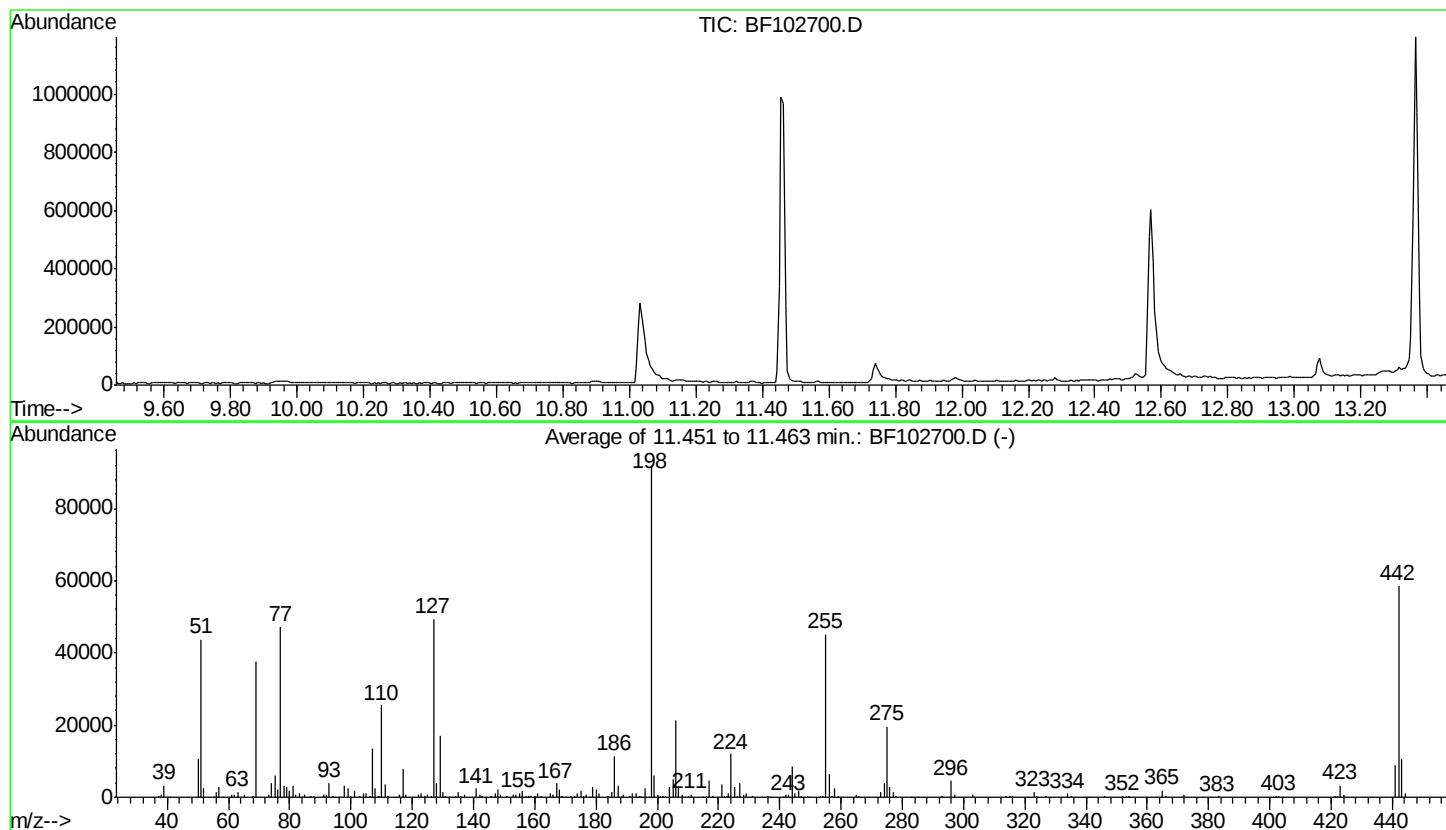

AutoFind: Scans 1592, 1593, 1594; Background Corrected with Scan 1587

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.5	43700	PASS
68	69	0.00	2	1.2	468	PASS
69	198	0.00	100	41.0	37647	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.8	49456	PASS
197	198	0.00	2	0.2	153	PASS
198	198	100	100	100.0	91904	PASS
199	198	5	9	6.5	6017	PASS
275	198	10	60	21.3	19546	PASS
365	198	1	100	2.1	1899	PASS
441	443	0.01	100	83.6	8963	PASS
442	198	50	100	63.7	58543	PASS
443	442	15	24	18.3	10724	PASS