


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020222\
 Data File : BF126777.D
 Acq On : 02 Feb 2022 10:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 02 15:08:47 2022

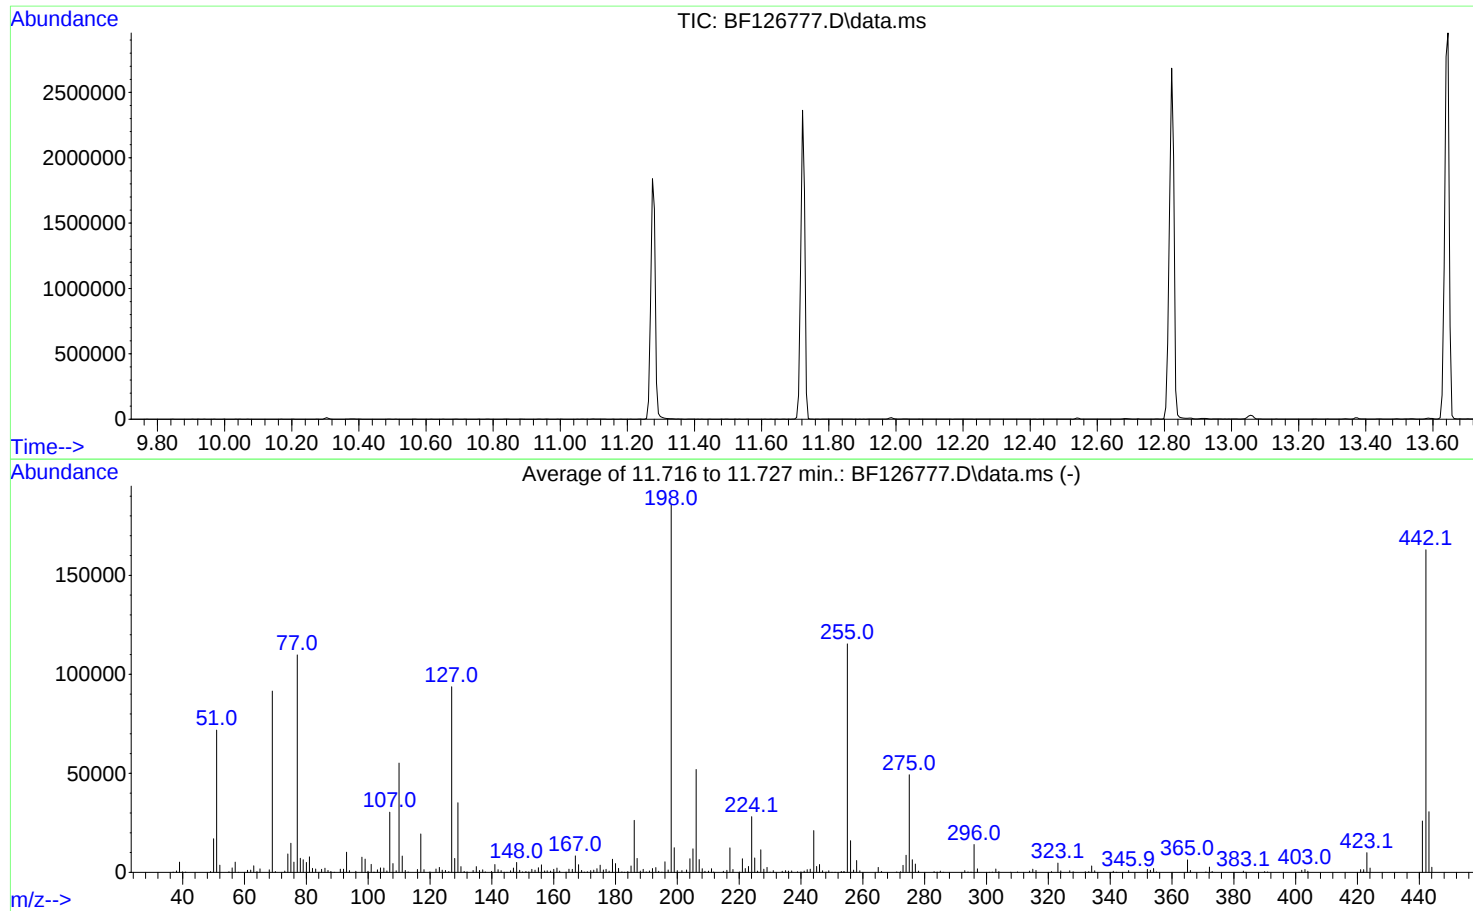




AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	71845	PASS
68	69	0.00	2	1.4	1327	PASS
69	198	0.00	100	49.3	91533	PASS
70	69	0.00	2	0.4	403	PASS
127	198	10	80	50.5	93771	PASS
197	198	0.00	2	0.7	1243	PASS
198	198	100	100	100.0	185776	PASS
199	198	5	9	6.7	12423	PASS
275	198	10	60	26.5	49299	PASS
365	198	1	100	3.4	6343	PASS
441	198	0.01	100	14.0	25960	PASS
442	442	50	100	100.0	162920	PASS
443	442	15	24	18.8	30629	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020222\
Data File : BF126777.D
Acq On : 02 Feb 2022 10:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 02 14:25:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 02 14:18:53 2022
Response via : Initial Calibration

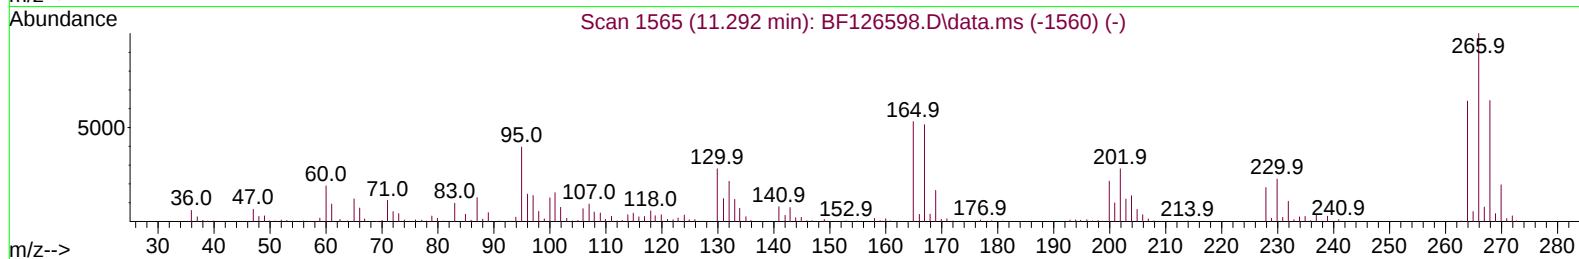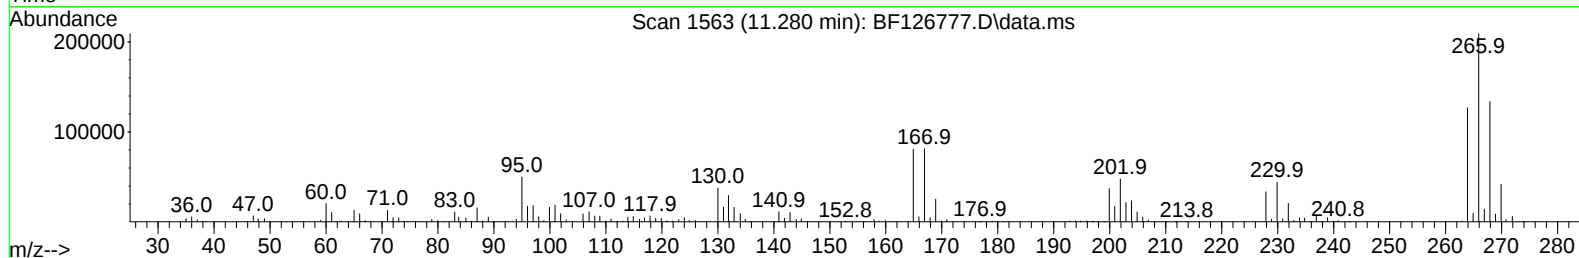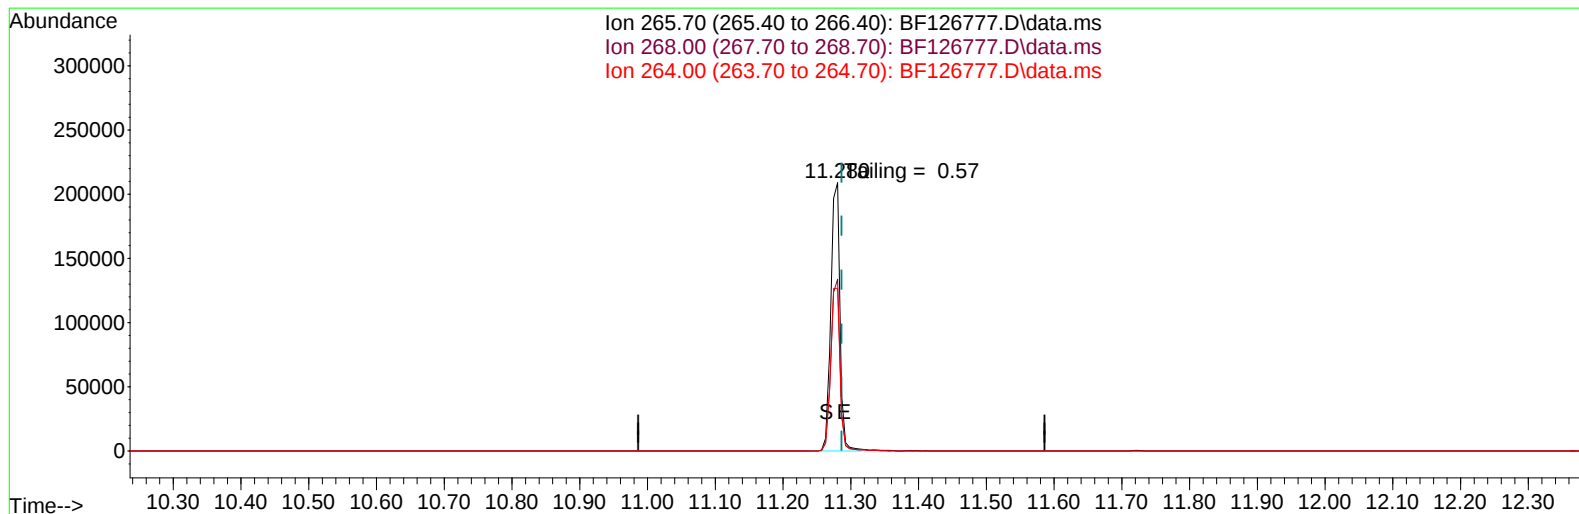

TIC: BF126777.D\data.ms

(70) Pentachlorophenol (C)

11.280min (-0.006) 37839.04 ng




response 196698

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	64.02
264.00	63.00	60.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020222\
Data File : BF126777.D
Acq On : 02 Feb 2022 10:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 02 14:25:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 02 14:18:53 2022
Response via : Initial Calibration

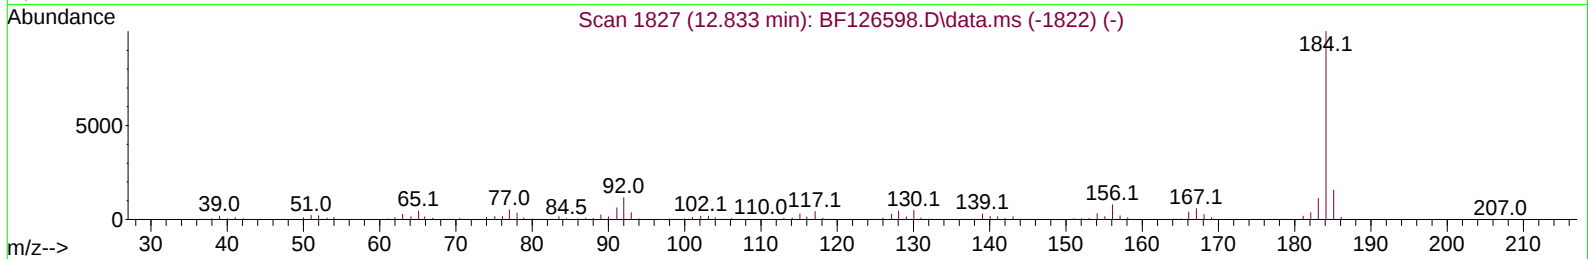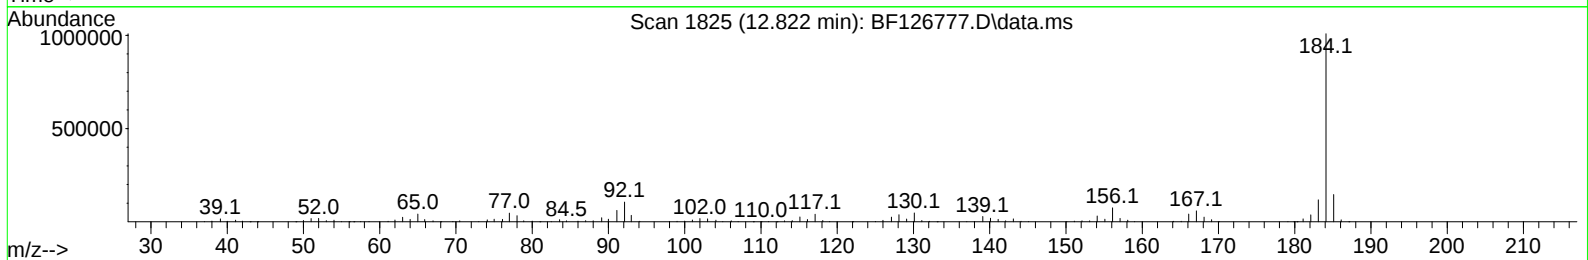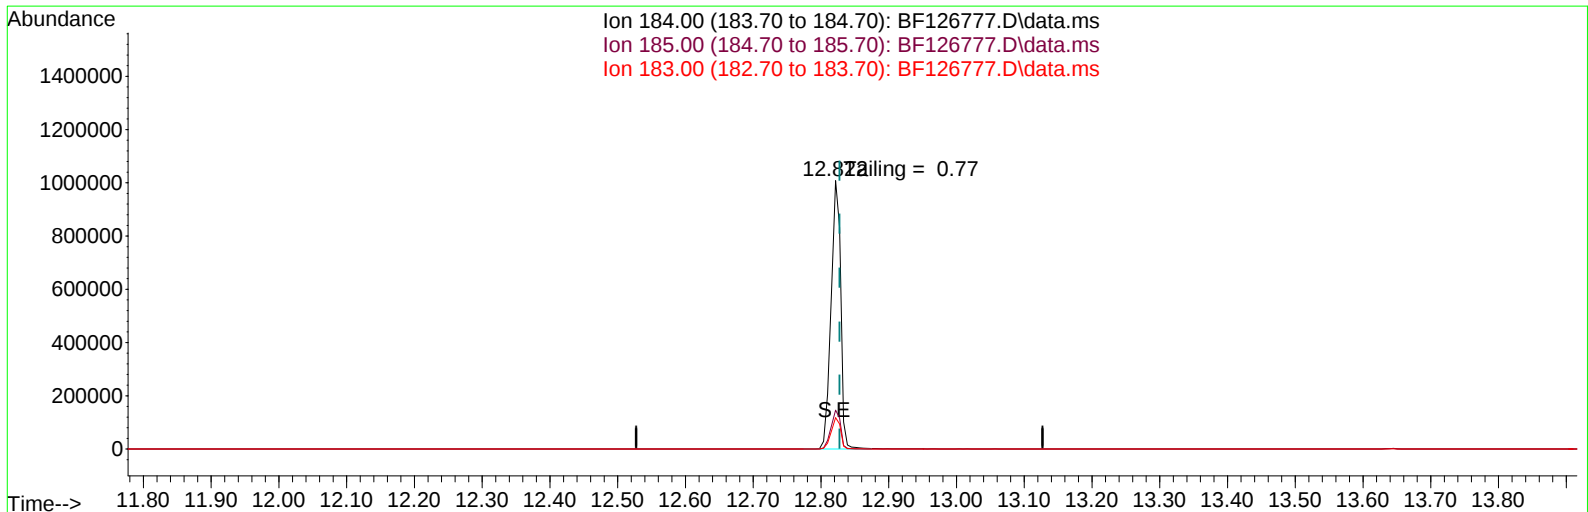

TIC: BF126777.D\data.ms

(77) Benzidine

12.822min (-0.006) 0.00 ng

response 998151

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.53
183.00	10.20	11.72
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/2/2022	BNA_F	<u>BF126777.D</u>
Compound Name	Response	Retention Time
DDT	533990	13.64
DDD	2521	13.37
DDE	110	13.06
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2631	536621	0.49