
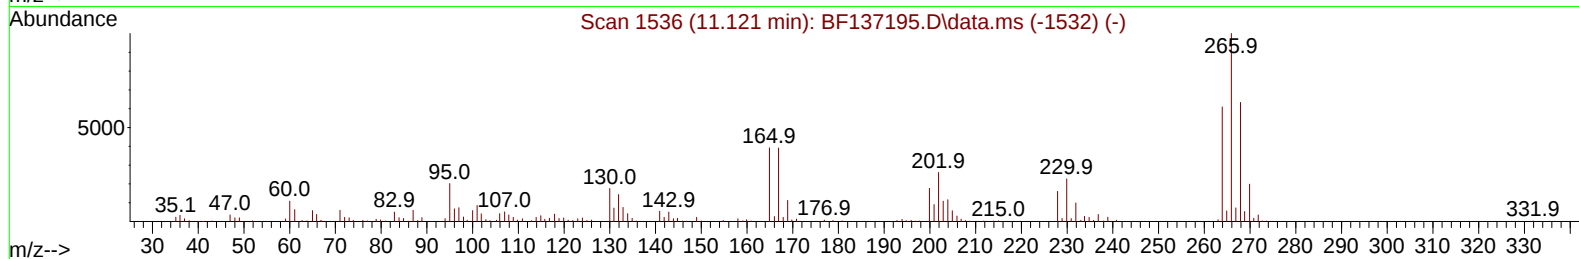
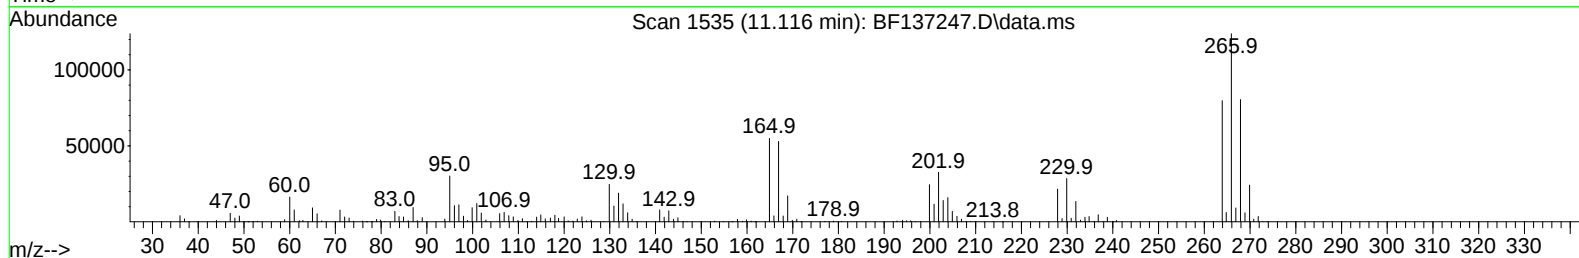


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020224\
Data File : BF137247.D
Acq On : 02 Feb 2024 09:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 02 11:41:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 04:56:22 2024
Response via : Initial Calibration

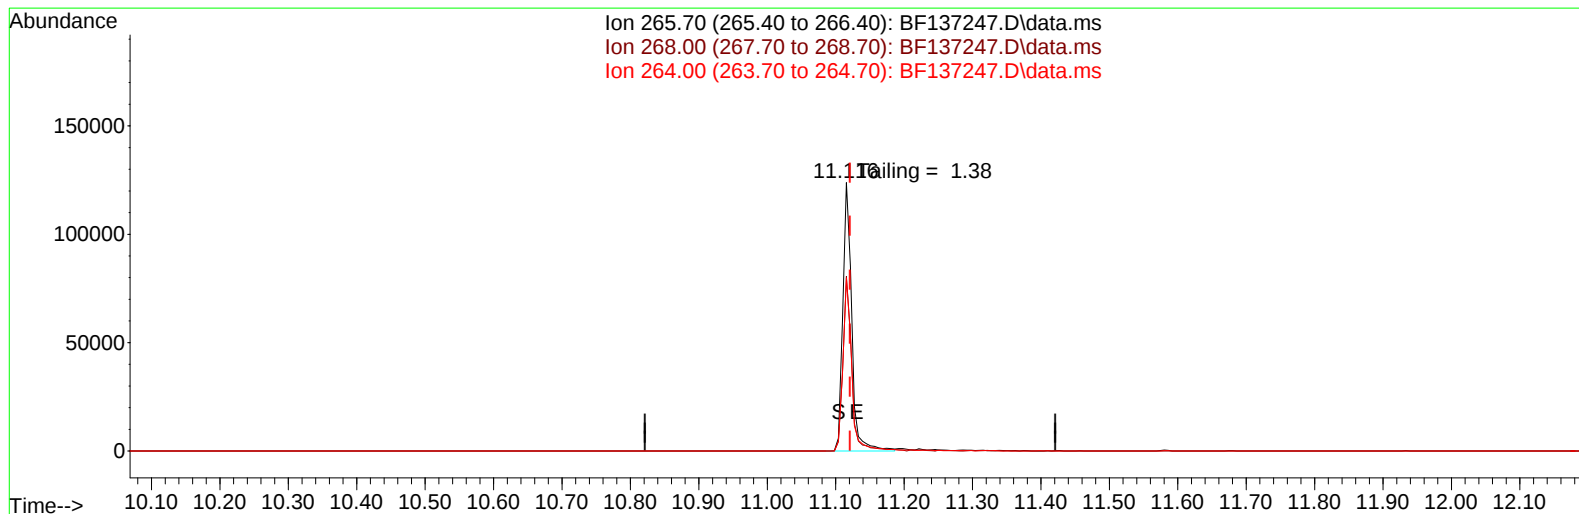

TIC: BF137247.D\data.ms

(70) Pentachlorophenol (C)




11.116min (-0.005) 35015.20 ng

response 112910

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	65.03
264.00	61.00	64.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020224\
Data File : BF137247.D
Acq On : 02 Feb 2024 09:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 02 11:41:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 04:56:22 2024
Response via : Initial Calibration

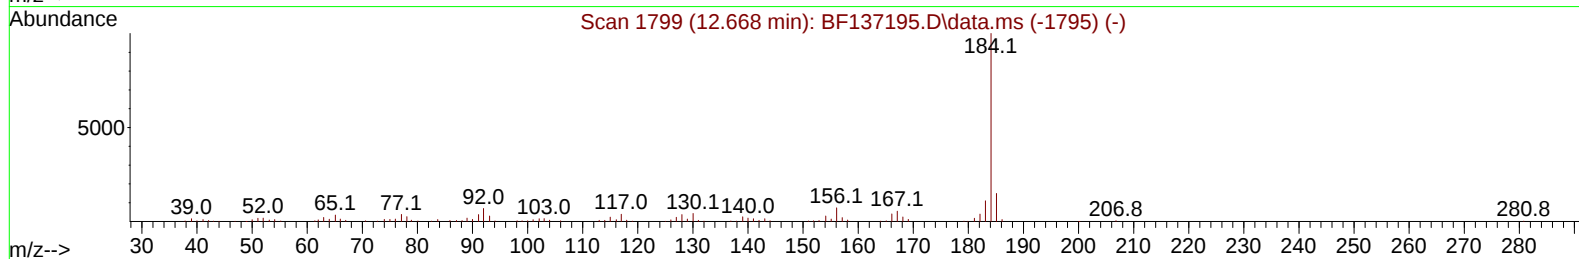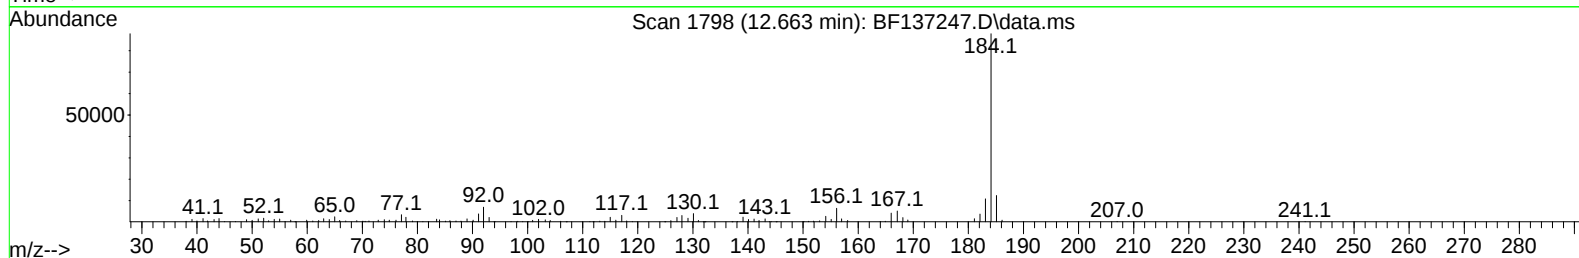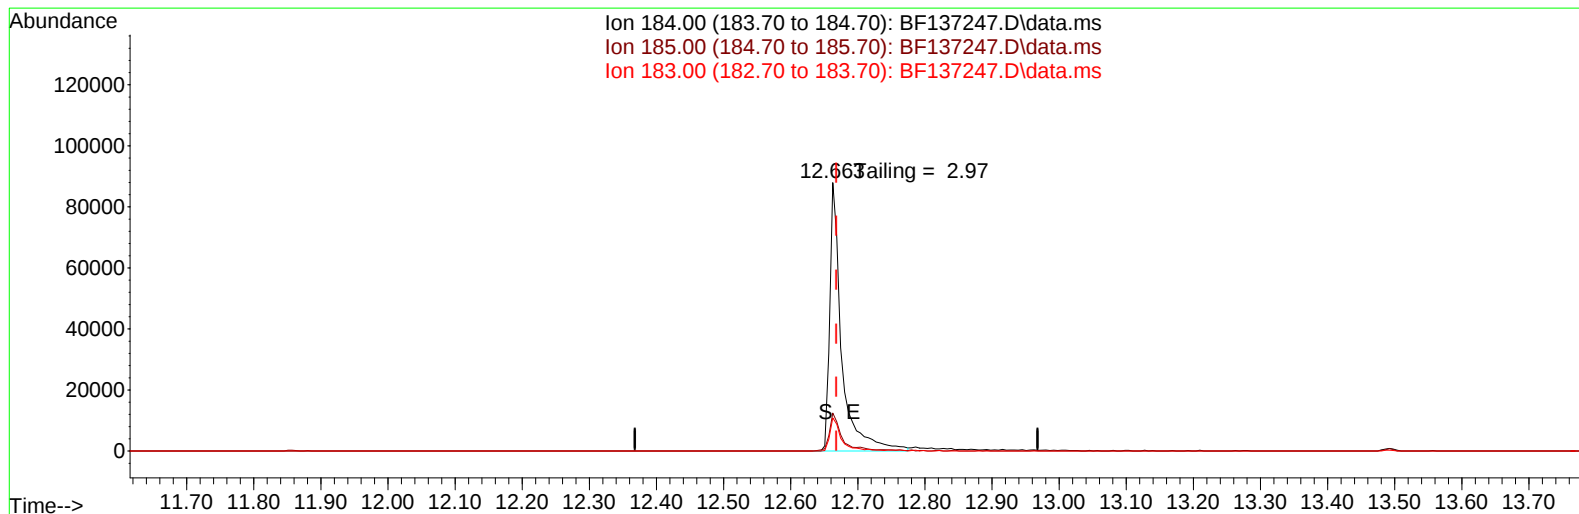

TIC: BF137247.D\data.ms

(77) Benzidine

12.663min (-0.005) 0.00 ng m

response 109077

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.15
183.00	11.00	12.35
0.00	0.00	0.00