

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020224\
 Data File : BF137260.D
 Acq On : 02 Feb 2024 17:47
 Operator : CG\JU
 Sample : P1337-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-5

Quant Time: Feb 02 22:43:27 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 04:56:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.792	152	51336	20.000	ng	0.00
21) Naphthalene-d8	8.069	136	198214	20.000	ng	0.00
39) Acenaphthene-d10	9.822	164	108863	20.000	ng	0.00
64) Phenanthrene-d10	11.310	188	174364	20.000	ng	0.00
76) Chrysene-d12	13.963	240	140049	20.000	ng	-0.01
86) Perylene-d12	15.445	264	107800	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.422	112	357819	115.013	ng	0.00
7) Phenol-d6	6.422	99	451906	101.783	ng	0.00
23) Nitrobenzene-d5	7.351	82	294849	66.599	ng	0.00
42) 2,4,6-Tribromophenol	10.610	330	115732	94.133	ng	-0.01
45) 2-Fluorobiphenyl	9.145	172	525187	66.318	ng	0.00
79) Terphenyl-d14	12.910	244	508044	49.315	ng	-0.01


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020224\
Data File : BF137260.D
Acq On : 02 Feb 2024 17:47
Operator : CG\JU
Sample : P1337-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-5

Quant Time: Feb 02 22:43:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 04:56:22 2024
Response via : Initial Calibration




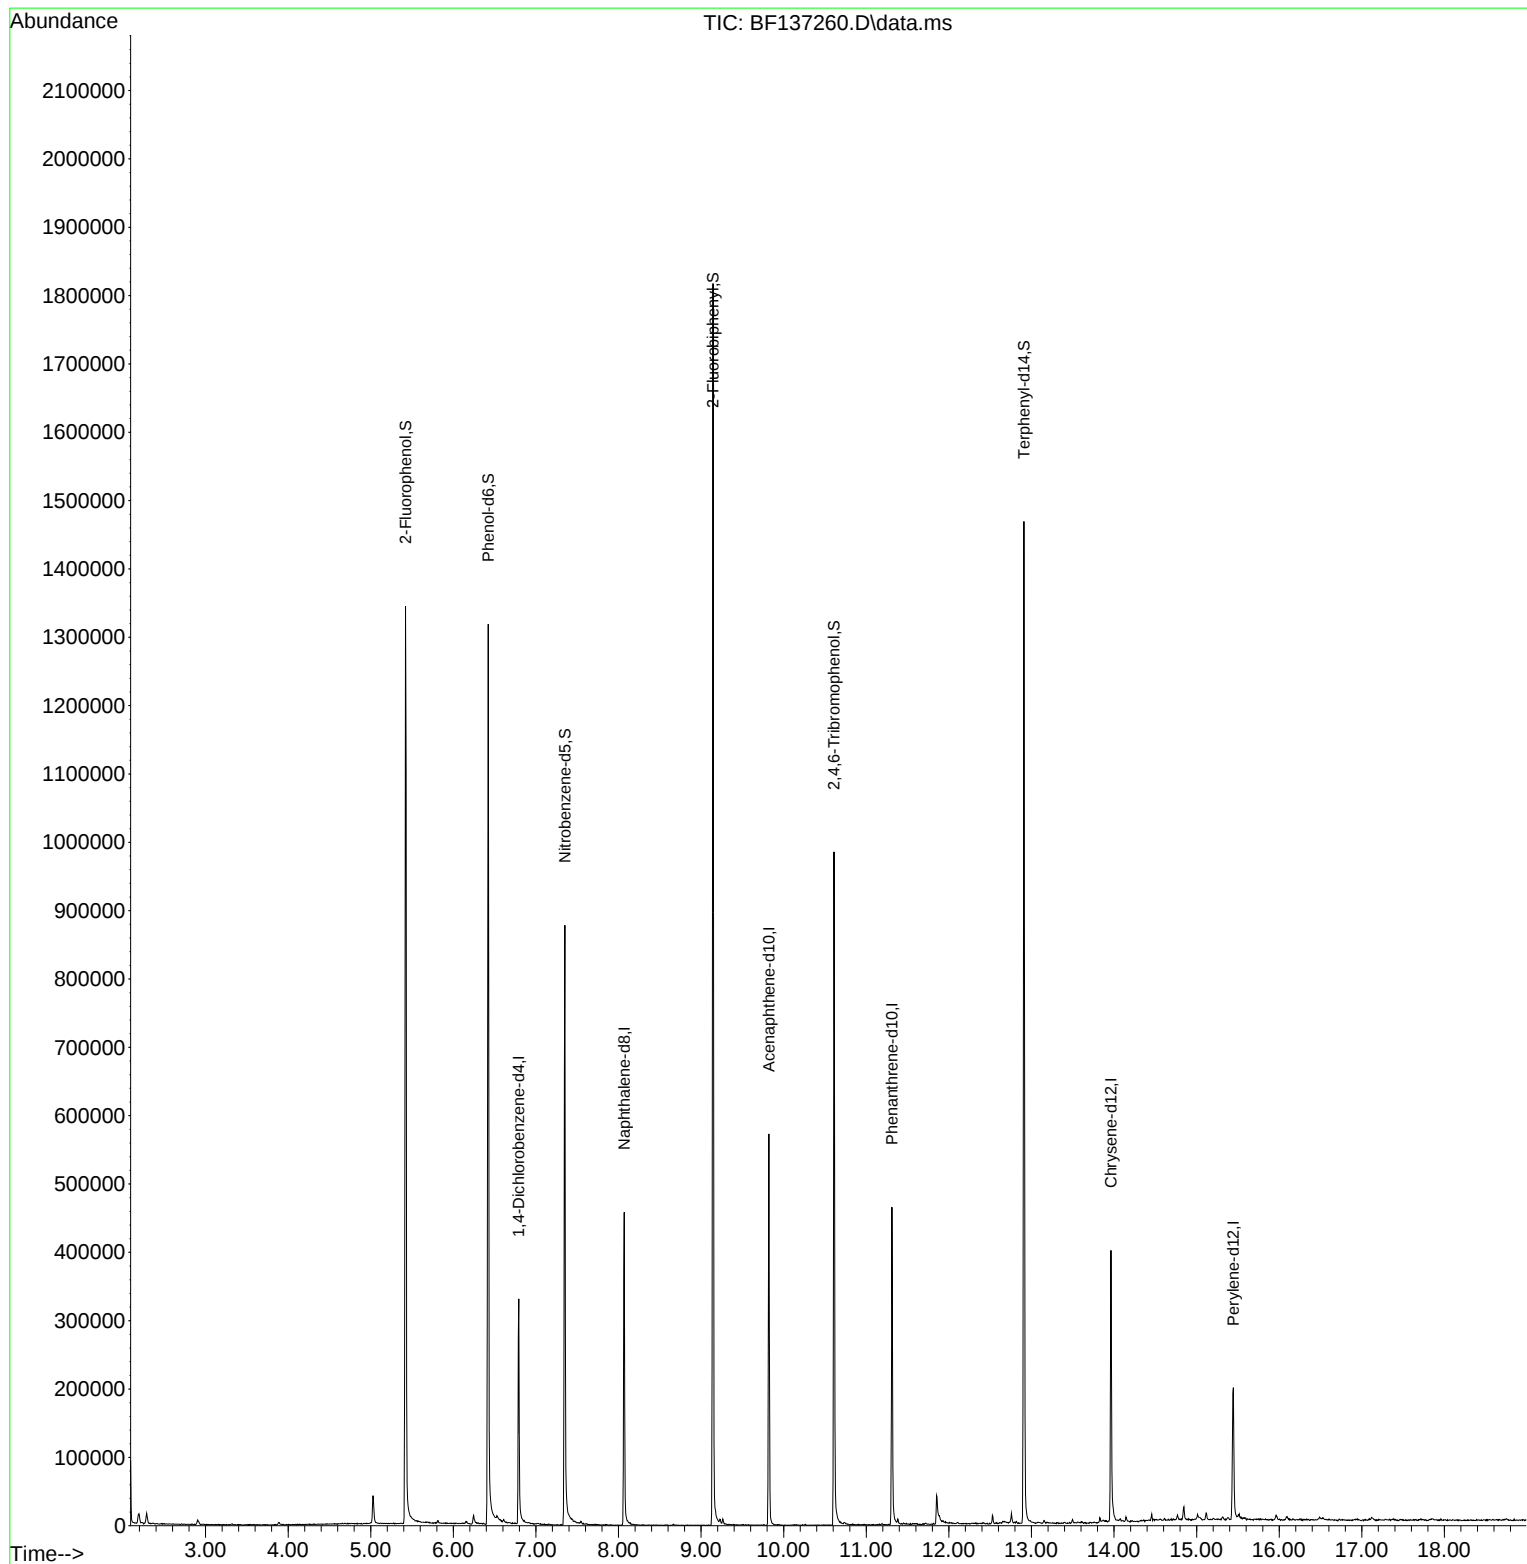


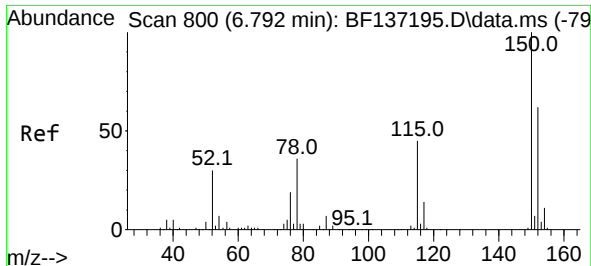

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.792 min Scan# 800
 Delta R.T. 0.000 min
 Lab File: BF137260.D
 Acq: 02 Feb 2024 17:47




Instrument :
 BNA_F
 ClientSampleId :
 TP-5


Tgt Ion:152 Resp: 51336
 Ion Ratio Lower Upper
 152 100
 150 155.6 129.8 194.8
 115 62.1 58.5 87.7

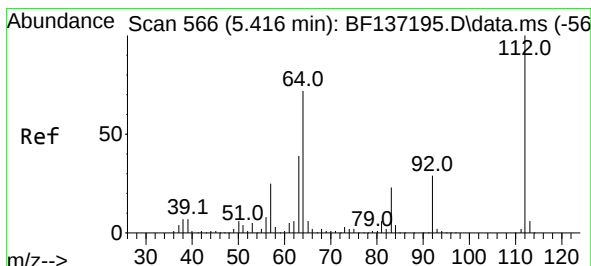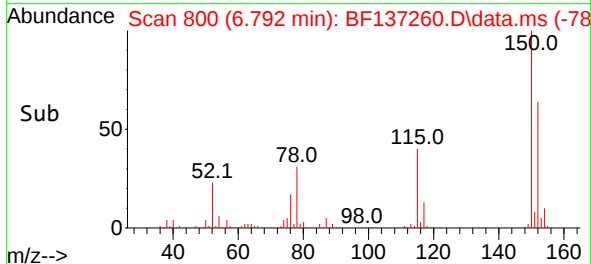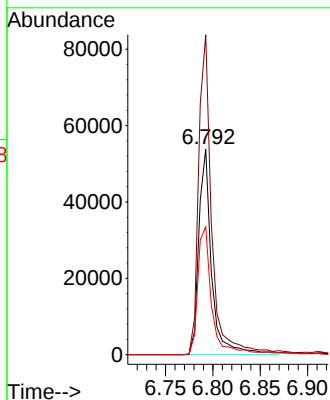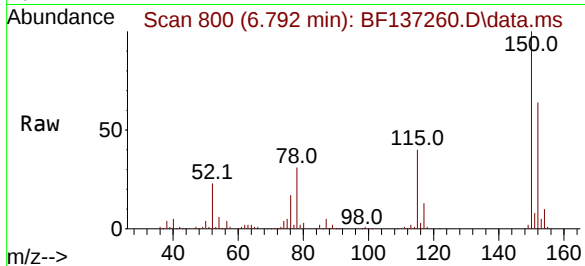

#5
 2-Fluorophenol
 Concen: 115.013 ng
 RT: 5.422 min Scan# 567
 Delta R.T. 0.006 min
 Lab File: BF137260.D
 Acq: 02 Feb 2024 17:47

Tgt Ion:112 Resp: 357819
 Ion Ratio Lower Upper
 112 100
 64 69.0 57.8 86.6
 63 37.0 31.4 47.0


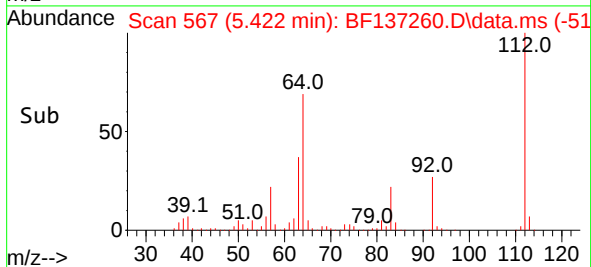
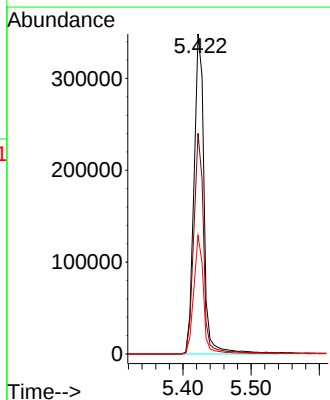
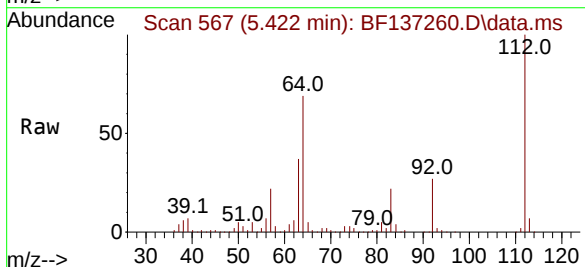


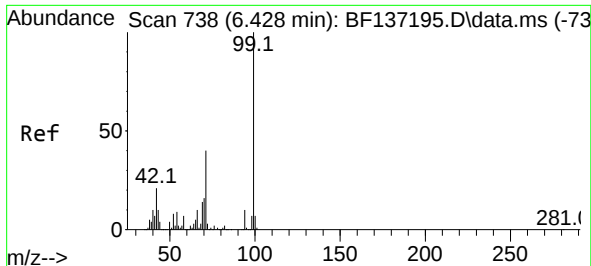

#7
Phenol-d6
Concen: 101.783 ng
RT: 6.422 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF137260.D
Acq: 02 Feb 2024 17:47




Instrument :
BNA_F
ClientSampleId :
TP-5


Tgt Ion: 99 Resp: 451906
Ion Ratio Lower Upper
99 100
42 19.6 16.4 24.6
71 40.9 32.4 48.6

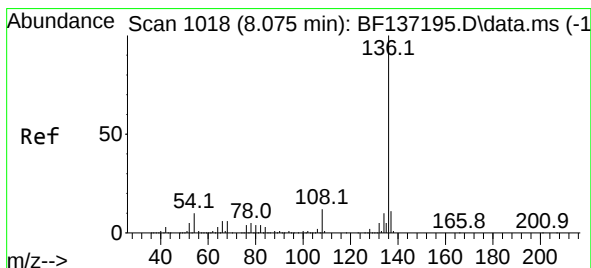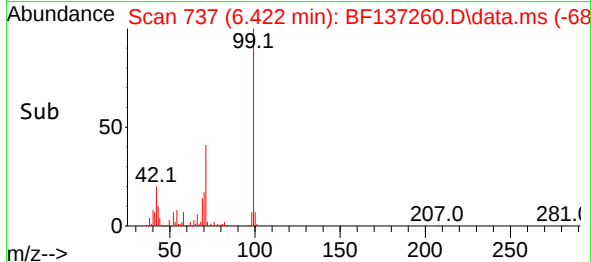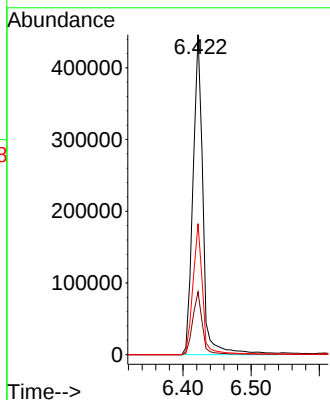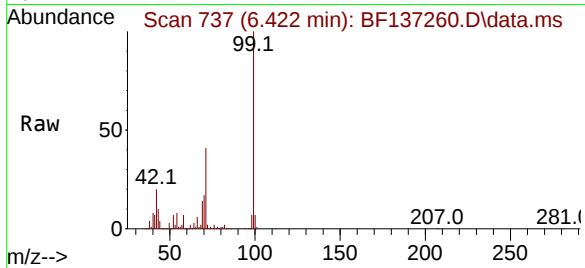

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.069 min Scan# 1017
Delta R.T. -0.006 min
Lab File: BF137260.D
Acq: 02 Feb 2024 17:47

Tgt Ion: 136 Resp: 198214
Ion Ratio Lower Upper
136 100
137 10.4 8.9 13.3
54 9.4 7.8 11.8
68 5.3 4.5 6.7


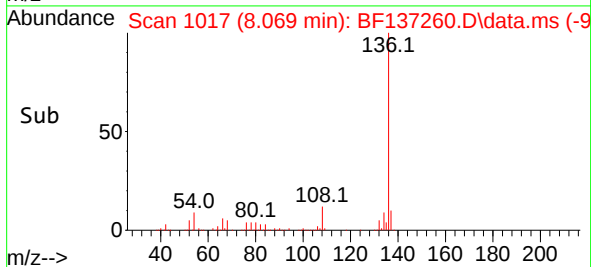
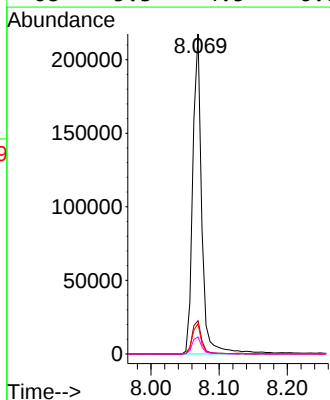
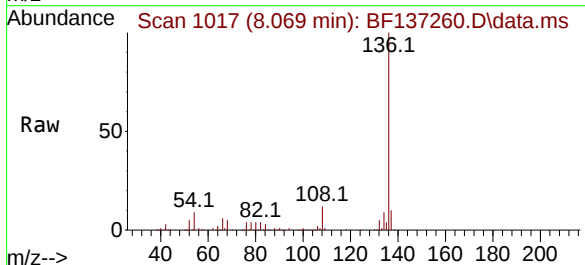


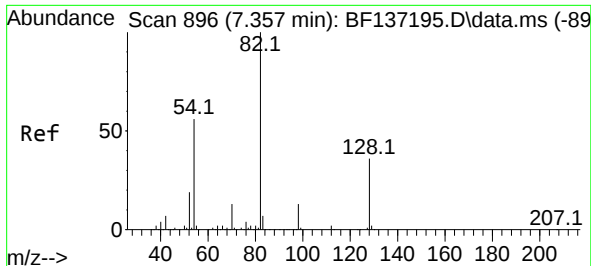

#23
Nitrobenzene-d5
Concen: 66.599 ng
RT: 7.351 min Scan# 895
Delta R.T. -0.006 min
Lab File: BF137260.D
Acq: 02 Feb 2024 17:47




Instrument :
BNA_F
ClientSampleId :
TP-5


Tgt Ion: 82 Resp: 294849
Ion Ratio Lower Upper
82 100
128 39.1 29.1 43.7
54 52.2 45.0 67.6

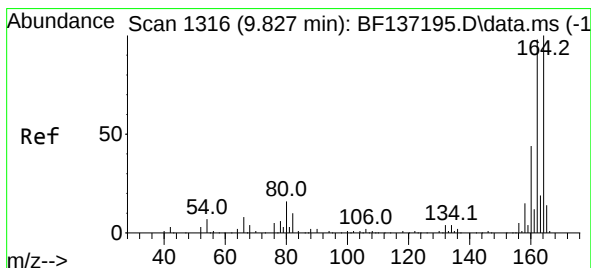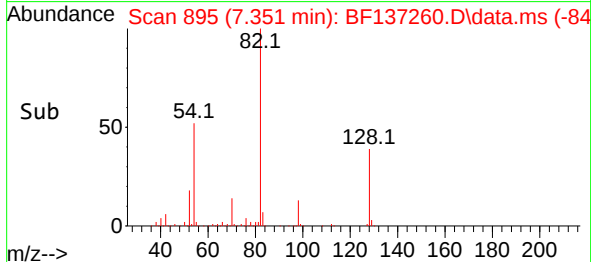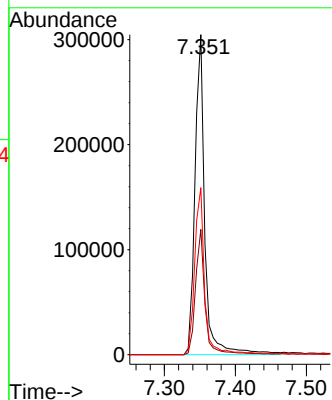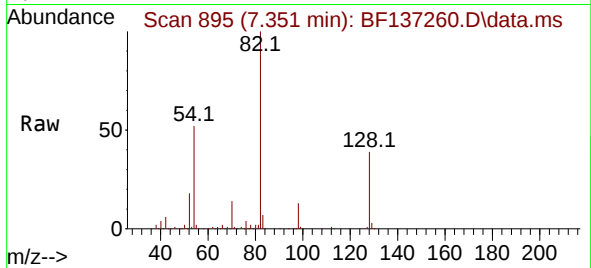

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.822 min Scan# 1315
Delta R.T. -0.005 min
Lab File: BF137260.D
Acq: 02 Feb 2024 17:47

Tgt Ion:164 Resp: 108863
Ion Ratio Lower Upper
164 100
162 96.7 78.3 117.5
160 42.7 35.4 53.2

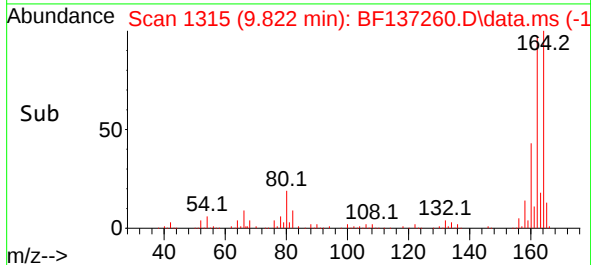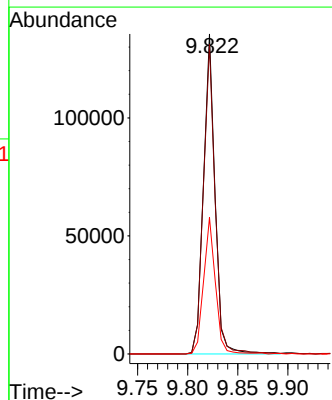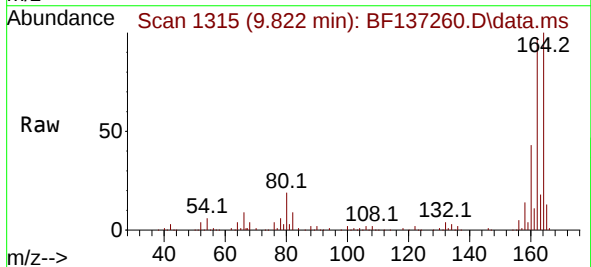

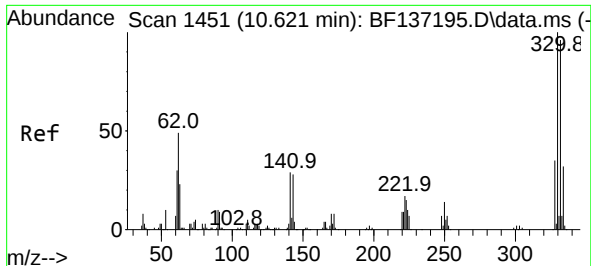

#42

2,4,6-Tribromophenol

Concen: 94.133 ng

RT: 10.610 min Scan# 1449

Delta R.T. -0.012 min

Lab File: BF137260.D

Acq: 02 Feb 2024 17:47

Instrument :

BNA_F

ClientSampleId :

TP-5





Tgt Ion:330 Resp: 115732

Ion Ratio Lower Upper

330 100

332 94.9 77.3 115.9

141 30.6 25.2 37.8

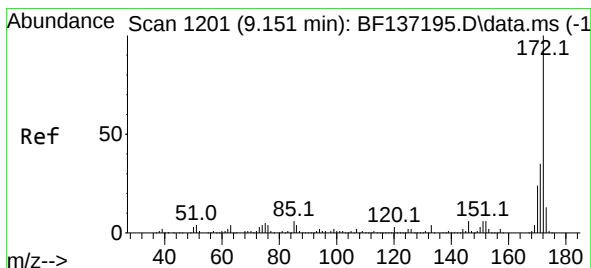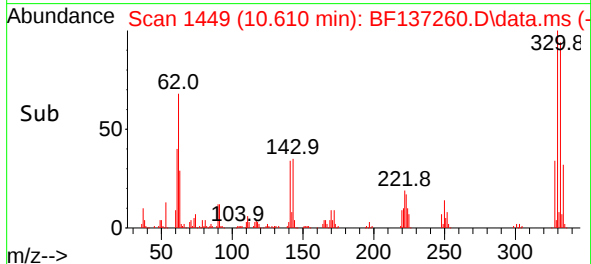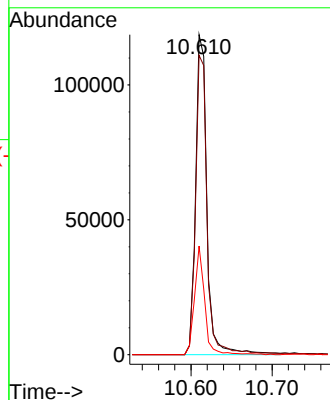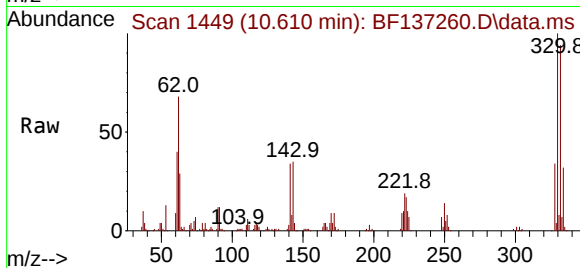

#45

2-Fluorobiphenyl

Concen: 66.318 ng

RT: 9.145 min Scan# 1200

Delta R.T. -0.006 min

Lab File: BF137260.D

Acq: 02 Feb 2024 17:47




Tgt Ion:172 Resp: 525187


Ion Ratio Lower Upper

172 100

171 36.1 28.3 42.5

170 23.9 19.1 28.7


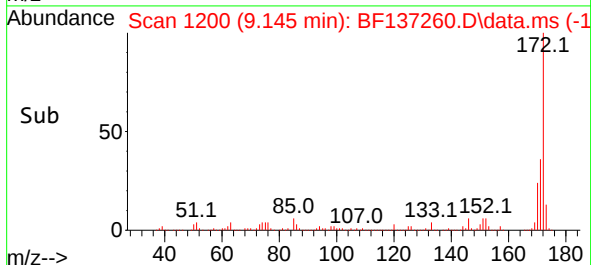
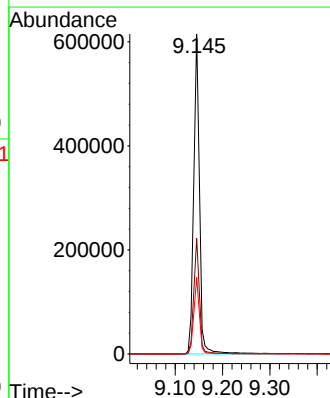
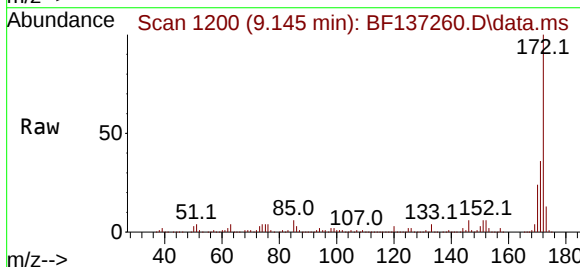


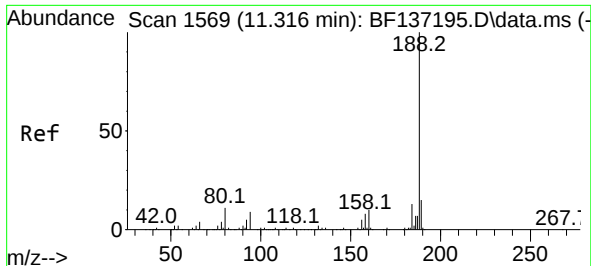

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.310 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF137260.D
Acq: 02 Feb 2024 17:47




Instrument :
BNA_F
ClientSampleId :
TP-5


Tgt Ion:188 Resp: 174364
Ion Ratio Lower Upper
188 100
94 7.9 7.0 10.4
80 9.7 8.8 13.2

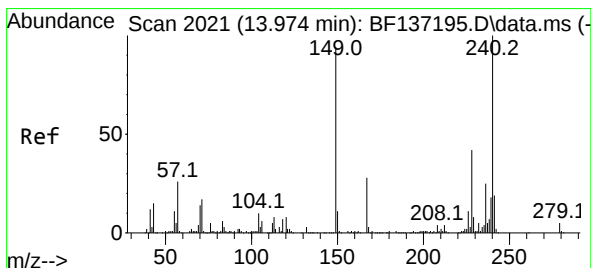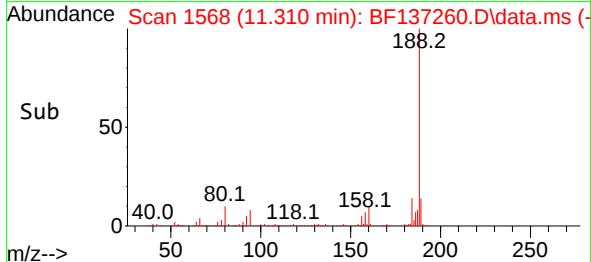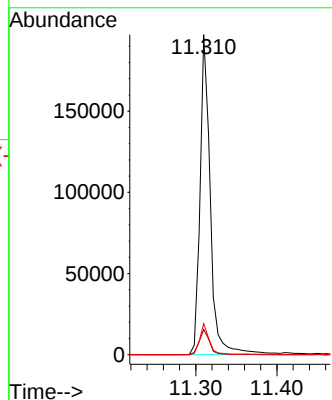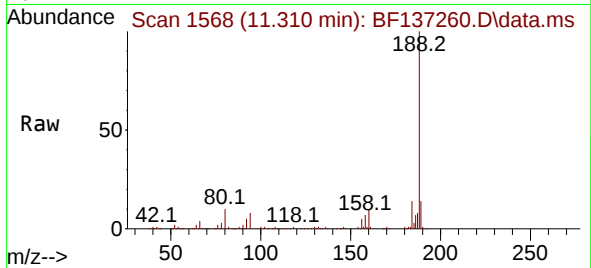

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.963 min Scan# 2019
Delta R.T. -0.012 min
Lab File: BF137260.D
Acq: 02 Feb 2024 17:47

Tgt Ion:240 Resp: 140049
Ion Ratio Lower Upper
240 100
120 7.8 6.3 9.5
236 25.5 20.3 30.5


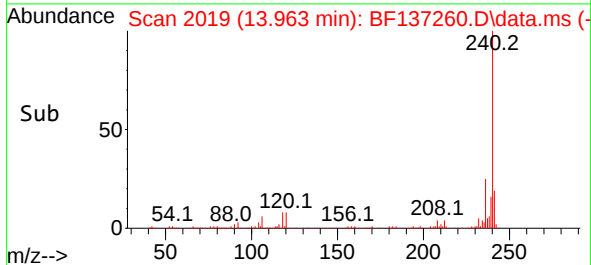
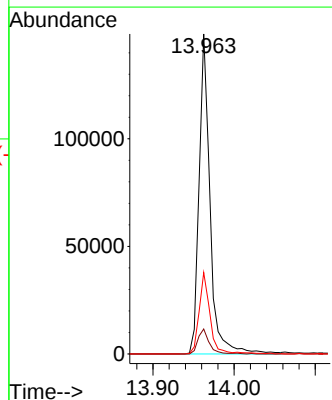
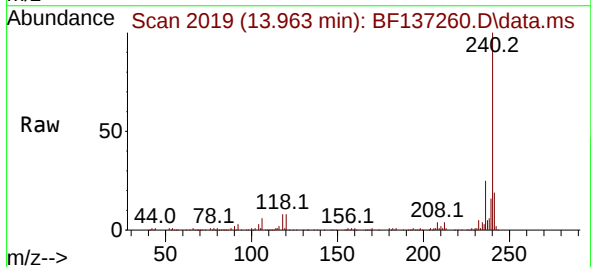


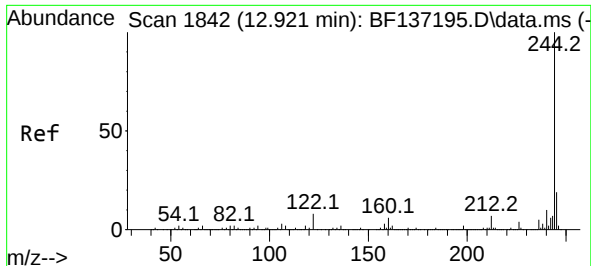

#79
 Terphenyl-d14
 Concen: 49.315 ng
 RT: 12.910 min Scan# 1840
 Delta R.T. -0.012 min
 Lab File: BF137260.D
 Acq: 02 Feb 2024 17:47

Instrument :
 BNA_F
 ClientSampleId :
 TP-5

Tgt Ion:244 Resp: 508044
 Ion Ratio Lower Upper
 244 100
 212 6.9 5.5 8.3
 122 8.6 6.2 9.4

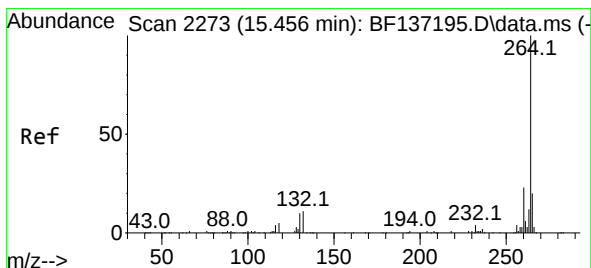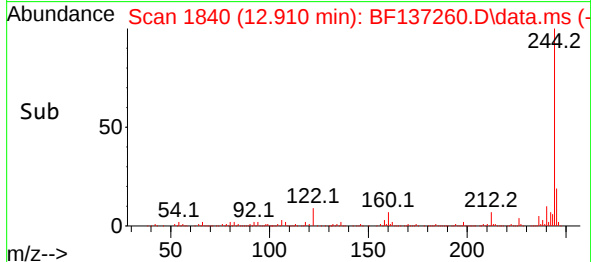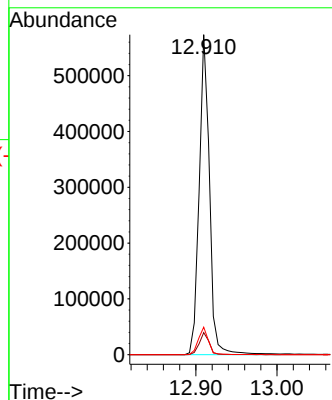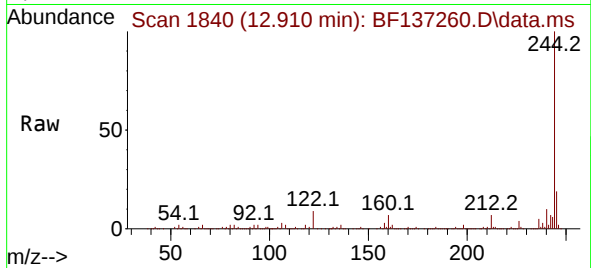

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.445 min Scan# 2271
 Delta R.T. -0.012 min
 Lab File: BF137260.D
 Acq: 02 Feb 2024 17:47

Tgt Ion:264 Resp: 107800
 Ion Ratio Lower Upper
 264 100
 260 22.5 18.2 27.4
 265 19.6 16.2 24.2

