


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF020224\  
Data File : BF137247.D  
Acq On : 02 Feb 2024 09:44  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF013024.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed Jan 31 04:56:22 2024

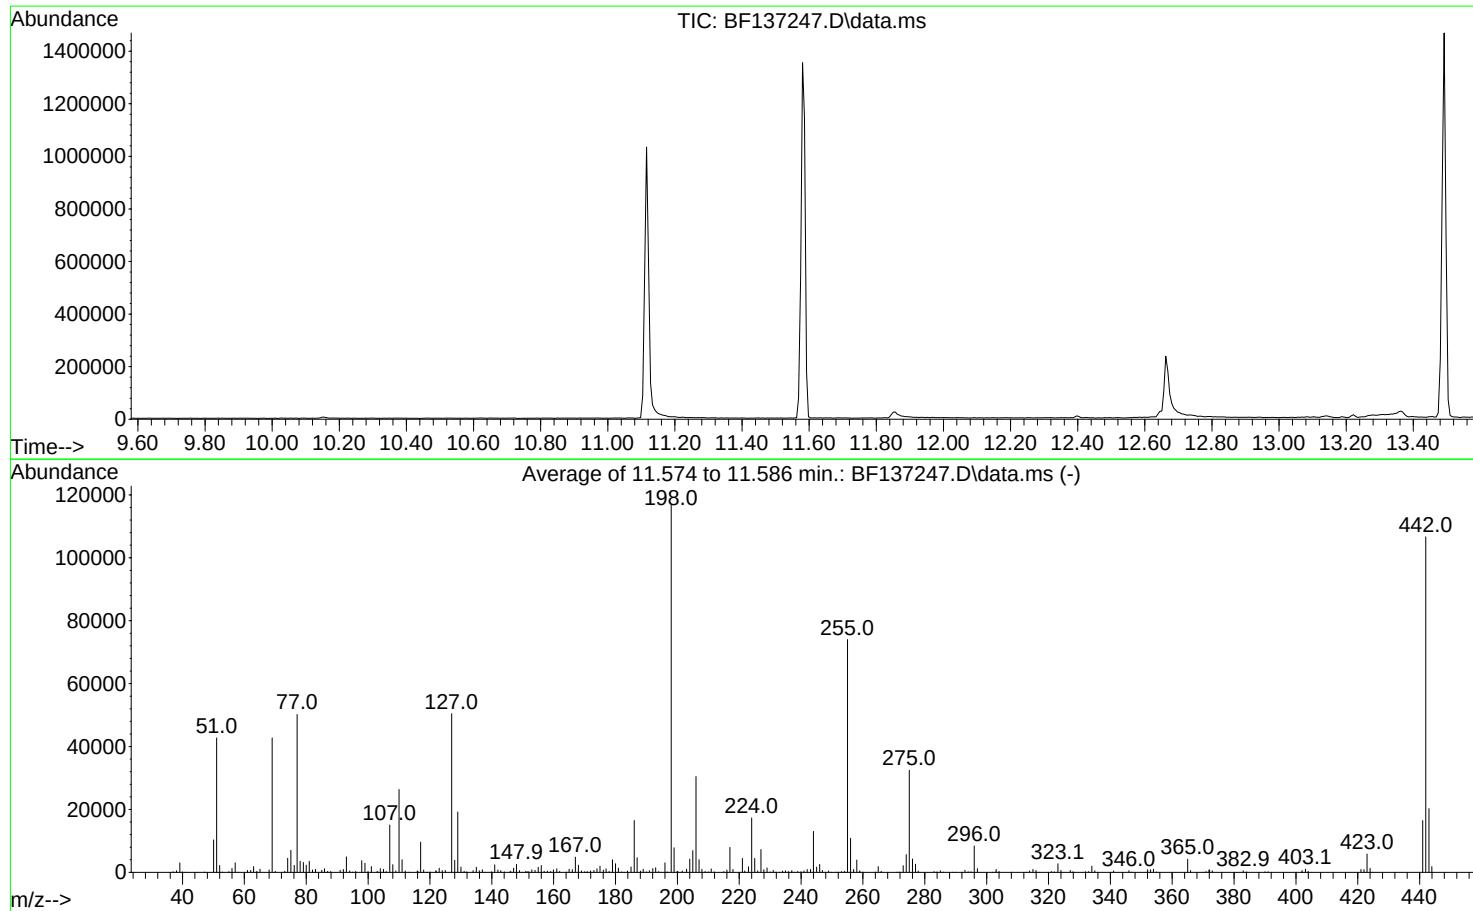




AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 36.6         | 42746      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.8          | 786        | PASS                |
| 69             | 198             | 0.00            | 100             | 36.5         | 42741      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.7          | 294        | PASS                |
| 127            | 198             | 10              | 80              | 43.1         | 50448      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.1          | 163        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 116939     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 7856       | PASS                |
| 275            | 198             | 10              | 60              | 27.7         | 32435      | PASS                |
| 365            | 198             | 1               | 100             | 3.6          | 4179       | PASS                |
| 441            | 198             | 0.01            | 100             | 14.1         | 16494      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 106645     | PASS                |
| 443            | 442             | 15              | 24              | 19.0         | 20228      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF020224\  
Data File : BF137247.D  
Acq On : 02 Feb 2024 09:44  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Feb 02 11:41:31 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF013024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jan 31 04:56:22 2024  
Response via : Initial Calibration

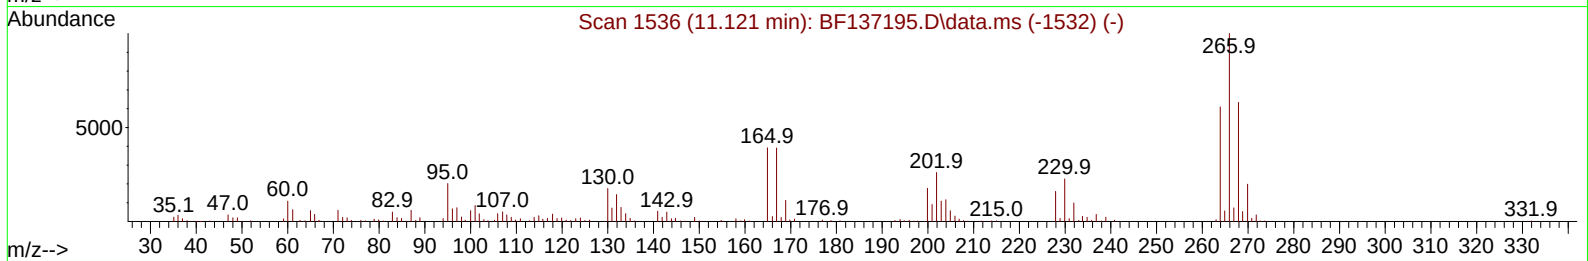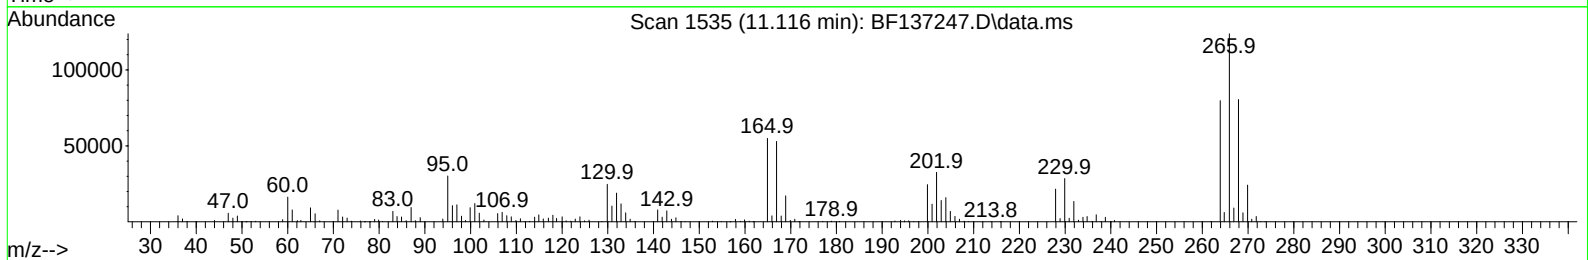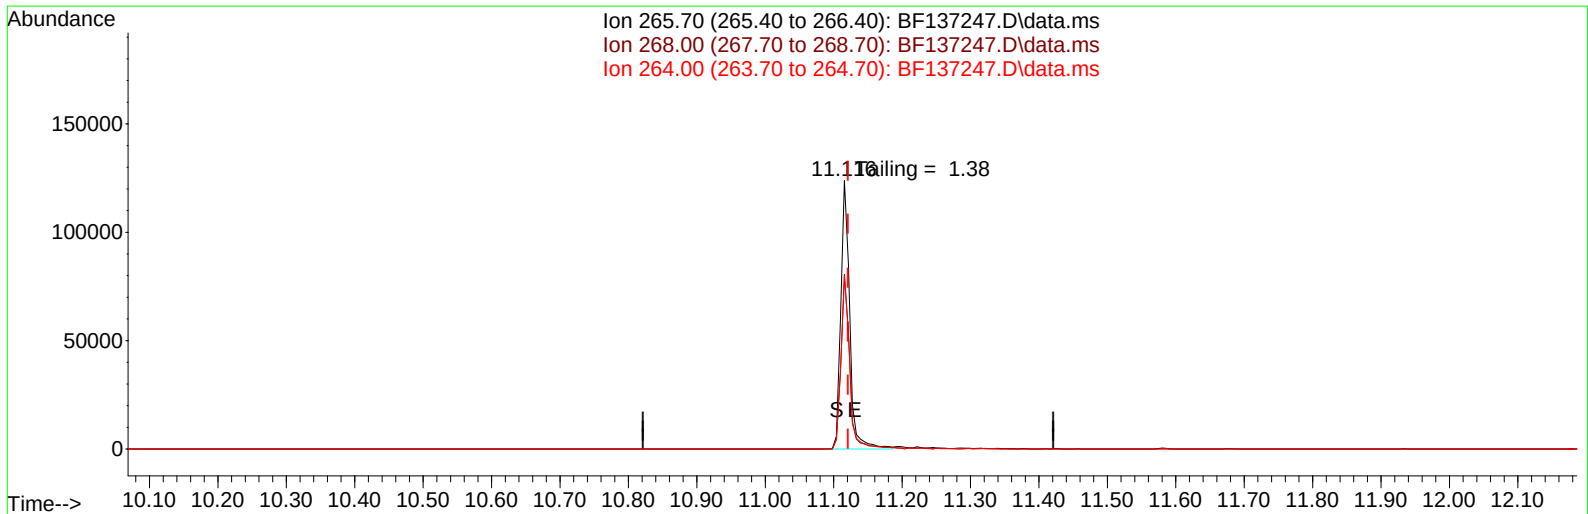

TIC: BF137247.D\data.ms

**(70) Pentachlorophenol (C)**

**11.116min (-0.005) 35015.20 ng**




**response 112910**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.30  | 65.03  |
| 264.00 | 61.00  | 64.49  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF020224\  
Data File : BF137247.D  
Acq On : 02 Feb 2024 09:44  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Feb 02 11:41:31 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF013024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jan 31 04:56:22 2024  
Response via : Initial Calibration

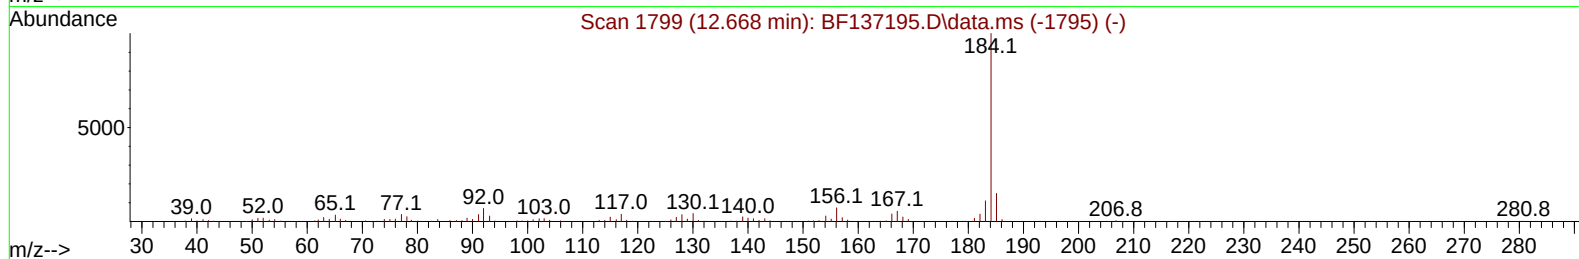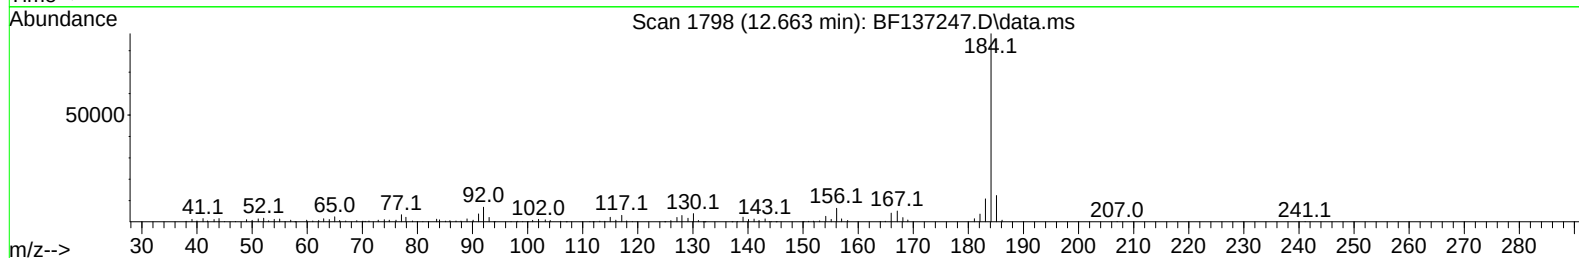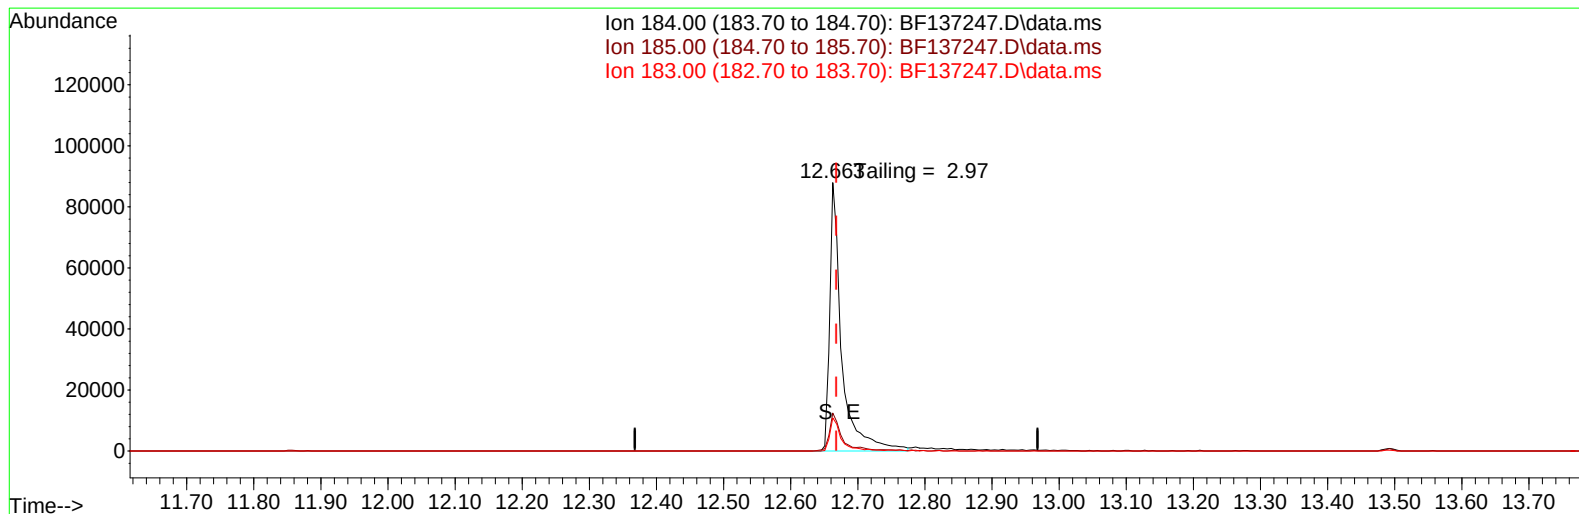

TIC: BF137247.D\data.ms

(77) Benzidine

12.663min (-0.005) 0.00 ng m

response 109077

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.90  | 14.15  |
| 183.00 | 11.00  | 12.35  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 2/2/2024      | BNA_F            | <u>BF137247.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 234762           | 13.492             |
| DDD           | 2659             | 13.221             |
| DDE           | 0                | 12.851             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 2659          | 237421           | 1.12               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP