

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020315\
 Data File : BF077171.D
 Acq On : 3 Feb 2015 20:36
 Operator : TP/IZ
 Sample : G1199-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DCW-WW-054-13015

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	36	37	41	rBV	5641	13540	1.15%	0.209%
2	1.378	41	43	52	rVB	45119	86382	7.36%	1.336%
3	3.664	238	243	245	rBV	4480	13695	1.17%	0.212%
4	3.733	247	249	256	rVV	13217	29690	2.53%	0.459%
5	4.704	331	334	342	rBV2	93011	240088	20.46%	3.713%
6	6.647	502	504	509	rBV	5509	15538	1.32%	0.240%
7	7.093	541	543	547	rBV	46031	107537	9.17%	1.663%
8	7.173	547	550	559	rVB	312641	621183	52.94%	9.607%
9	7.688	592	595	599	rBV	79110	151925	12.95%	2.350%
10	7.916	612	615	619	rBV	3315	12885	1.10%	0.199%
11	7.996	619	622	626	rBV	362312	606199	51.66%	9.375%
12	8.910	700	702	705	rVB	6080	13506	1.15%	0.209%
13	8.990	705	709	714	rBV	274045	496487	42.31%	7.679%
14	10.591	846	849	854	rBV	128726	199139	16.97%	3.080%
15	13.242	1078	1081	1084	rBV	645809	1003016	85.48%	15.512%
16	14.705	1206	1209	1214	rVB2	134457	236637	20.17%	3.660%
17	15.974	1316	1320	1324	rBV	4656	15853	1.35%	0.245%
18	16.397	1353	1357	1358	rBV	7378	14806	1.26%	0.229%
19	16.443	1358	1361	1369	rVB	397531	554489	47.26%	8.576%
20	17.563	1457	1459	1463	rVB	202939	235185	20.04%	3.637%
21	18.980	1581	1583	1588	rBV	4532	13941	1.19%	0.216%
22	19.814	1653	1656	1658	rBV	907467	1173339	100.00%	18.147%
23	20.157	1682	1686	1692	rVB	3932	16296	1.39%	0.252%
24	21.072	1763	1766	1774	rVB	251209	304397	25.94%	4.708%
25	22.375	1876	1880	1883	rBV	4158	12818	1.09%	0.198%
26	22.695	1906	1908	1915	rVB	148002	230217	19.62%	3.560%
27	23.312	1960	1962	1966	rBV2	6148	20116	1.71%	0.311%
28	23.963	2017	2019	2024	rBV	4151	11815	1.01%	0.183%
29	24.123	2030	2033	2036	rBV	5510	15152	1.29%	0.234%


Sum of corrected areas: 6465871

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020315\
Data File : BF077171.D
Acq On : 3 Feb 2015 20:36
Operator : TP/IZ
Sample : G1199-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DCW-WW-054-13015

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

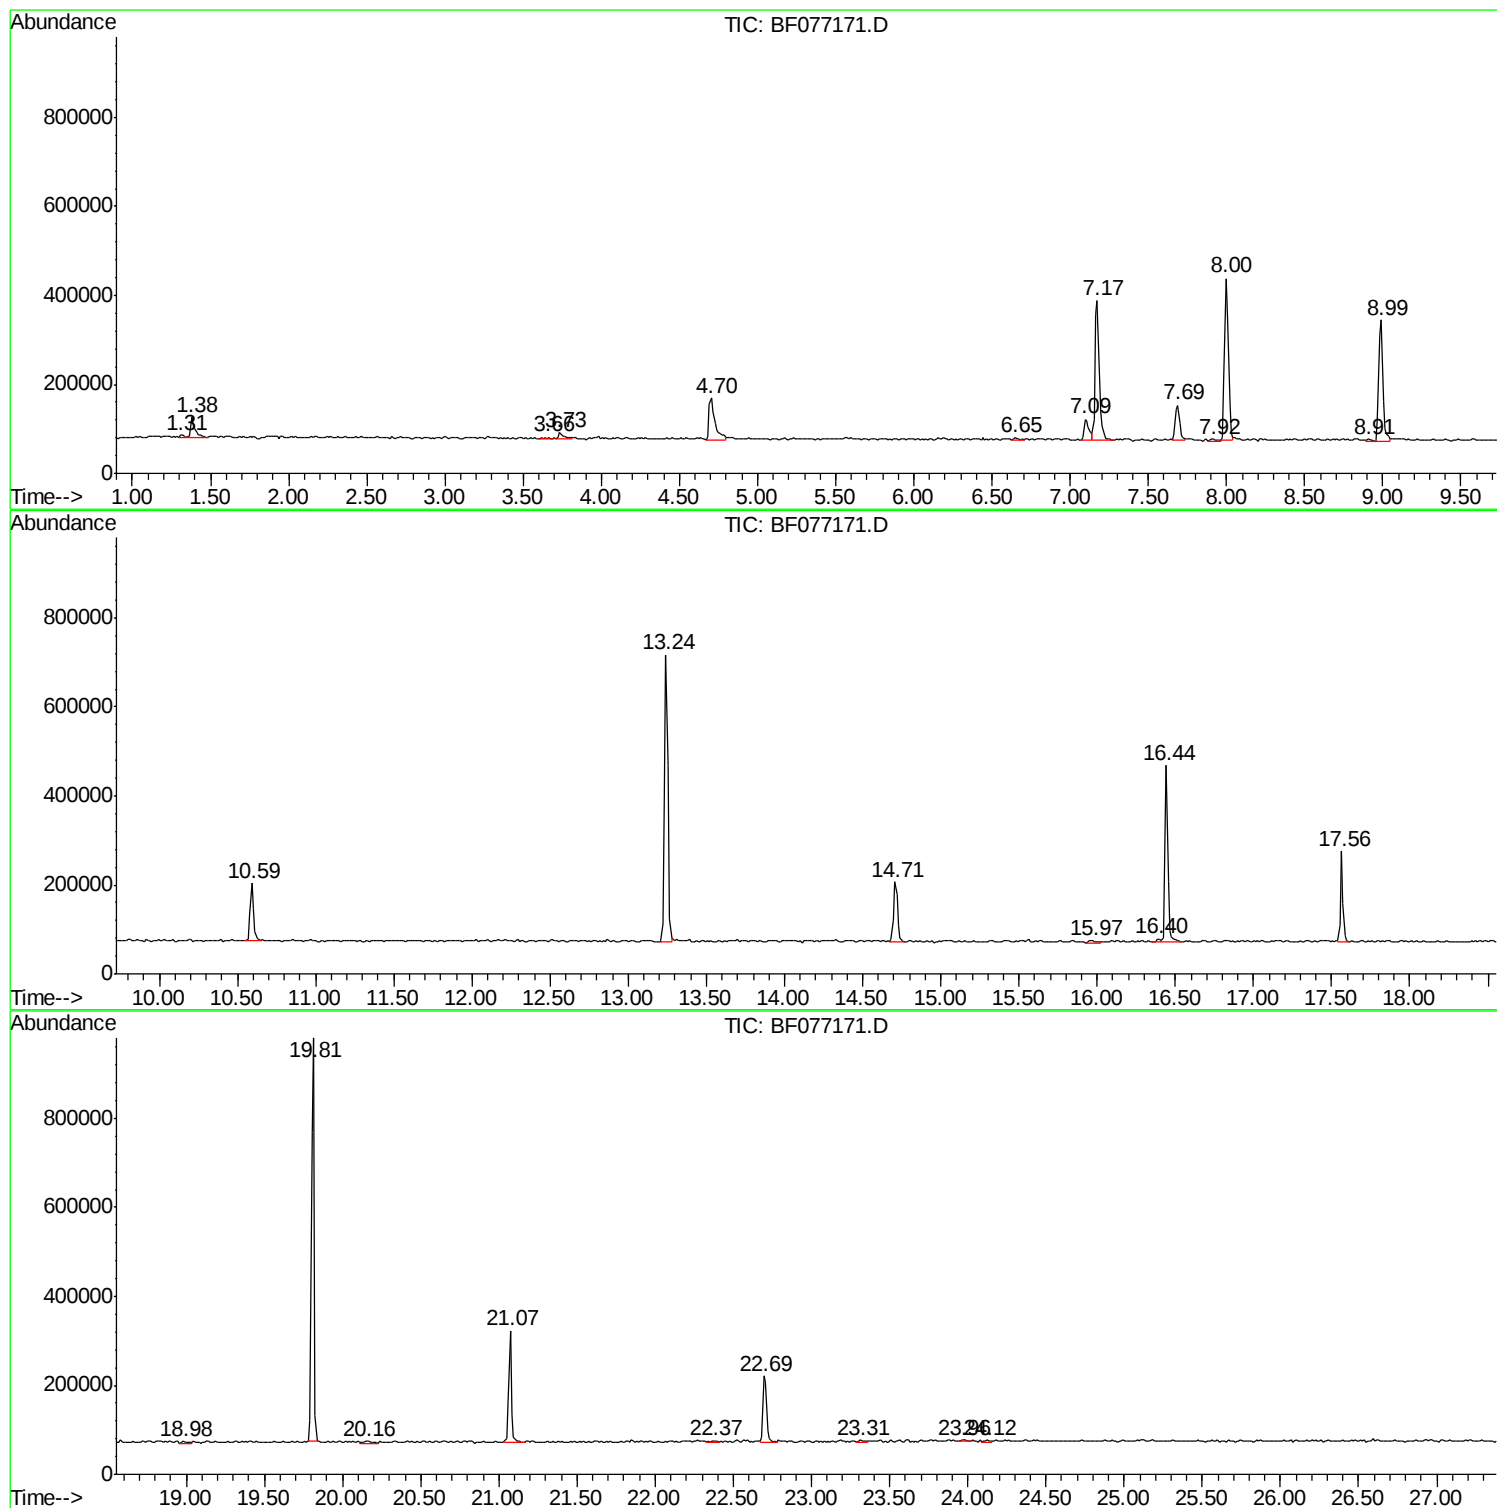

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020315\
Data File : BF077171.D
Acq On : 3 Feb 2015 20:36
Operator : TP/IZ
Sample : G1199-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DCW-WW-054-13015










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 unknown7.17 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.17	81.78 ng	621183	1,4-Dichlorobenzene-d4	7.69

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	25
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
4		Amphetaminil	250	C17H18N2	017590-01-1	12
5		Benzeneethanamine, .alpha.-methy...	223	C16H17N	002980-02-1	12

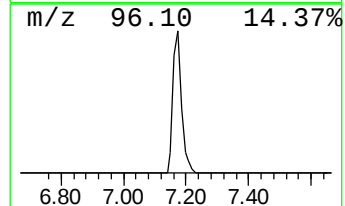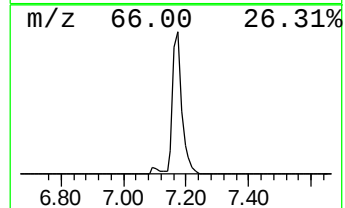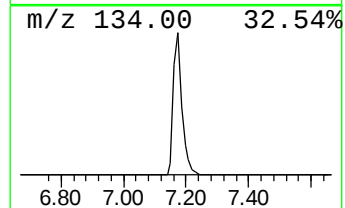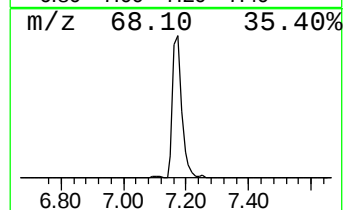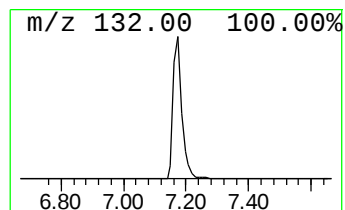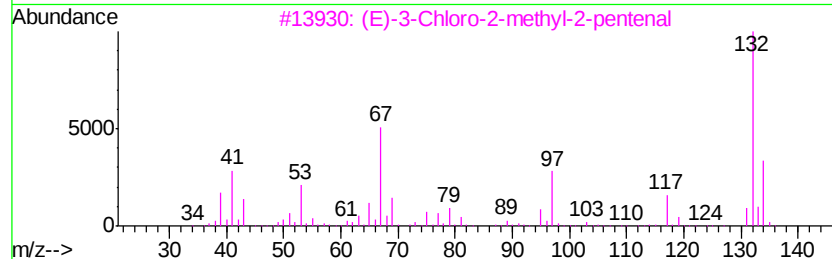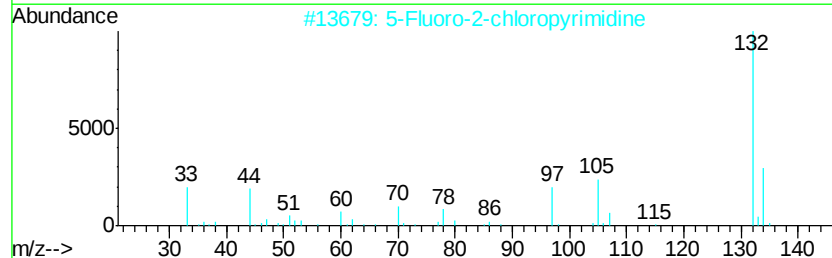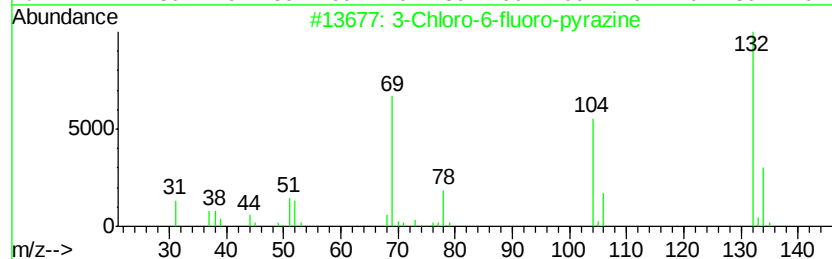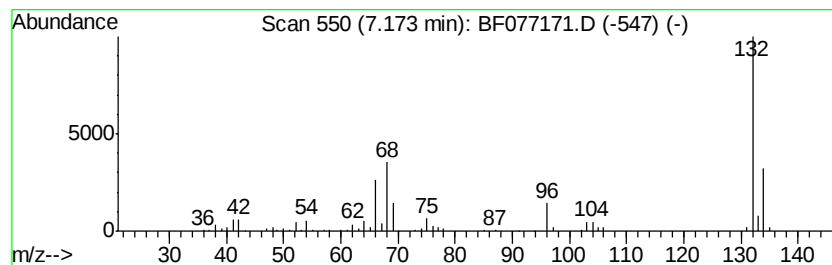

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020315\
Data File : BF077171.D
Acq On : 3 Feb 2015 20:36
Operator : TP/IZ
Sample : G1199-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DCW-WW-054-13015

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.17	7.17	81.8	ng	621183	1	7.69	151925	20.0