


Data Path : Z:\HPCHEM1\BNA_F\Data\BF020315\
 Data File : BF077160.D
 Acq On : 3 Feb 2015 11:35
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 30 22:48:24 2015

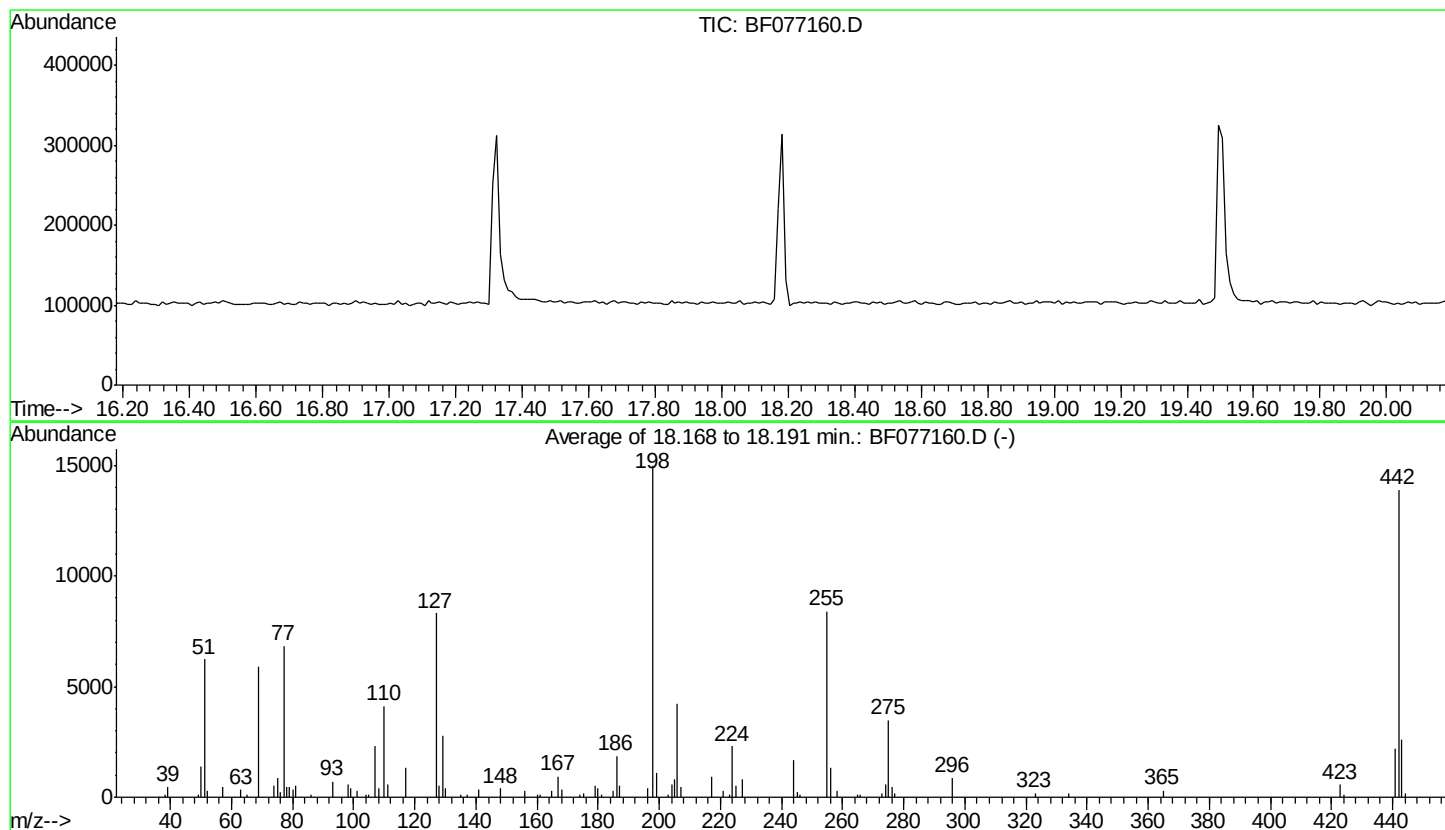

AutoFind: Scans 1512, 1513, 1514; Background Corrected with Scan 1508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.6	6230	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.4	5911	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.4	8310	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14987	PASS
199	198	5	9	7.5	1121	PASS
275	198	10	60	23.3	3488	PASS
365	198	1	100	2.0	305	PASS
441	442	0.01	24	15.7	2180	PASS
442	198	50	100	92.6	13885	PASS
443	442	15	24	18.8	2615	PASS