
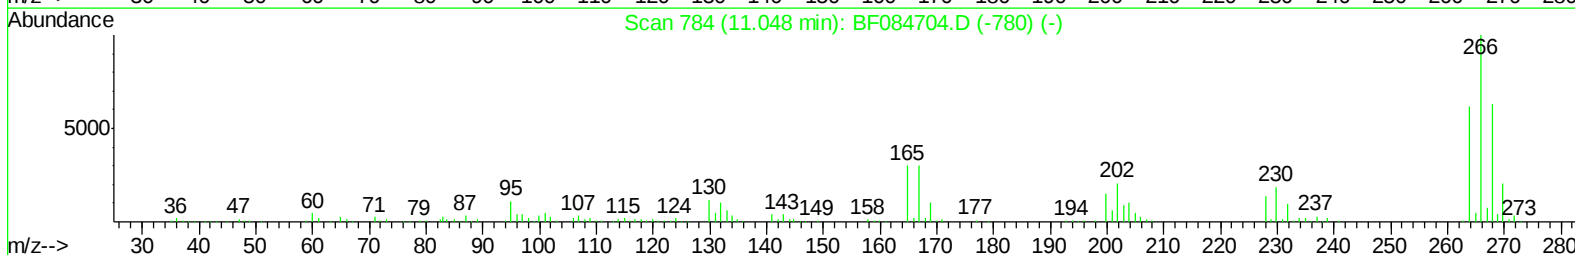
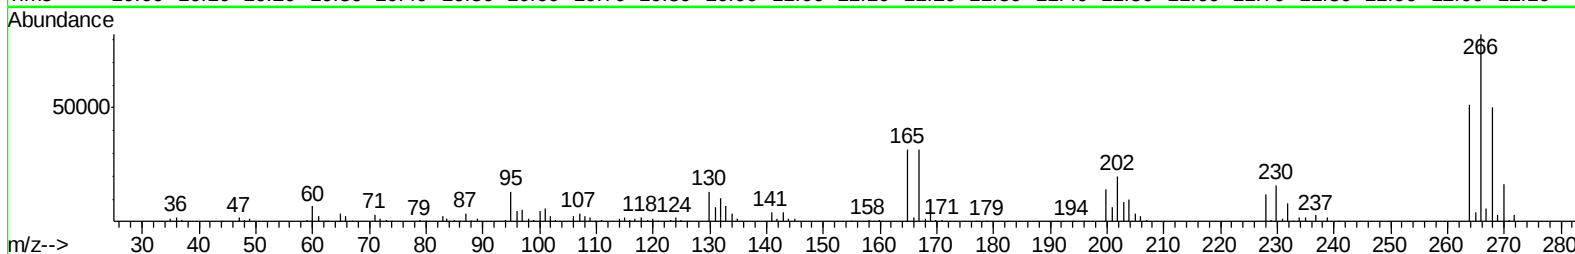


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020316\
Data File : BF084803.D
Acq On : 3 Feb 2016 23:56
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 07:09:15 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 03 14:16:01 2016
Response via : Initial Calibration

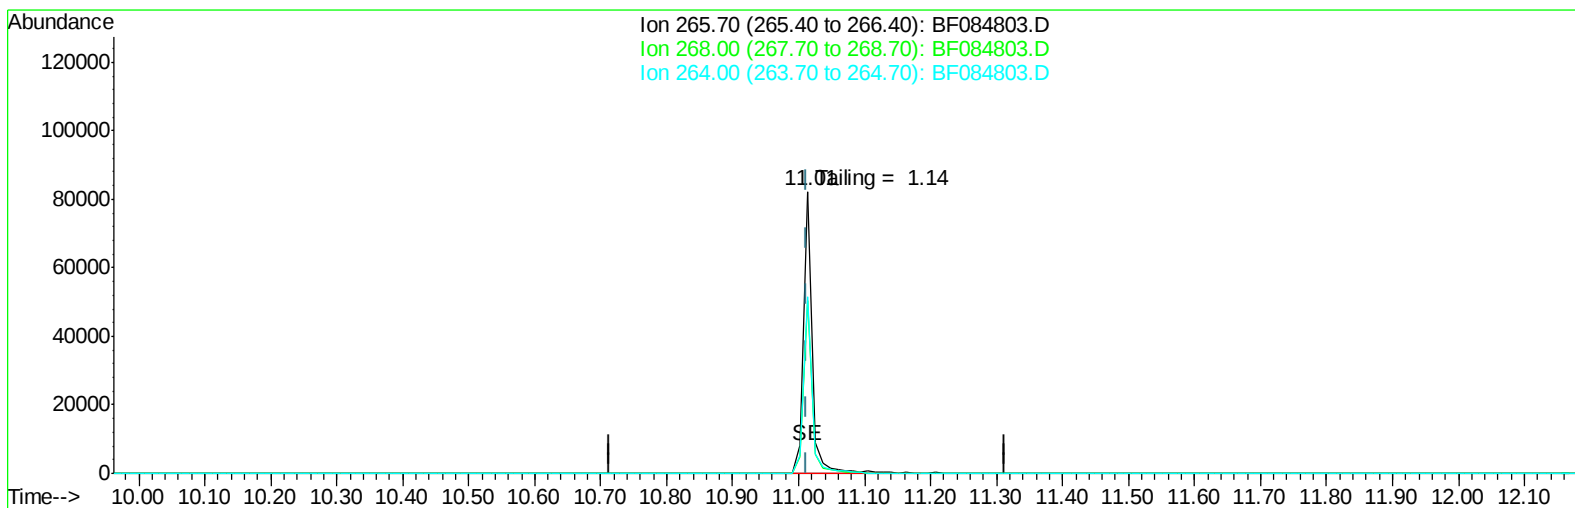

TIC: BF084803.D

(69) Pentachlorophenol (C)




11.014min (+0.000) 53471.97ng

response 75004

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	61.22
264.00	62.70	62.54
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020316\
 Data File : BF084803.D
 Acq On : 3 Feb 2016 23:56
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 07:09:15 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 03 14:16:01 2016
 Response via : Initial Calibration

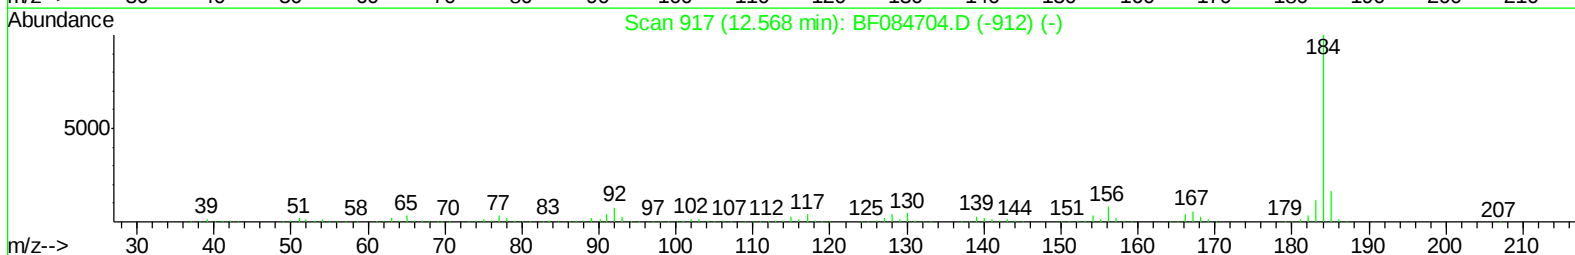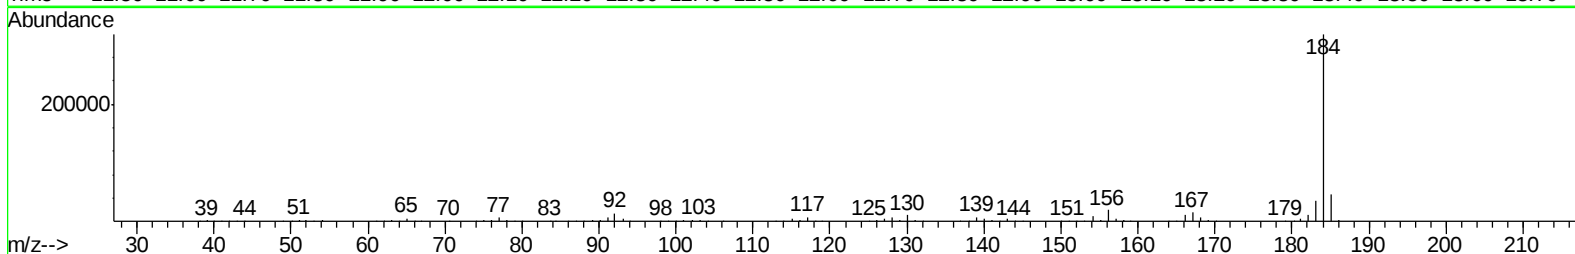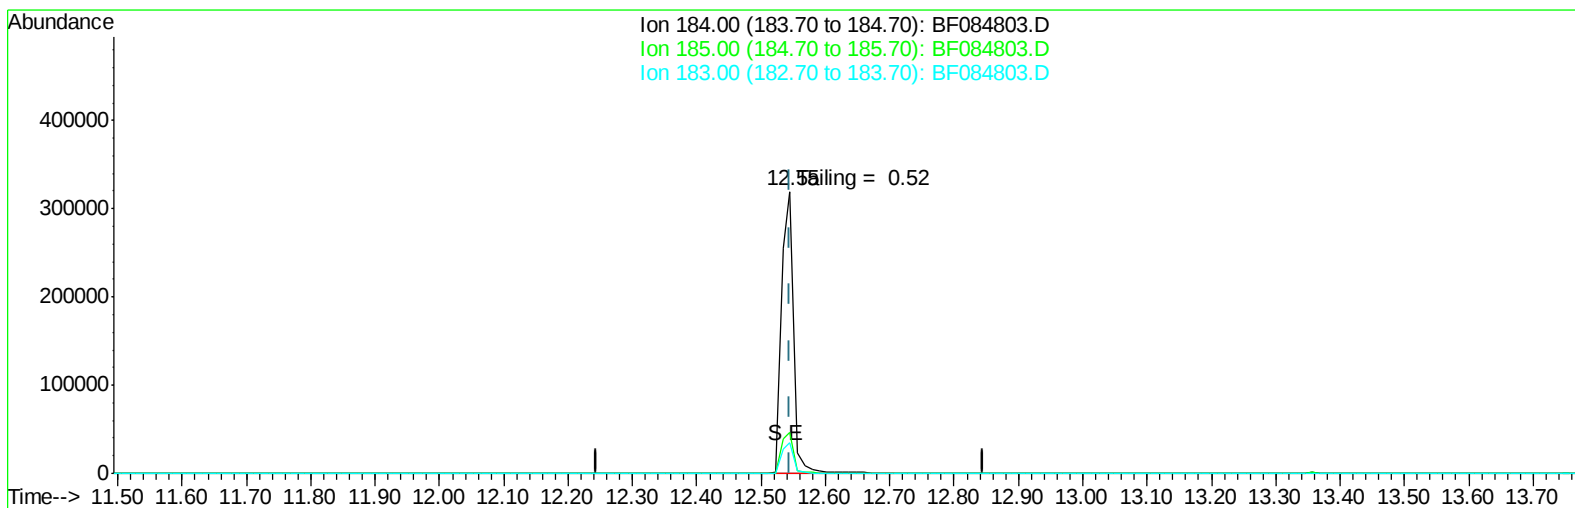

TIC: BF084803.D

(76) Benzidine

12.545min (+0.000) 0.00ng

response 430668

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.48
183.00	12.30	10.96
0.00	0.00	0.00