

Data Path : Z:\HPCHEM1\BNA F\DATA\BF020316\
 Data File : BF084801.D
 Acq On : 3 Feb 2016 22:59
 Operator : SJ/IZ
 Sample : H1331-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WEST-SIDEWALL(9)

Quant Time: Feb 04 03:58:50 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 03 14:16:01 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.68	152	165208	20.00	ng	0.00
21) Naphthalene-d8	7.97	136	730319	20.00	ng	0.00
38) Acenaphthene-d10	9.72	164	333306	20.00	ng	-0.01
63) Phenanthrene-d10	11.20	188	596267	20.00	ng	-0.01
75) Chrysene-d12	13.83	240	505968	20.00	ng	-0.01
86) Perylene-d12	15.21	264	348880	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.29	112	1415171	133.42	ng	0.01
7) Phenol-d6	6.34	99	1543514	117.39	ng	0.00
23) Nitrobenzene-d5	7.25	82	951146	73.37	ng	-0.01
41) 2,4,6-Tribromophenol	10.51	330	420053	120.82	ng	-0.01
44) 2-Fluorobiphenyl	9.06	172	1868039	100.54	ng	0.00
78) Terphenyl-d14	12.80	244	1789879	80.16	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.45	163	230949	9.10	ng	Qvalue # 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF020316\
Data File : BF084801.D
Acq On : 3 Feb 2016 22:59
Operator : SJ/IZ
Sample : H1331-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WEST-SIDEWALL(9)

Quant Time: Feb 04 03:58:50 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 03 14:16:01 2016
Response via : Initial Calibration

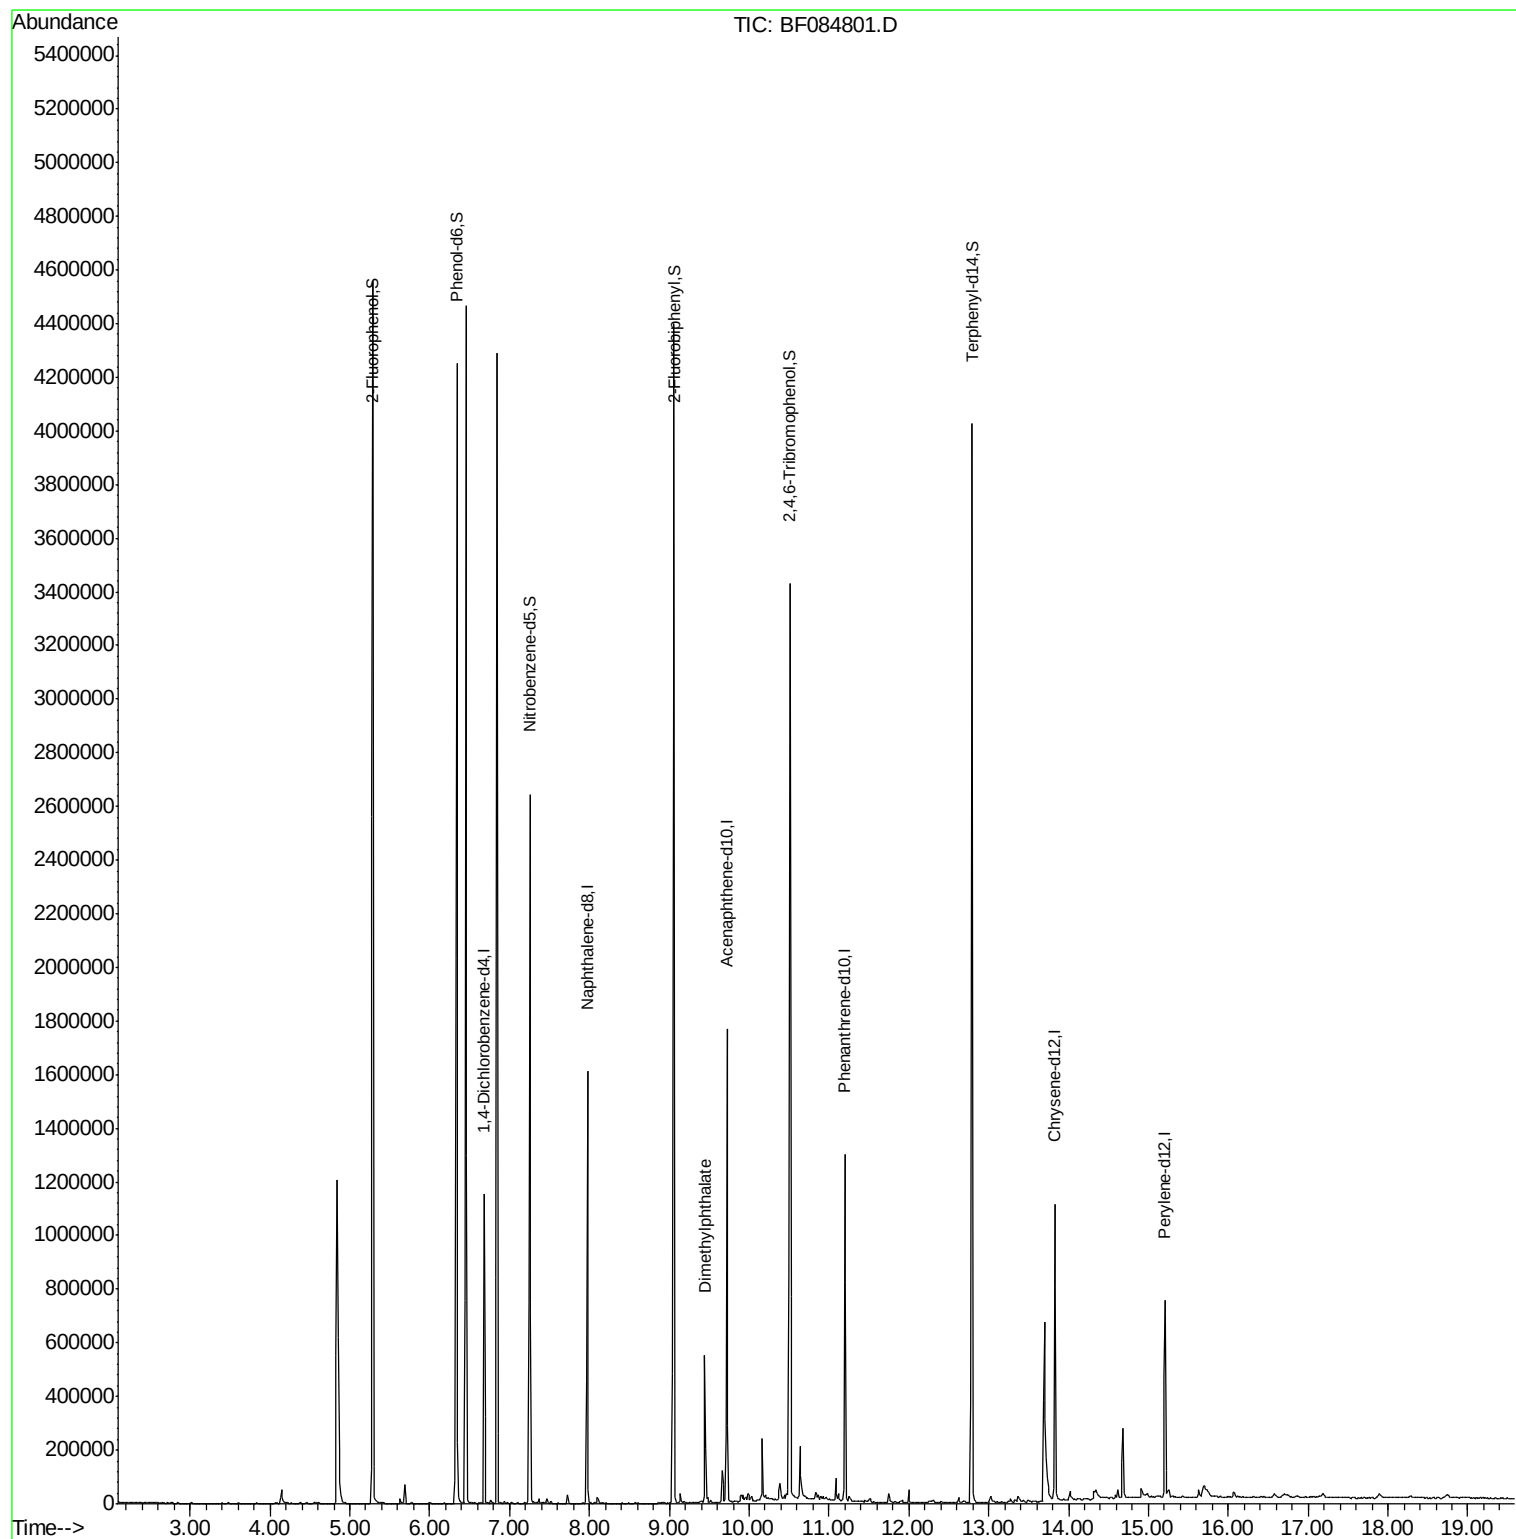

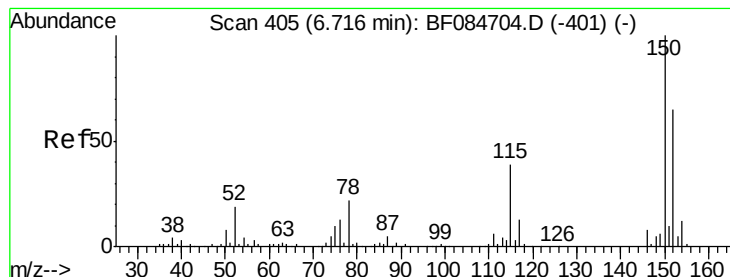


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.68 min Scan# 402
Delta R.T. -0.00 min
Lab File: BF084801.D
Acq: 3 Feb 2016 22:59

Instrument :
BNA_F
ClientSampleId :
WEST-SIDEWALL(9)

Tot Ion	Ratio	Lower	Upper
152	100		
150	159.7	123.0	184.4
115	72.3	51.4	77.2

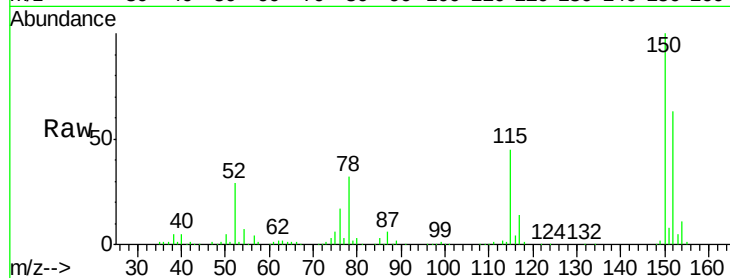


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

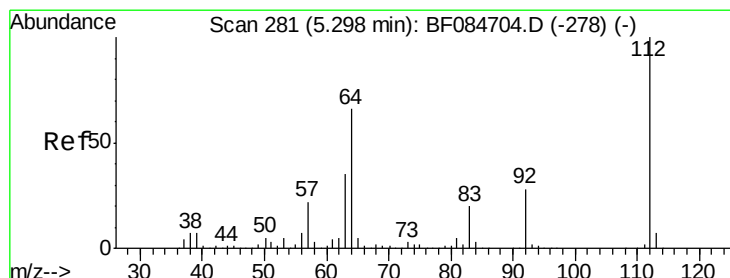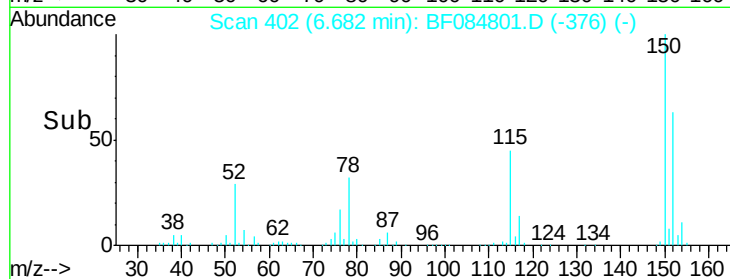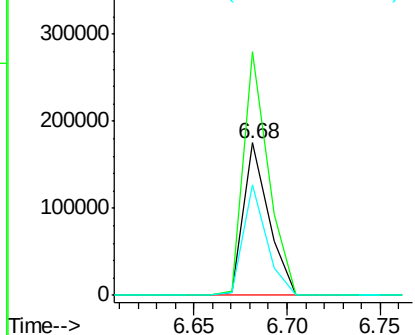



#5


2-Fluorophenol
Concen: 133.42 ng
RT: 5.29 min Scan# 280
Delta R.T. 0.01 min
Lab File: BF084801.D
Acq: 3 Feb 2016 22:59

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.4	36.6	55.0#
63	31.6	19.4	29.0#

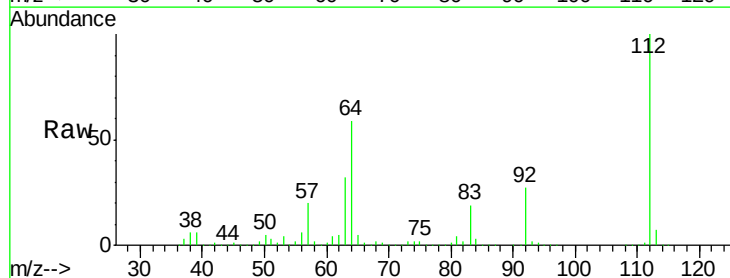

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

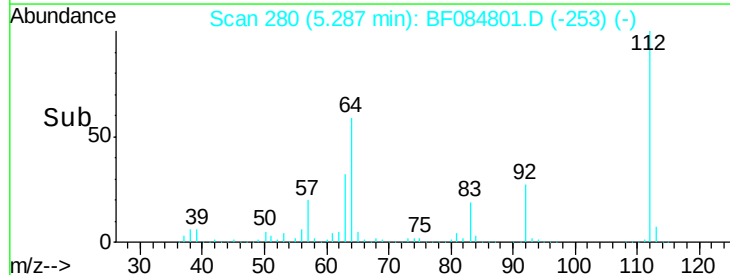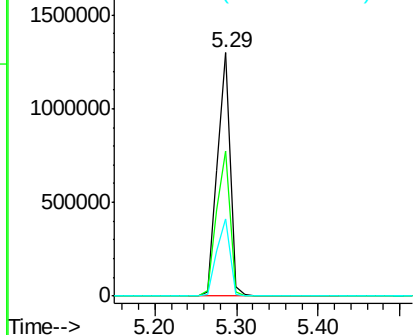

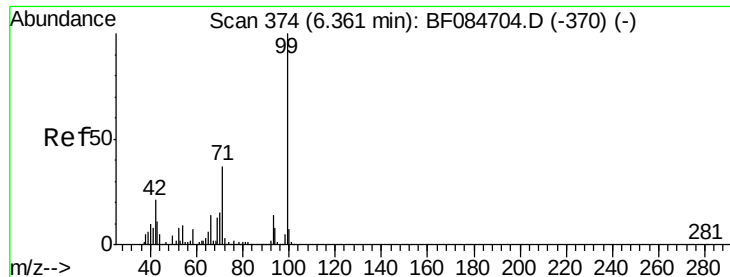

#7

Phenol-d6

Concen: 117.39 ng

RT: 6.34 min Scan# 372

Delta R.T. 0.00 min

Lab File: BF084801.D

Acq: 3 Feb 2016 22:59

Instrument :





BNA_F

ClientSampleId :

WEST-SIDEWALL(9)

Tot Ion: 99 Resp: 1543514

Ion	Ratio	Lower	Upper
99	100		
42	20.5	12.8	19.2#
71	37.7	30.9	46.3

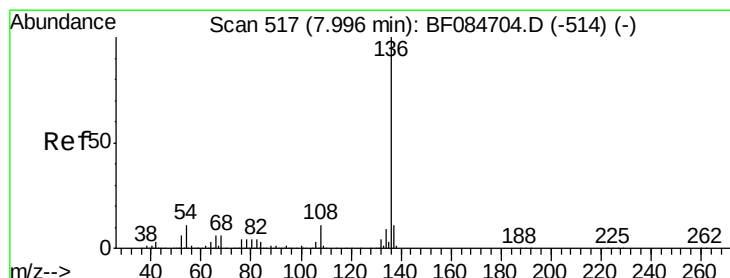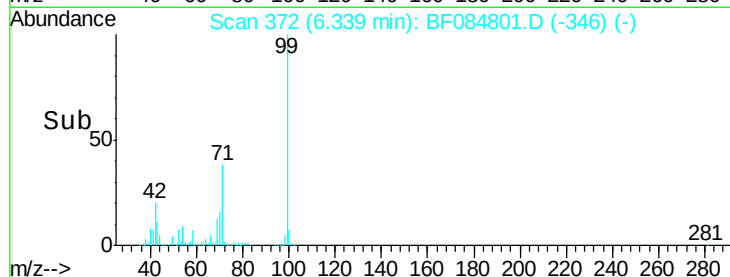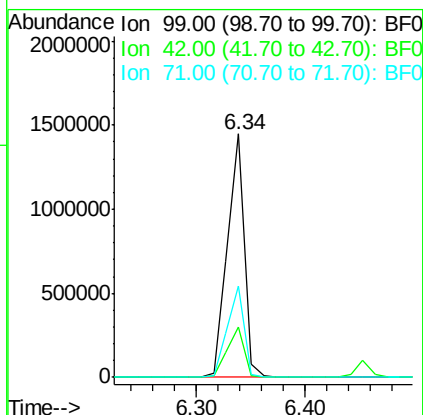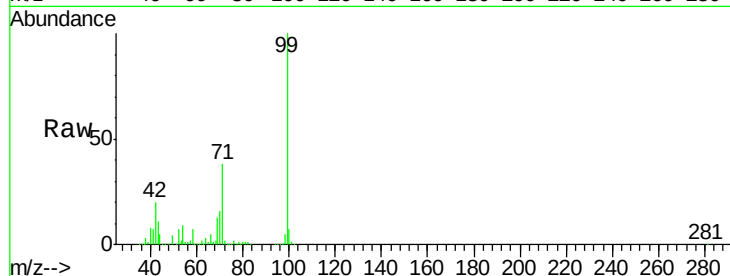

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.97 min Scan# 515




Delta R.T. 0.00 min


Lab File: BF084801.D

Acq: 3 Feb 2016 22:59

Tgt Ion: 136 Resp: 730319

Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.7	13.1
54	7.6	5.8	8.8
68	4.6	4.2	6.2

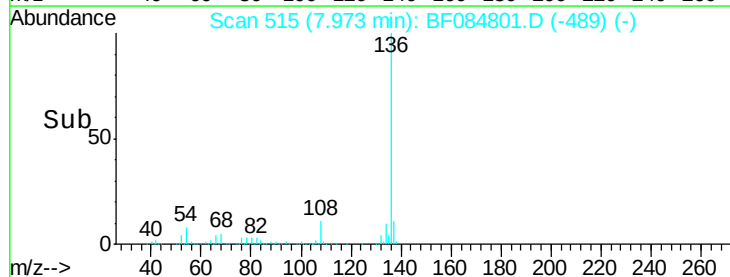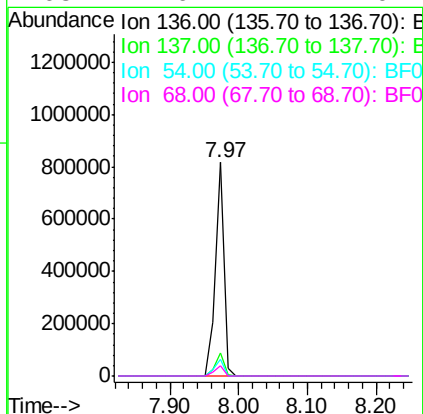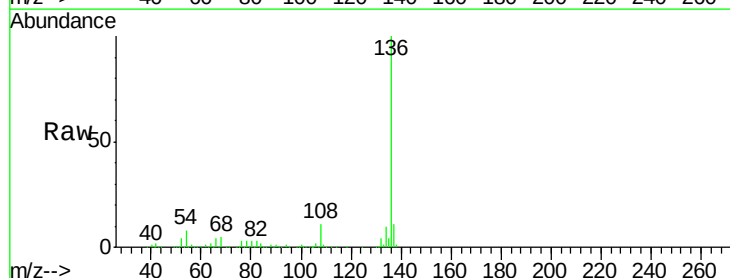


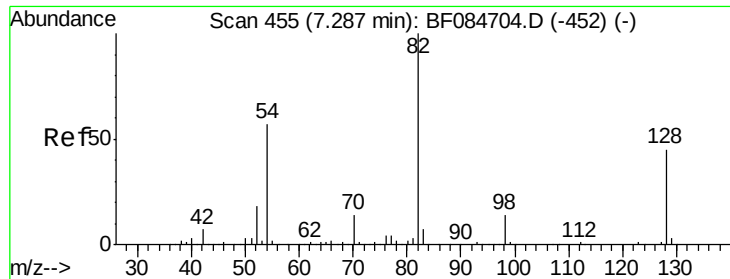




#23
 Nitrobenzene-d5
 Concen: 73.37 ng
 RT: 7.25 min Scan# 452
 Delta R.T. -0.01 min
 Lab File: BF084801.D
 Acq: 3 Feb 2016 22:59

Instrument :
 BNA_F
 ClientSampleId :
 WEST-SIDEWALL(9)

Tot Ion	82	Resp	951146
Ion Ratio	Lower	Upper	
82	100		
128	41.8	34.6	51.8
54	57.7	38.4	57.6

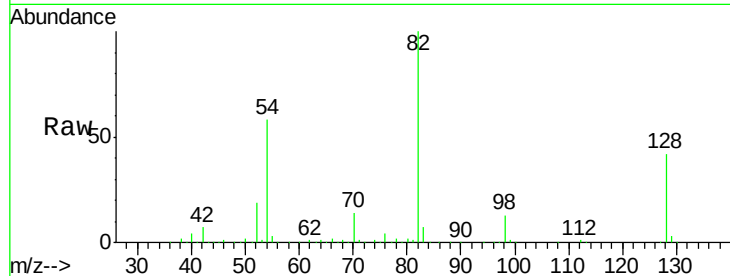


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

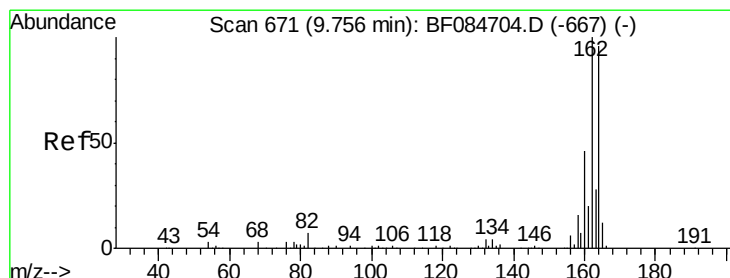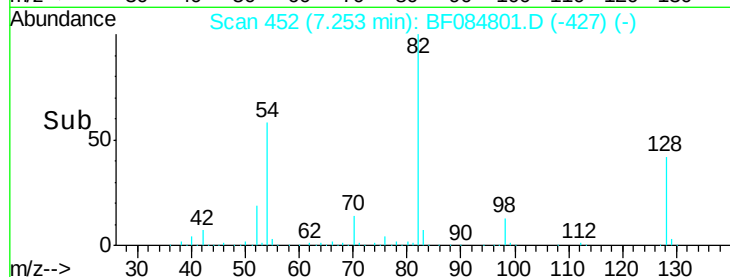
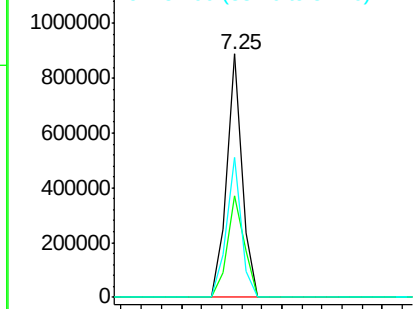



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.72 min Scan# 668
 Delta R.T. -0.01 min
 Lab File: BF084801.D
 Acq: 3 Feb 2016 22:59

Tgt Ion	164	Resp	333306
Ion Ratio	Lower	Upper	
164	100		
162	104.9	85.1	127.7
160	47.6	37.5	56.3

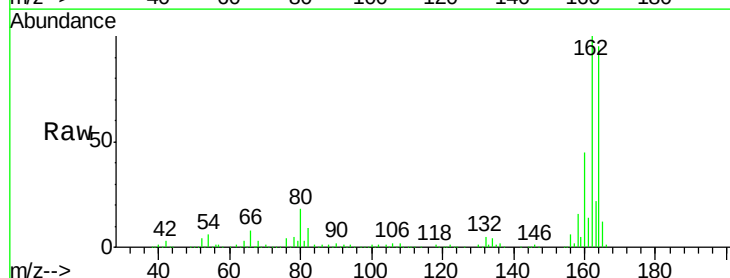

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

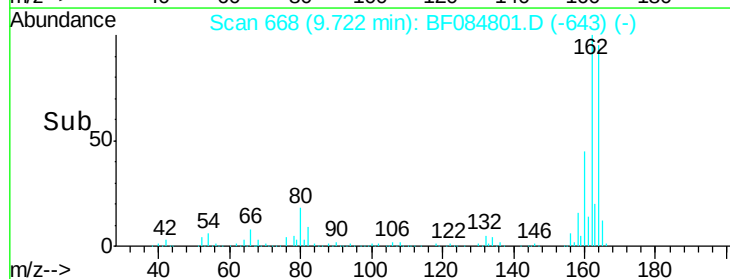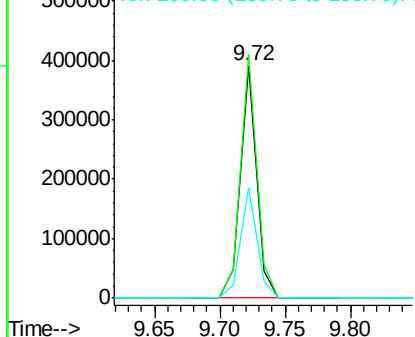


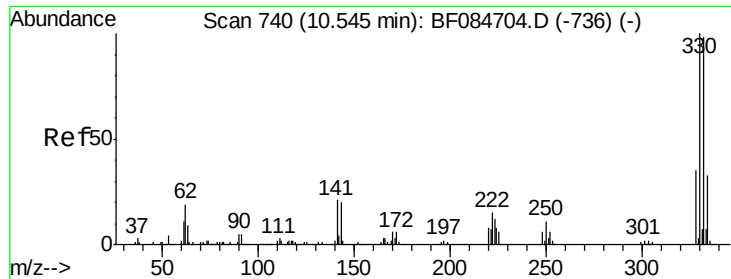




#41
 2,4,6-Tribromophenol
 Concen: 120.82 ng
 RT: 10.51 min Scan# 737
 Delta R.T. -0.01 min
 Lab File: BF084801.D
 Acq: 3 Feb 2016 22:59

Instrument :
 BNA_F
 ClientSampleId :
 WEST-SIDEWALL(9)

Tot Ion:330 Resp: 420053
 Ion Ratio Lower Upper
 330 100
 332 97.0 76.6 114.8
 141 38.4 27.8 41.6

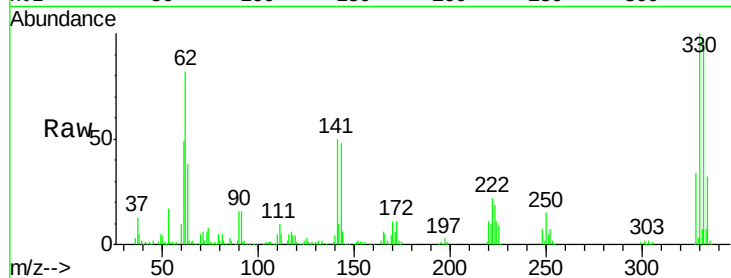


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

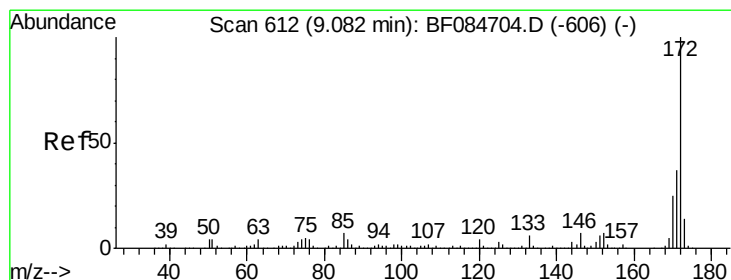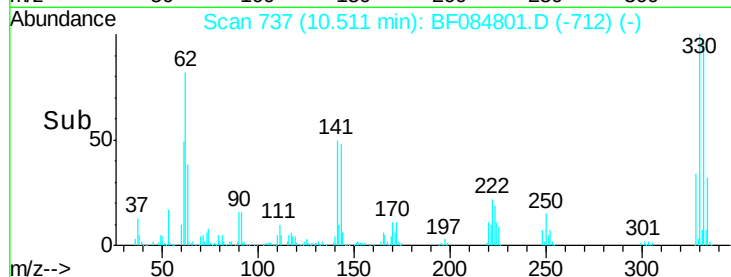
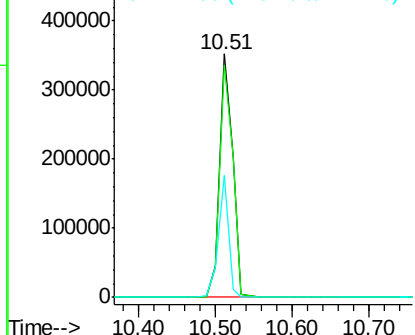



#44
 2-Fluorobiphenyl
 Concen: 100.54 ng
 RT: 9.06 min Scan# 610
 Delta R.T. -0.00 min
 Lab File: BF084801.D
 Acq: 3 Feb 2016 22:59

Tgt Ion:172 Resp: 1868039
 Ion Ratio Lower Upper
 172 100
 171 36.8 28.9 43.3
 170 24.8 18.6 27.8

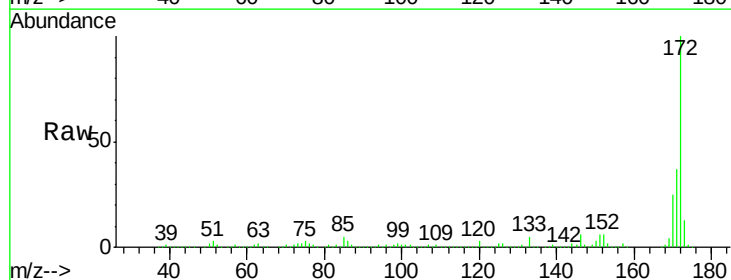

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

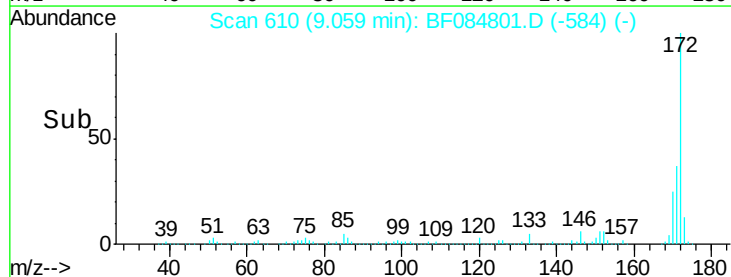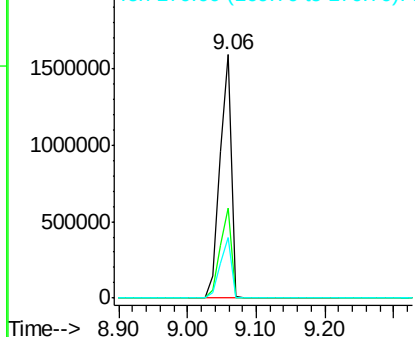

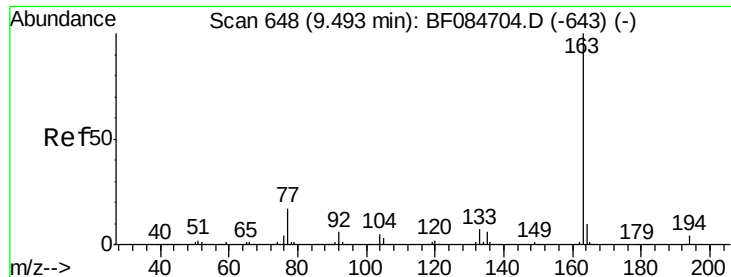

#49

Dimethylphthalate

Concen: 9.10 ng

RT: 9.45 min Scan# 644

Delta R.T. -0.02 min

Lab File: BF084801.D

Acq: 3 Feb 2016 22:59

Instrument :

BNA_F

ClientSampleId :

WEST-SIDEWALL(9)


Tot Ion:163 Resp: 230949

Ion Ratio Lower Upper

163 100

194 2.7 8.0 12.0#




164 10.0 8.0 12.0

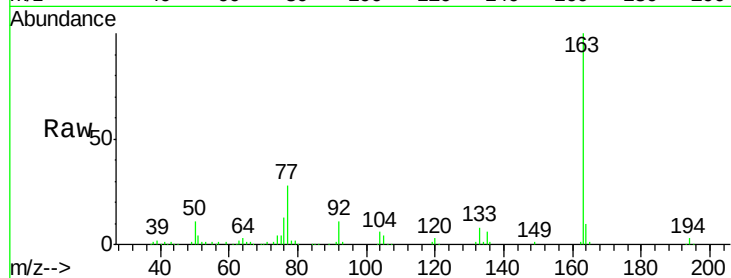

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

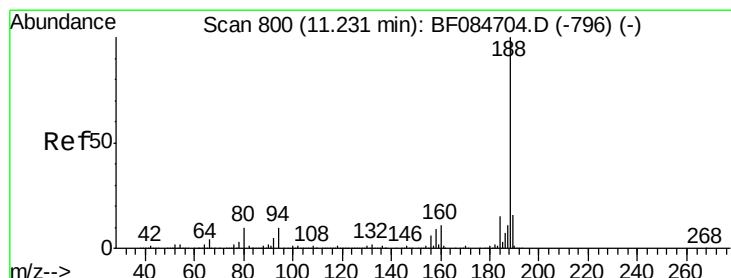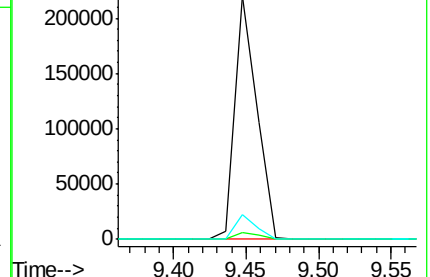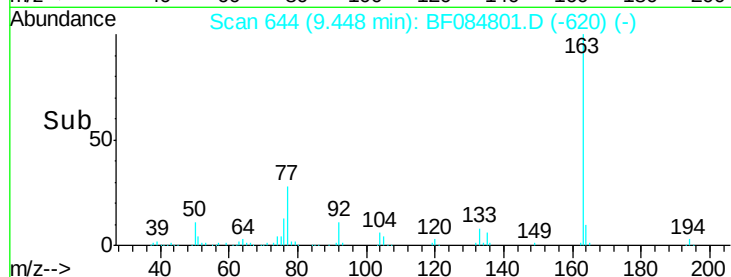

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.20 min Scan# 797

Delta R.T. -0.01 min

Lab File: BF084801.D

Acq: 3 Feb 2016 22:59


Tgt Ion:188 Resp: 596267

Ion Ratio Lower Upper

188 100

94 12.0 9.0 13.4



80 13.0 9.6 14.4

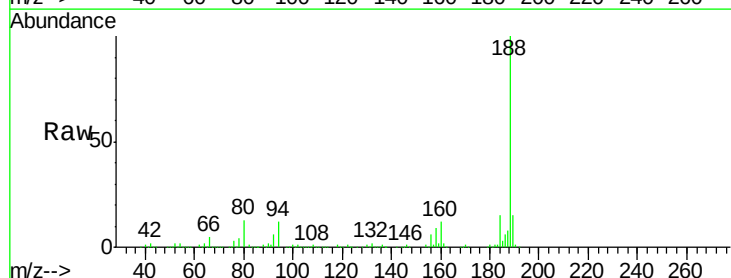


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

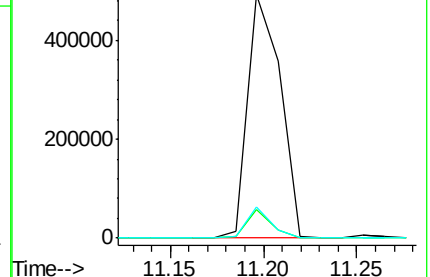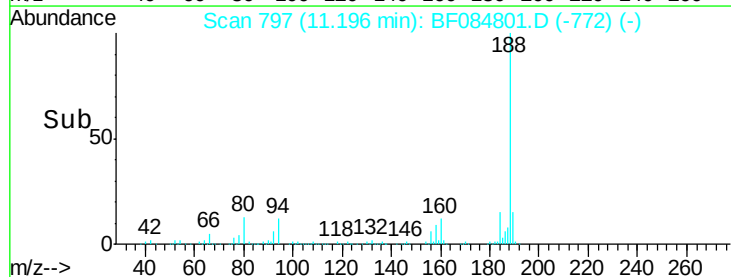

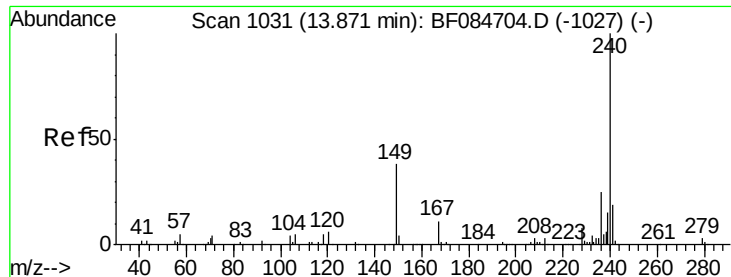

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.83 min Scan# 1027

Delta R.T. -0.01 min

Lab File: BF084801.D

Acq: 3 Feb 2016 22:59

Instrument :

BNA_F

ClientSampleId :

WEST-SIDEWALL(9)


Tot Ion:240 Resp: 505968

Ion Ratio Lower Upper

240 100

120 15.8 9.5 14.3#




236 25.9 20.6 31.0

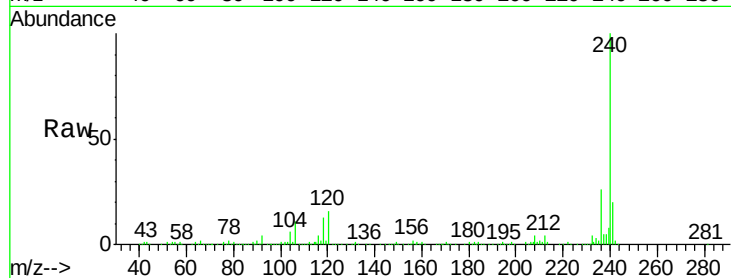

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

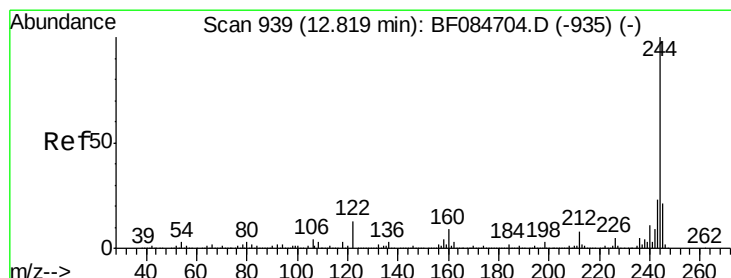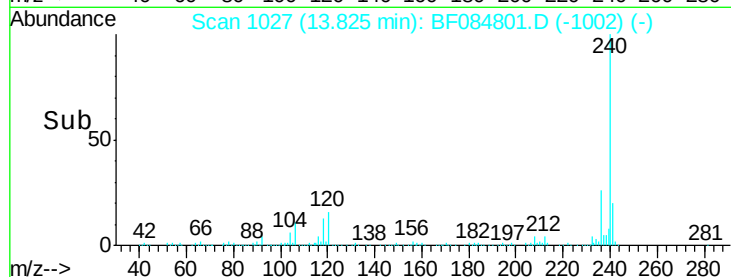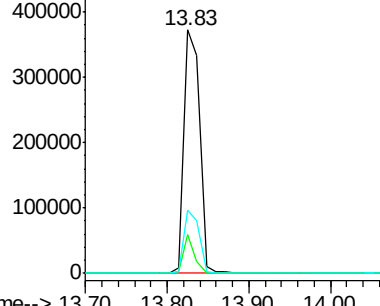

#78

Terphenyl-d14

Concen: 80.16 ng

RT: 12.80 min Scan# 937

Delta R.T. 0.00 min

Lab File: BF084801.D

Acq: 3 Feb 2016 22:59


Tgt Ion:244 Resp: 1789879

Ion Ratio Lower Upper

244 100

212 7.0 5.7 8.5



122 7.2 7.4 11.0#

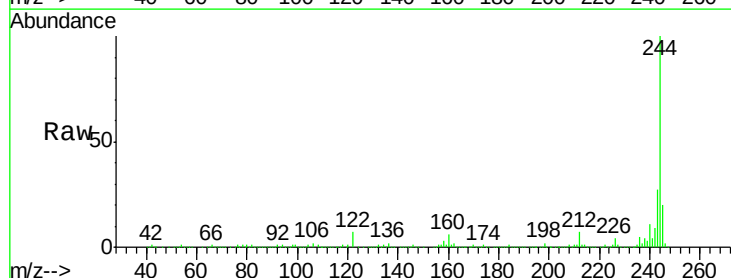


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

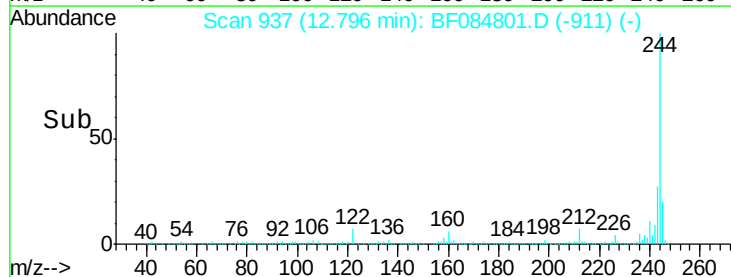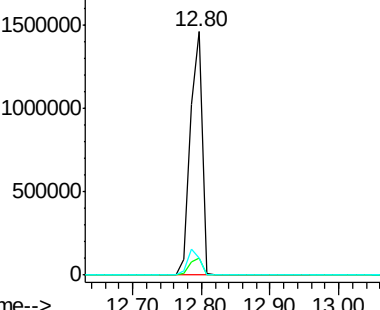


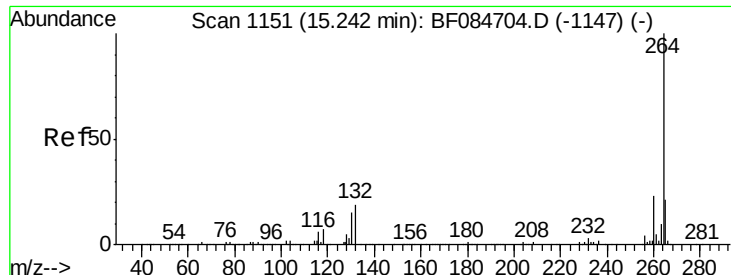

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.21 min Scan# 1148
Delta R.T. 0.00 min
Lab File: BF084801.D
Acq: 3 Feb 2016 22:59

Instrument :
BNA_F
ClientSampleId :
WEST-SIDEWALL(9)

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.0	19.4	29.2
265	21.8	17.8	26.6

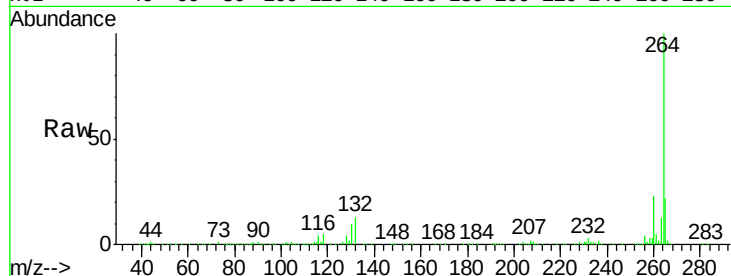

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

