


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020316\
 Data File : BF084803.D
 Acq On : 3 Feb 2016 23:56
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 03 14:16:01 2016

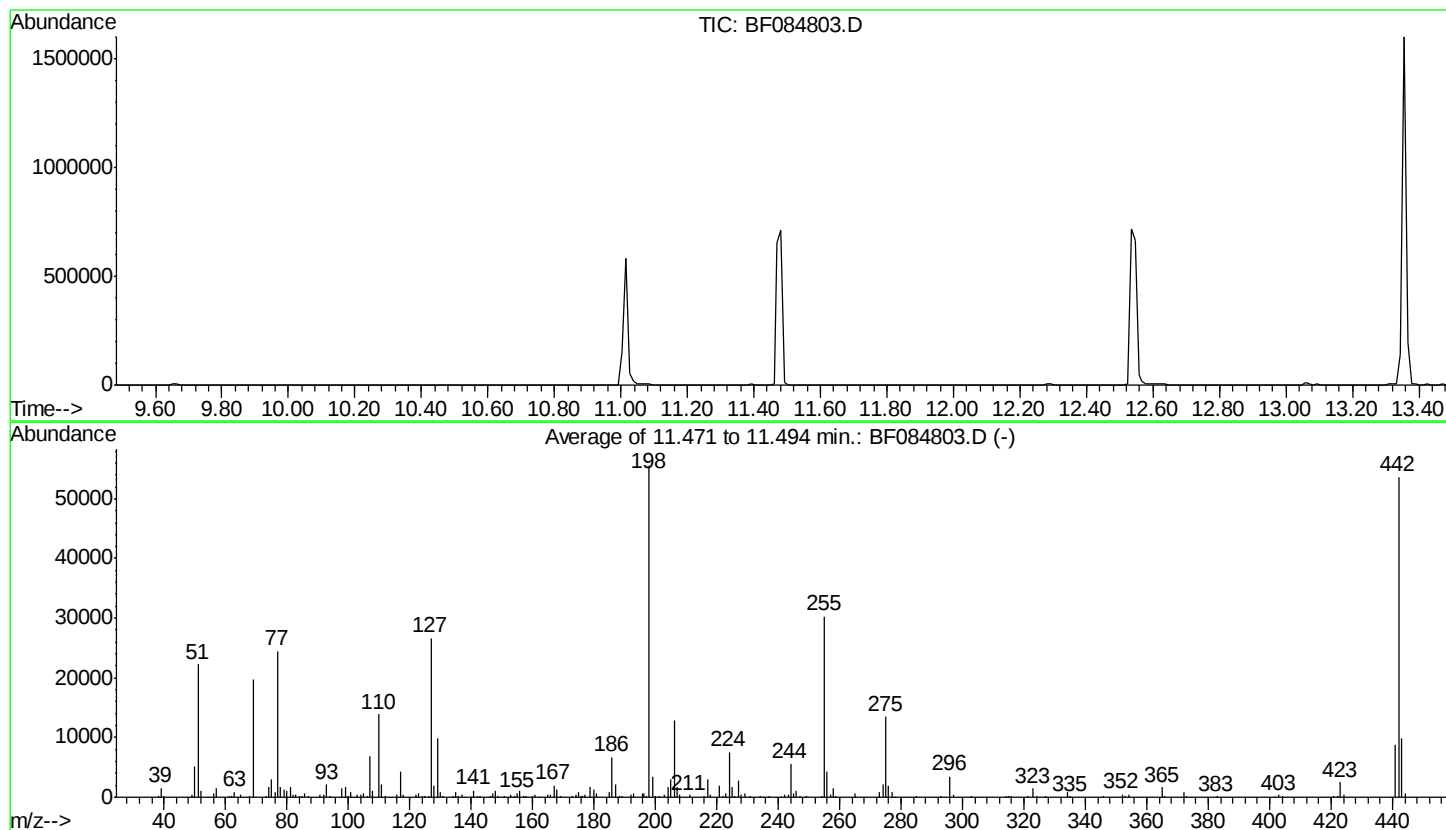

AutoFind: Scans 821, 822, 823; Background Corrected with Scan 817

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	22267	PASS
68	69	0.00	2	1.5	289	PASS
69	198	0.00	100	35.6	19764	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.1	26698	PASS
197	198	0.00	2	0.5	282	PASS
198	198	100	100	100.0	55547	PASS
199	198	5	9	6.2	3445	PASS
275	198	10	60	24.2	13465	PASS
365	198	1	100	2.9	1619	PASS
441	442	0.01	24	16.2	8720	PASS
442	198	50	100	96.7	53704	PASS
443	442	15	24	18.3	9811	PASS