
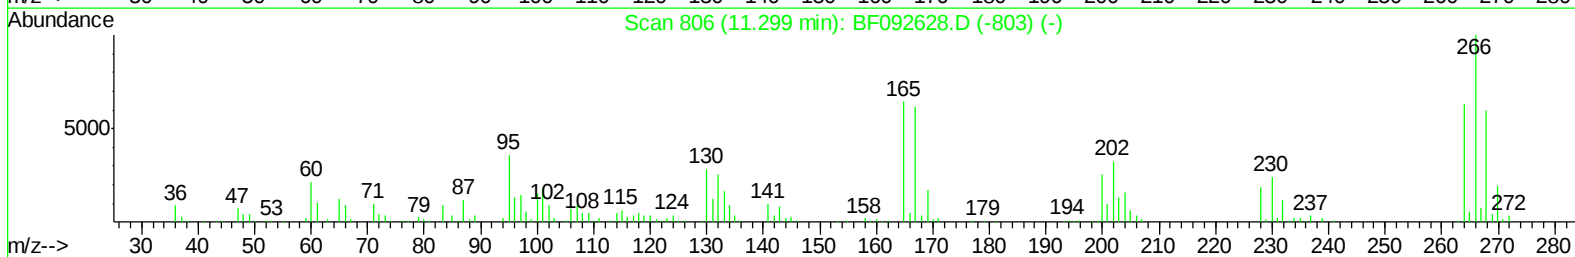
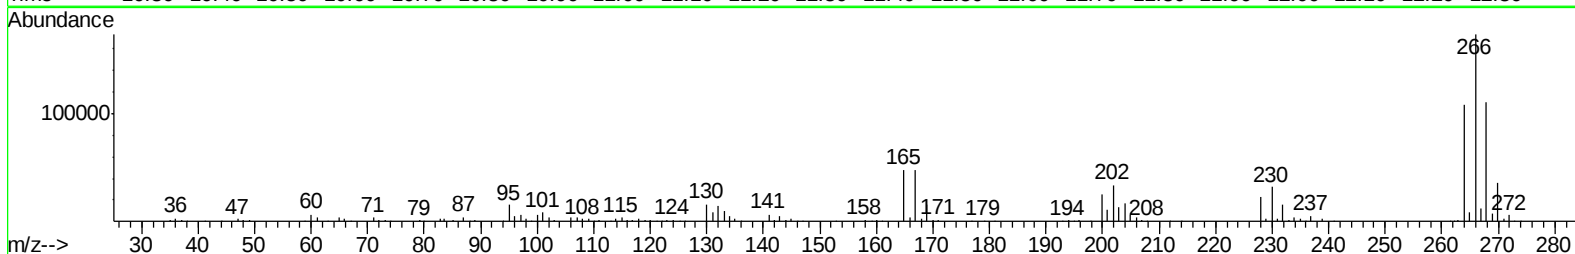


Data Path : Z:\HPCHEM1\BNA_F\Data\BF020317\
Data File : BF092779.D
Acq On : 3 Feb 2017 16:42
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 05:41:09 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 30 14:50:05 2017
Response via : Initial Calibration

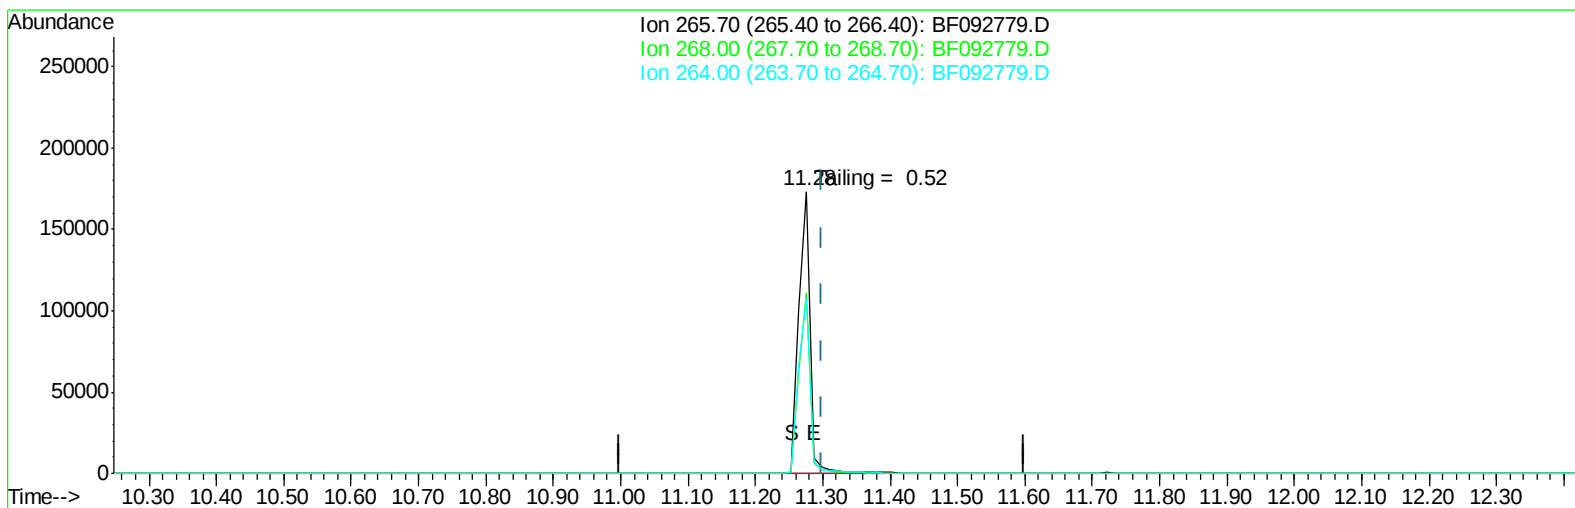

TIC: BF092779.D

(69) Pentachlorophenol (C)




11.276min (-0.023) 48121.90ng

response 204873

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	64.12
264.00	62.90	62.11
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF020317\
Data File : BF092779.D
Acq On : 3 Feb 2017 16:42
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 05:41:09 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 30 14:50:05 2017
Response via : Initial Calibration

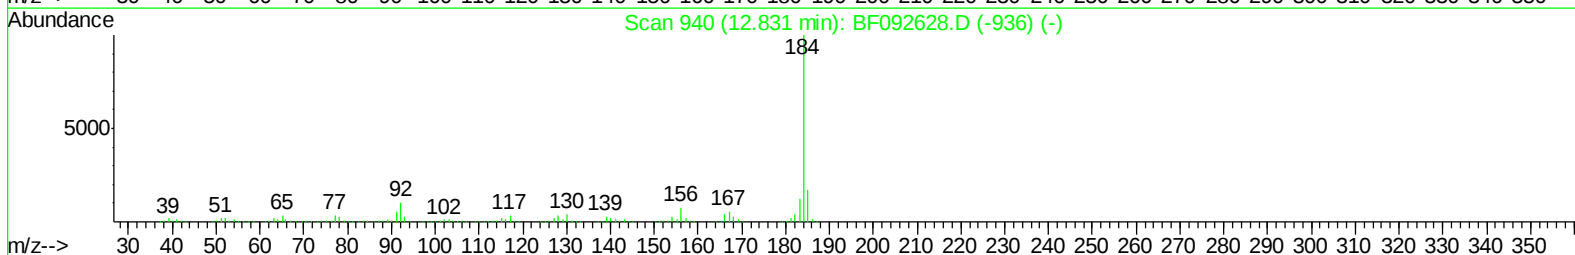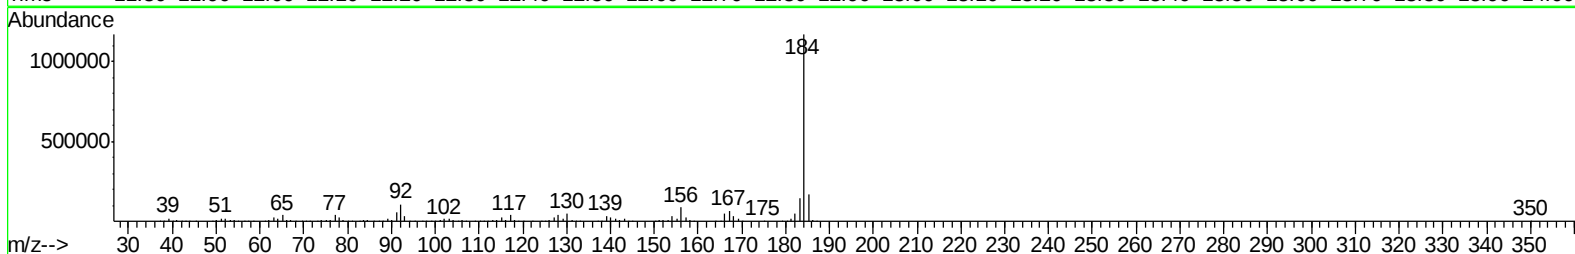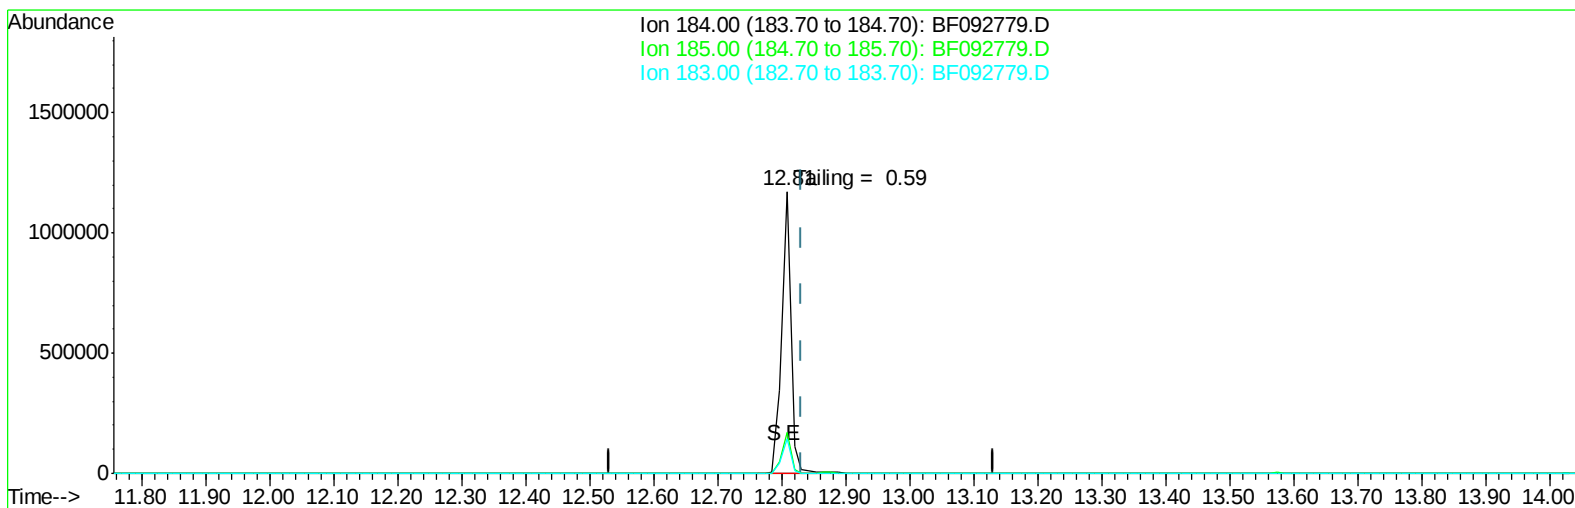

TIC: BF092779.D

(76) Benzidine

12.808min (-0.023) 0.00ng

response 1170717

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.36
183.00	11.50	12.51
0.00	0.00	0.00