
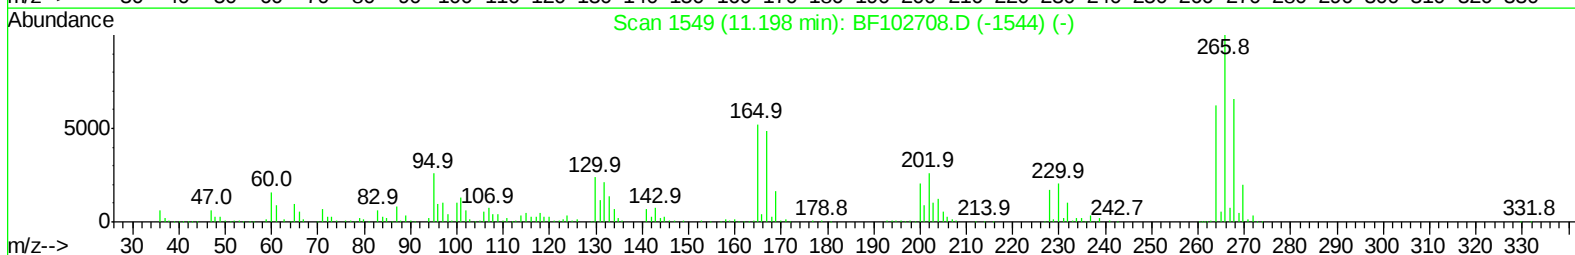
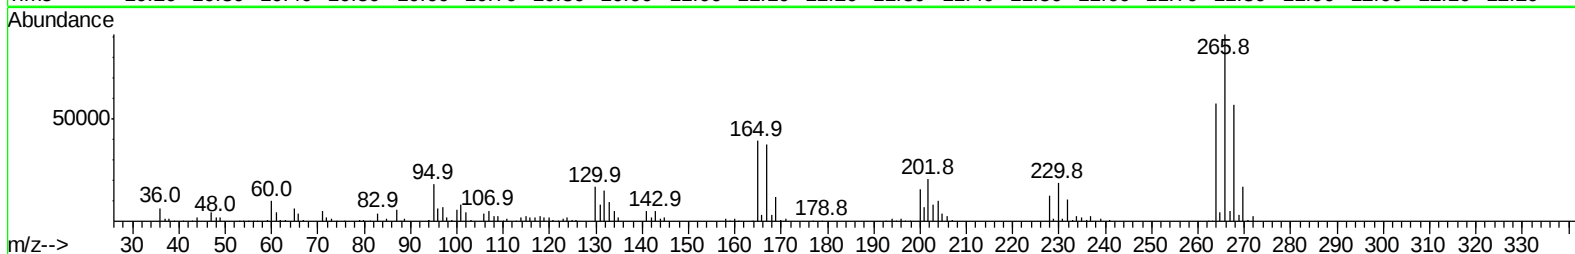


Data Path : U:\HPCHEM1\BNA F\DATA\BF020318\
Data File : BF102704.D
Acq On : 3 Feb 2018 8:38
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 02:58:35 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 00:38:27 2018
Response via : Initial Calibration

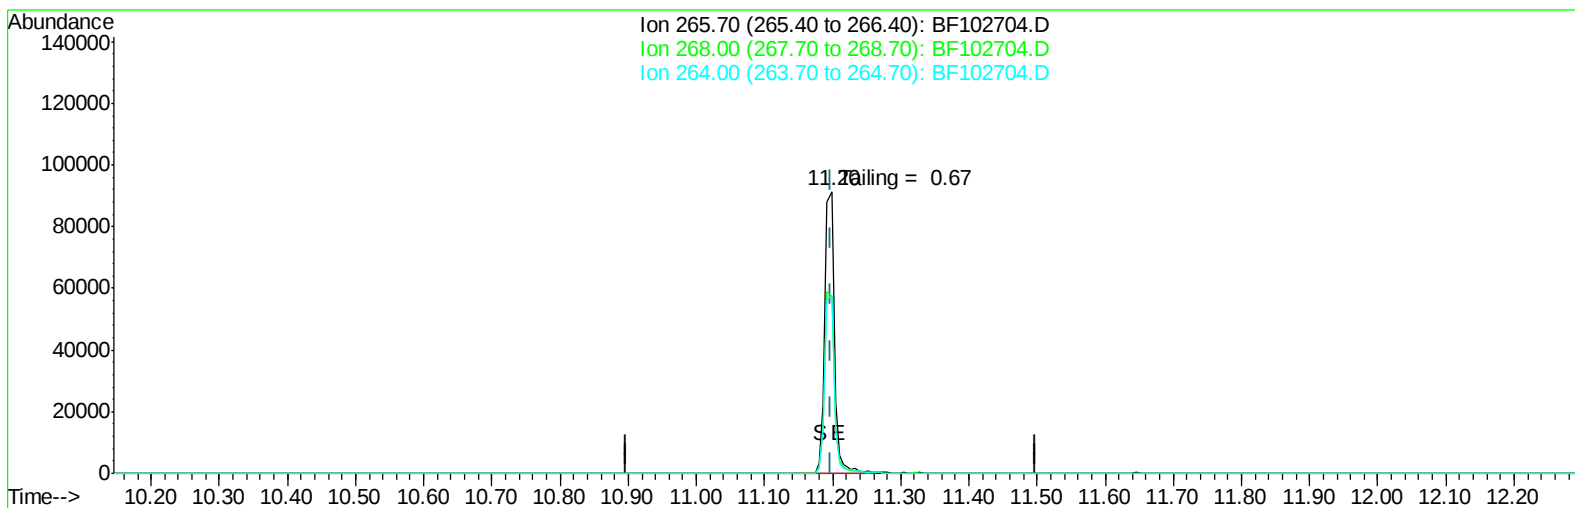

TIC: BF102704.D

(69) Pentachlorophenol (C)




11.198min (+0.000) 117278.96ng

response 86767

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.61
264.00	61.90	63.05
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF020318\
Data File : BF102704.D
Acq On : 3 Feb 2018 8:38
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 02:58:35 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 00:38:27 2018
Response via : Initial Calibration

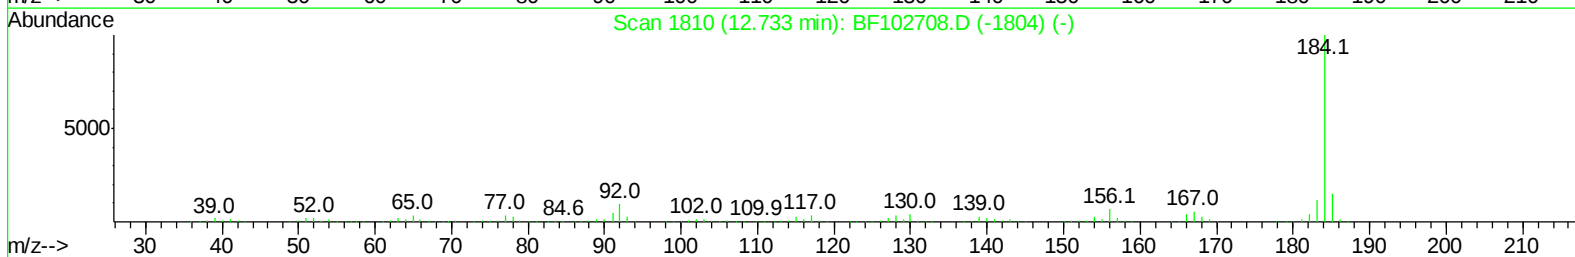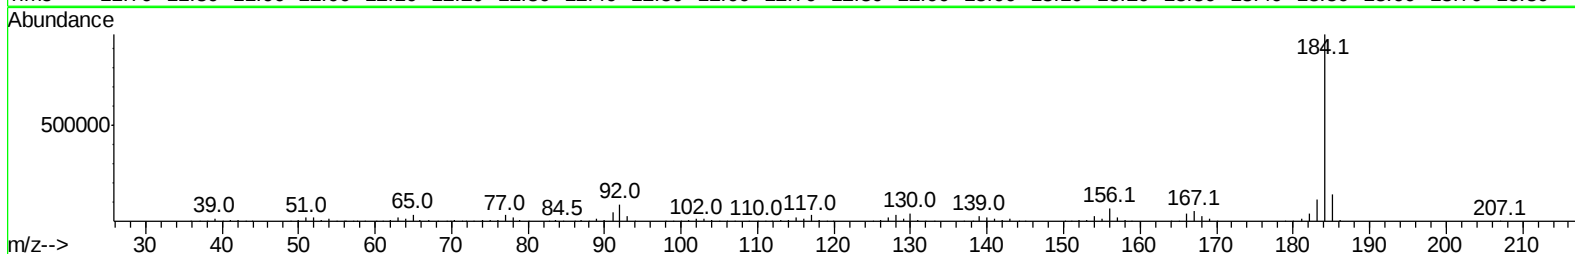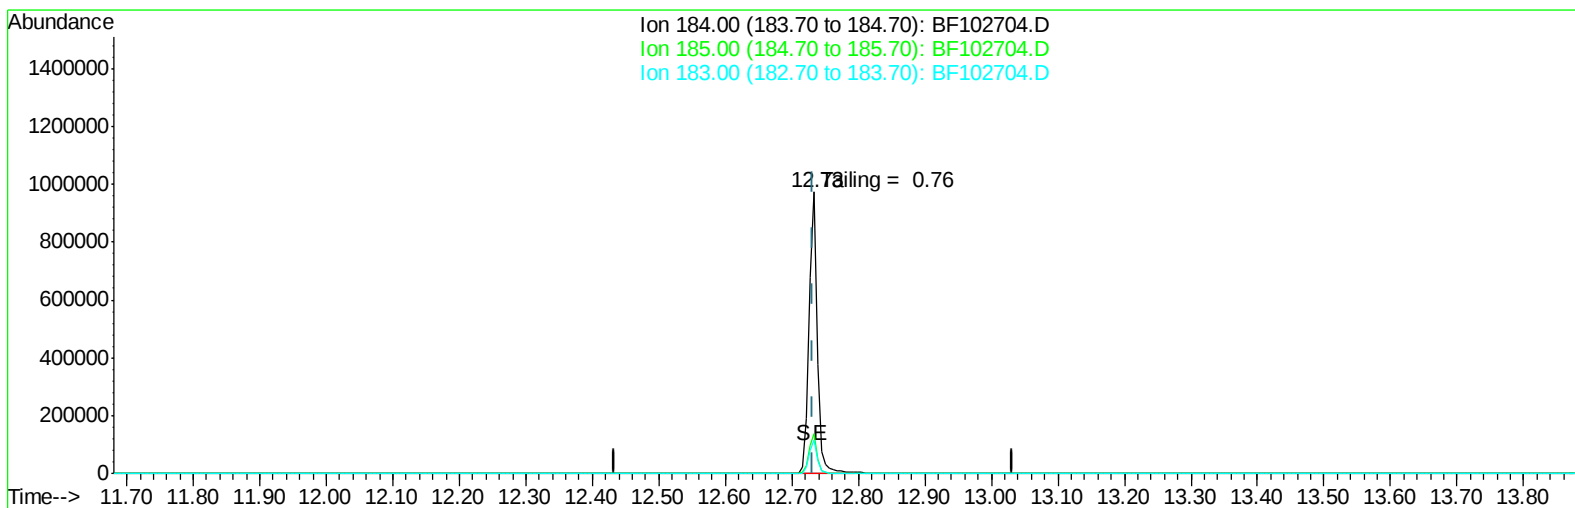

TIC: BF102704.D

(76) Benzidine

12.733min (+0.000) 0.00ng

response 861242

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.19
183.00	11.60	12.00
0.00	0.00	0.00