
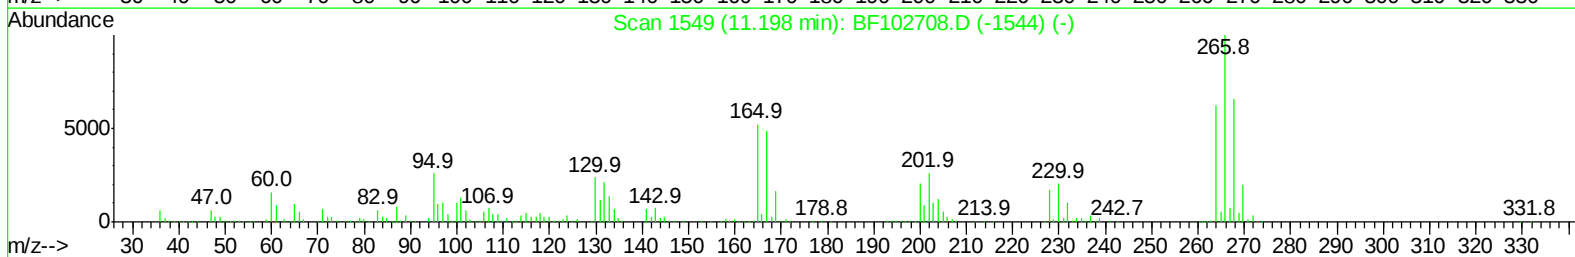
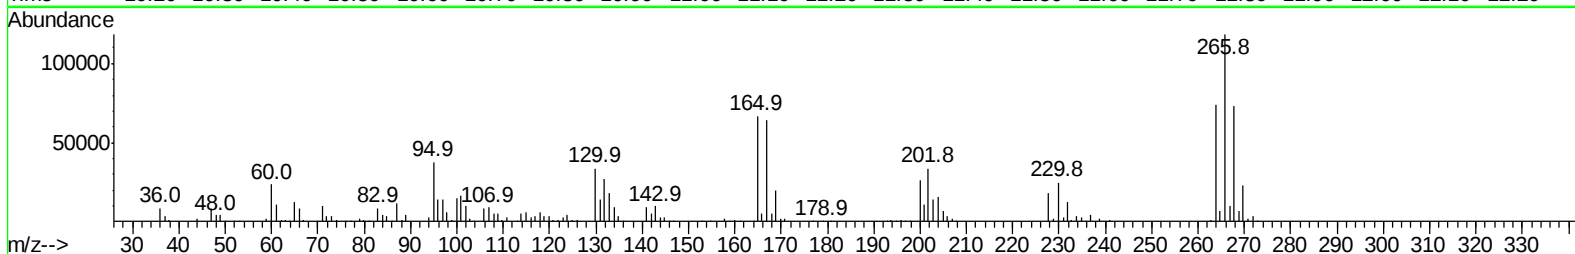


Data Path : U:\HPCHEM1\BNA F\DATA\BF020318\
Data File : BF102713.D
Acq On : 3 Feb 2018 13:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 03:04:15 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 00:38:27 2018
Response via : Initial Calibration

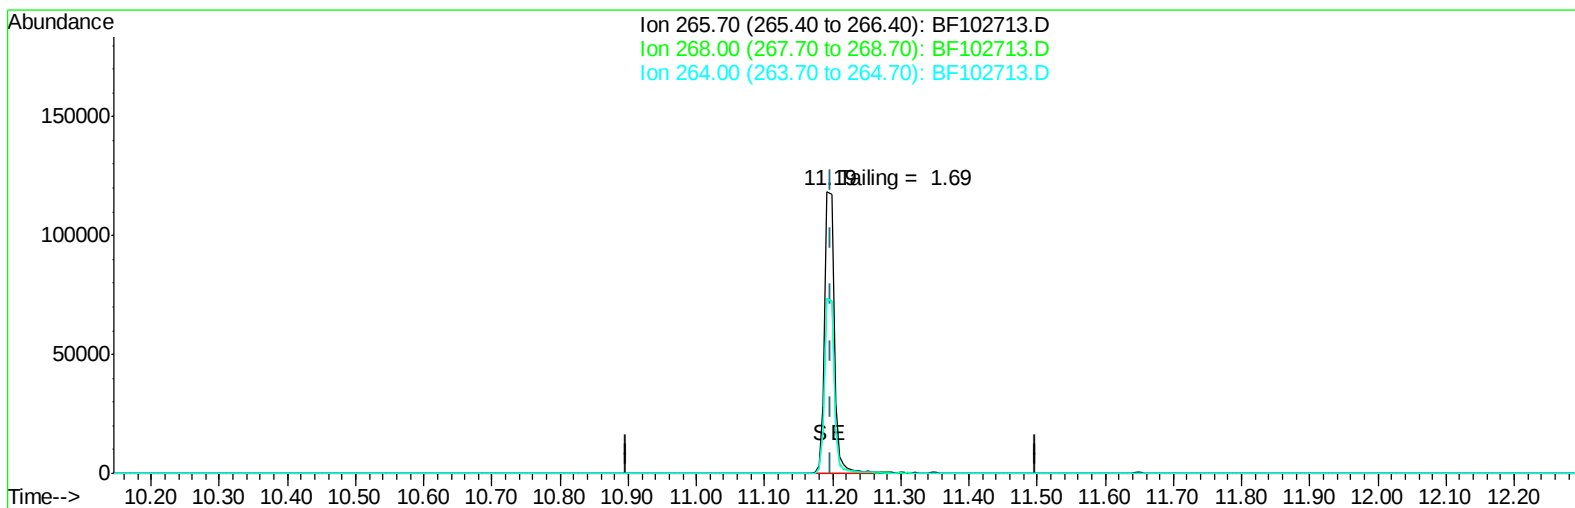

TIC: BF102713.D

(69) Pentachlorophenol (C)




11.192min (-0.006) 31990.62ng

response 112641

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.75
264.00	61.90	62.20
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF020318\
Data File : BF102713.D
Acq On : 3 Feb 2018 13:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 03:04:15 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 00:38:27 2018
Response via : Initial Calibration

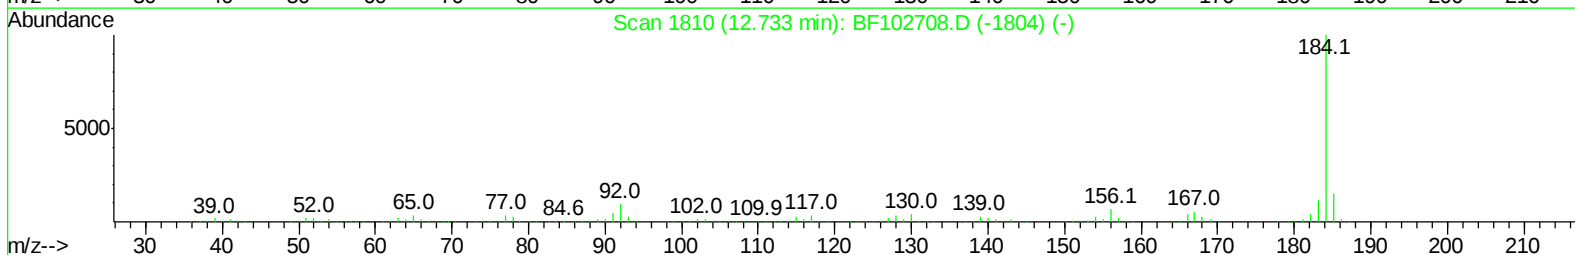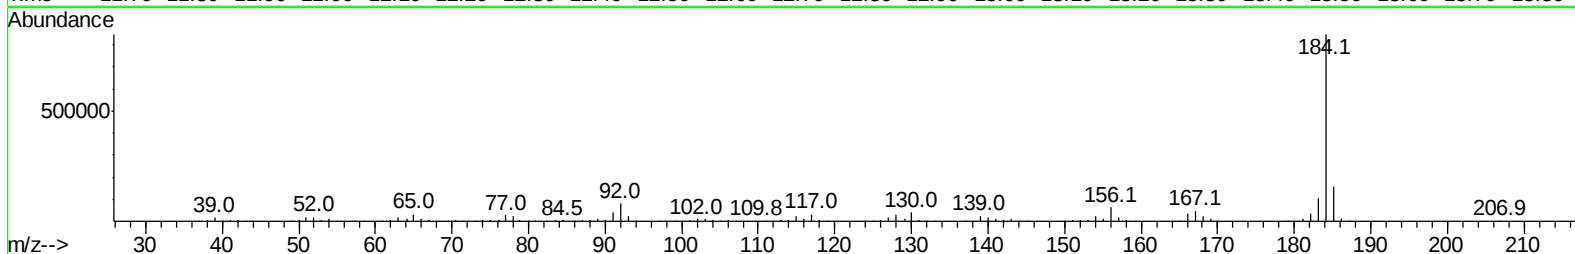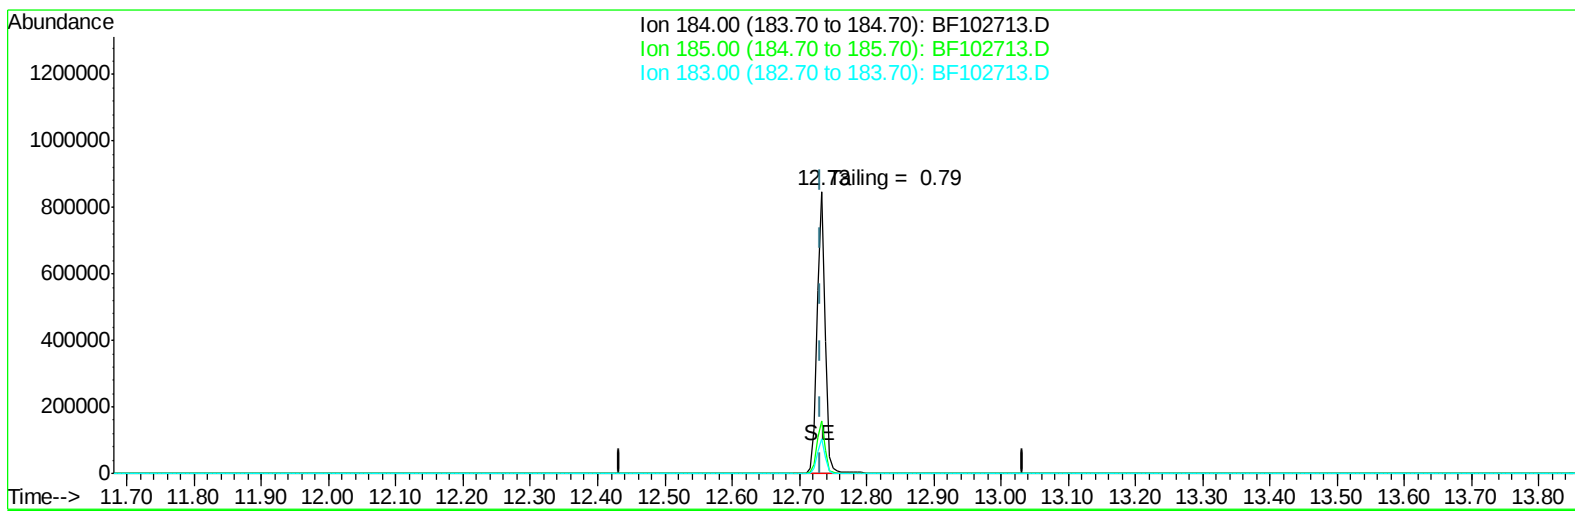

TIC: BF102713.D

(76) Benzidine

12.733min (+0.000) 0.00ng

response 726312

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	18.49
183.00	11.60	12.42
0.00	0.00	0.00