

Data Path : U:\HPCHEM1\BNA F\DATA\BF020318\
 Data File : BF102723.D
 Acq On : 3 Feb 2018 18:03
 Operator : SJ/JU
 Sample : J1436-17
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B25

Quant Time: Feb 05 02:32:33 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 00:38:27 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.88	152	194240	20.00	ng	0.00
21) Naphthalene-d8	8.16	136	793555	20.00	ng	0.00
38) Acenaphthene-d10	9.92	164	345937	20.00	ng	0.00
63) Phenanthrene-d10	11.40	188	519665	20.00	ng	0.00
75) Chrysene-d12	14.04	240	359267	20.00	ng	0.00
86) Perylene-d12	15.52	264	367881	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.50	112	1336733	104.51	ng	0.01
7) Phenol-d6	6.50	99	1585225	102.94	ng	0.00
23) Nitrobenzene-d5	7.44	82	954126	83.41	ng	0.00
41) 2,4,6-Tribromophenol	10.70	330	295688	106.19	ng	0.00
44) 2-Fluorobiphenyl	9.24	172	1551058	74.40	ng	0.00
78) Terphenyl-d14	12.99	244	1065098	70.20	ng	0.00
Target Compounds						
10) Phenol	6.52	94	77288	4.683	ng	98
49) Dimethylphthalate	9.63	163	167386	6.206	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : U:\HPCHEM1\BNA F\DATA\BF020318\
Data File : BF102723.D
Acq On : 3 Feb 2018 18:03
Operator : SJ/JU
Sample : J1436-17
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
B25

Quant Time: Feb 05 02:32:33 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 00:38:27 2018
Response via : Initial Calibration

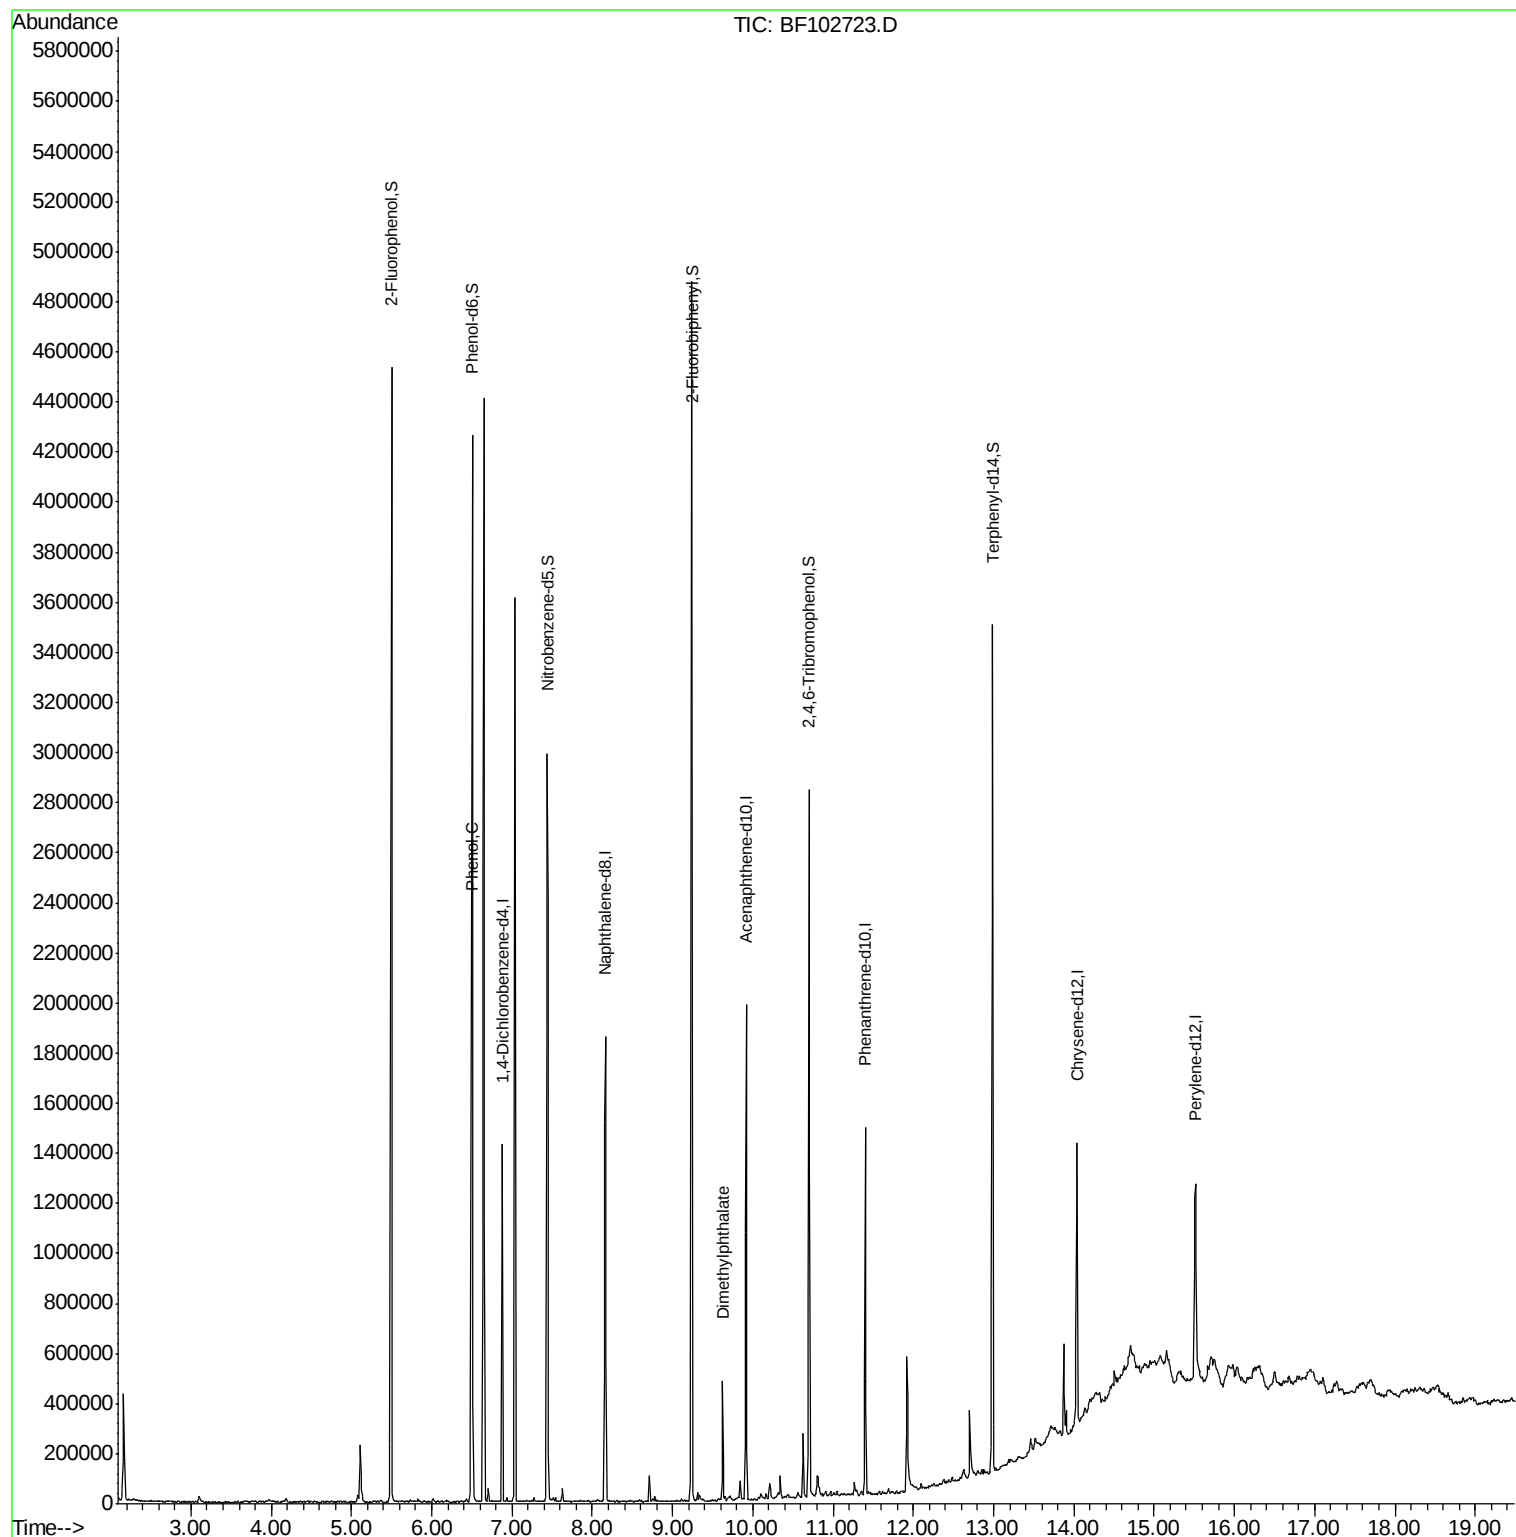

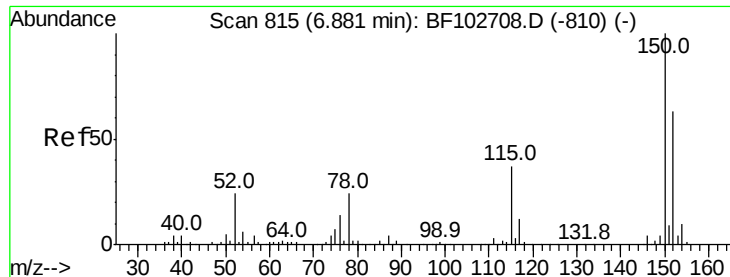


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.88 min Scan# 815
Delta R.T. 0.00 min
Lab File: BF102723.D
Acq: 3 Feb 2018 18:03

Instrument :
BNA_F
ClientSampled :
B25

Tot Ion:152 Resp: 194240
Ion Ratio Lower Upper
152 100
150 155.8 124.6 186.8
115 60.6 50.1 75.1

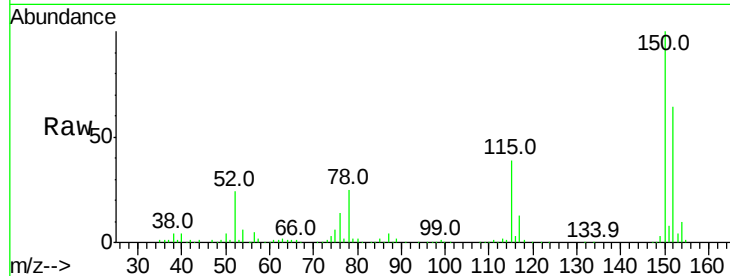


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

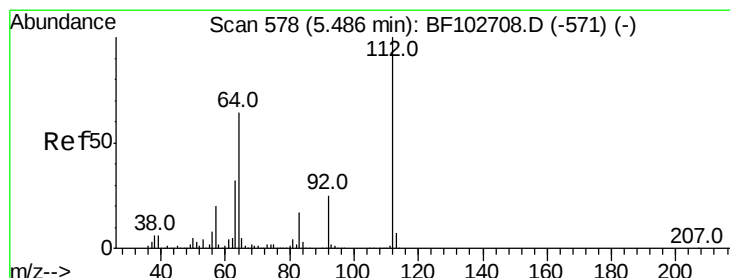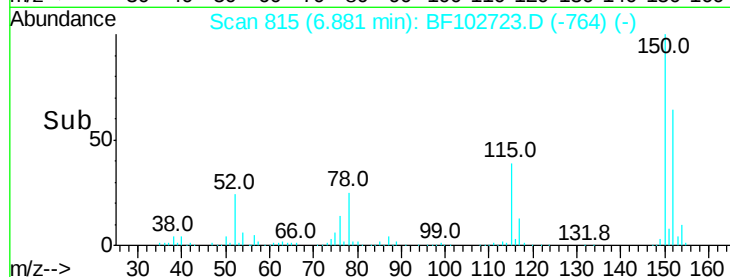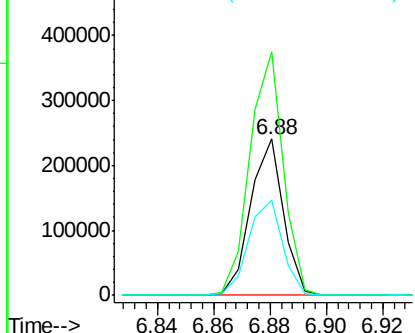



#5


2-Fluorophenol
Concen: 104.513 ng
RT: 5.50 min Scan# 580
Delta R.T. 0.01 min
Lab File: BF102723.D
Acq: 3 Feb 2018 18:03

Tgt Ion:112 Resp: 1336733
Ion Ratio Lower Upper
112 100
64 63.7 47.9 71.9
63 32.4 23.7 35.5

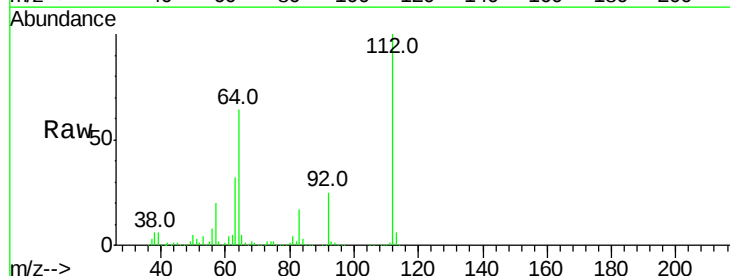

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

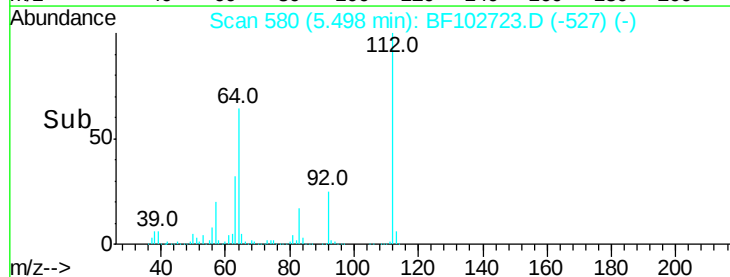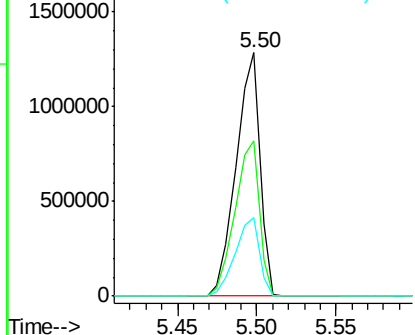

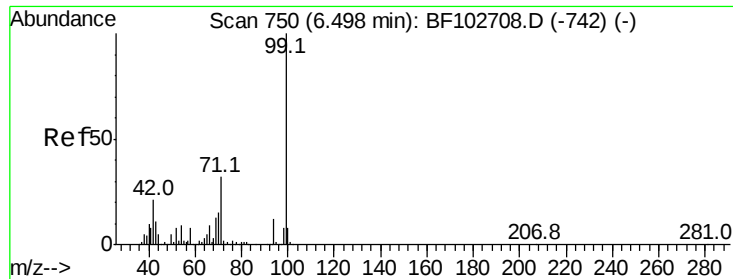

#7

Phenol-d6

Concen: 102.935 ng

RT: 6.50 min Scan# 751

Delta R.T. 0.01 min

Lab File: BF102723.D

Acq: 3 Feb 2018 18:03

Instrument :

BNA_F

ClientSampleId :

B25





Tot Ion: 99 Resp: 1585225

Ion Ratio Lower Upper

99 100

42 20.5 14.5 21.7

71 33.9 25.4 38.0

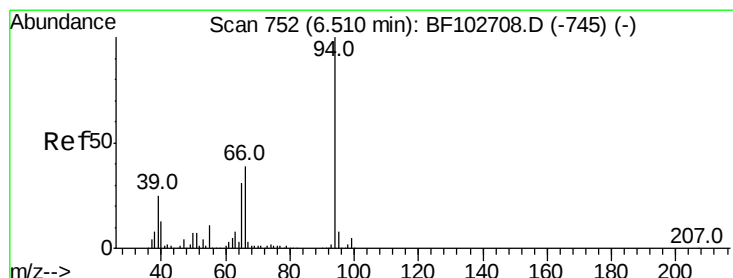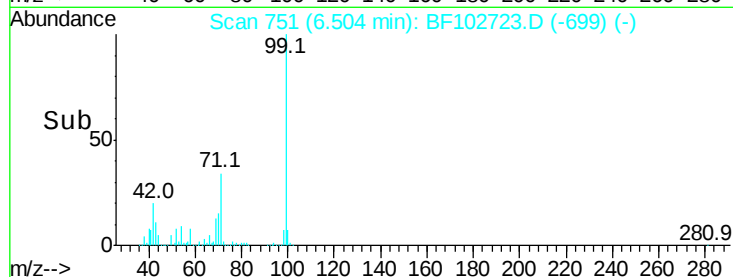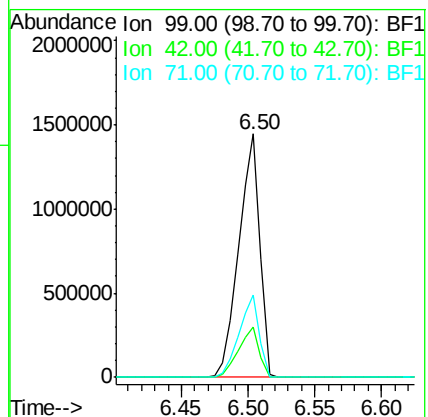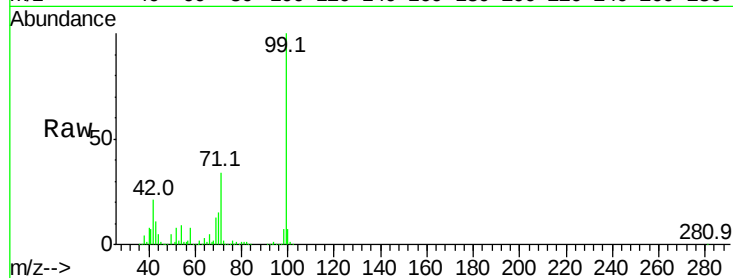

#10

Phenol

Concen: 4.683 ng

RT: 6.52 min Scan# 753

Delta R.T. 0.01 min

Lab File: BF102723.D

Acq: 3 Feb 2018 18:03




Tgt Ion: 94 Resp: 77288


Ion Ratio Lower Upper

94 100

65 28.7 7.9 47.9

66 35.3 16.2 56.2

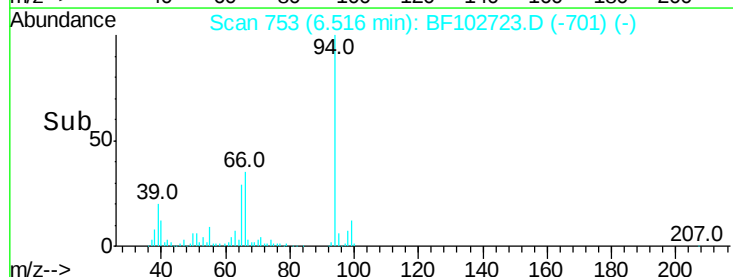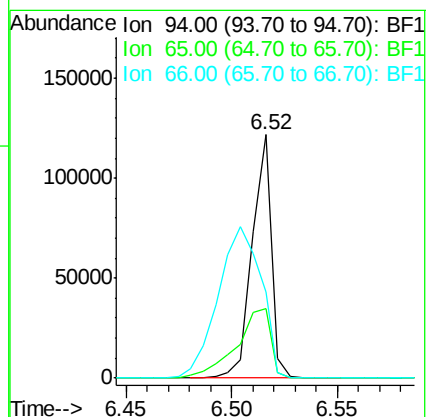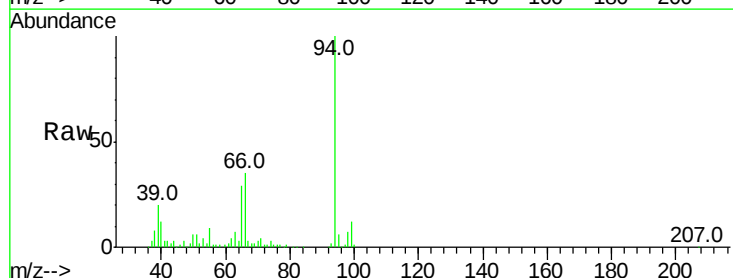

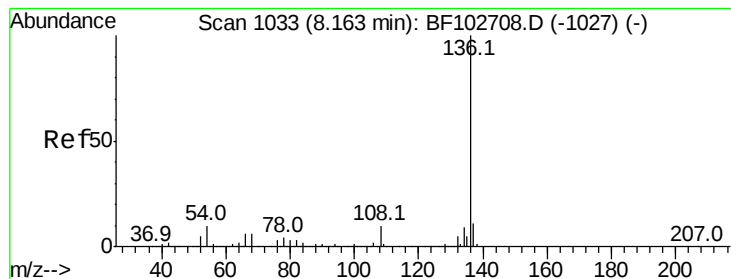

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.16 min Scan# 1033

Delta R.T. 0.00 min

Lab File: BF102723.D

Acq: 3 Feb 2018 18:03

Instrument :

BNA_F

ClientSampleId :

B25

Tot Ion:136 Resp: 793555


Ion Ratio Lower Upper

136 100

137 11.0 8.9 13.3

54 9.2 6.6 9.8

68 6.0 5.0 7.4



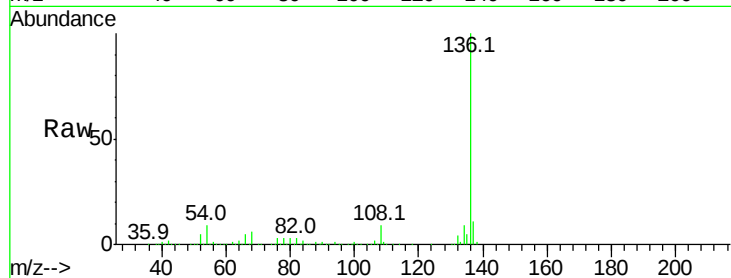


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

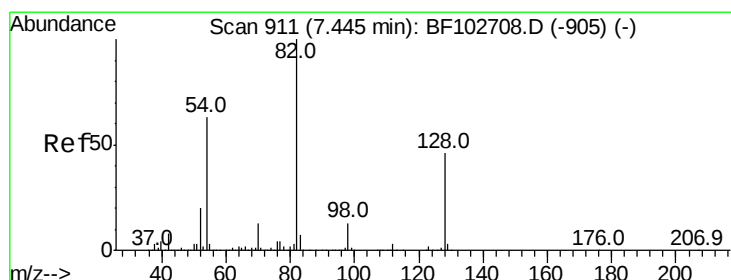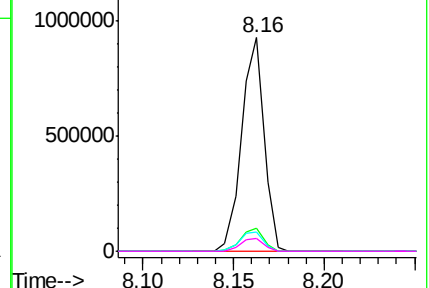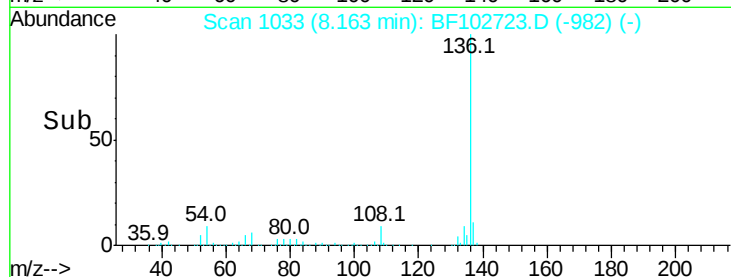

#23

Nitrobenzene-d5

Concen: 83.407 ng

RT: 7.44 min Scan# 910

Delta R.T. -0.01 min

Lab File: BF102723.D

Acq: 3 Feb 2018 18:03


Tgt Ion: 82 Resp: 954126

Ion Ratio Lower Upper

82 100

128 45.1 36.1 54.1



54 64.6 41.4 62.2#

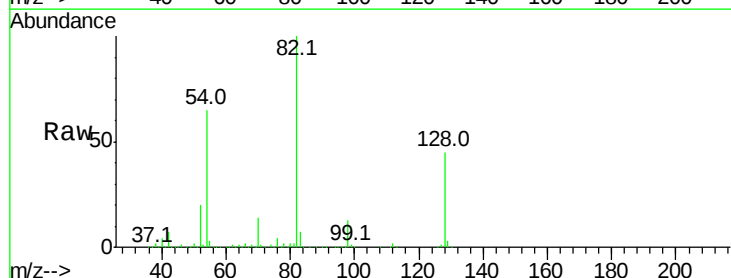


Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1



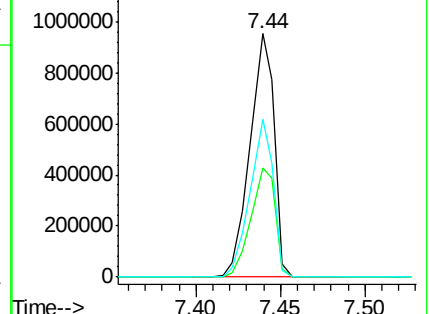
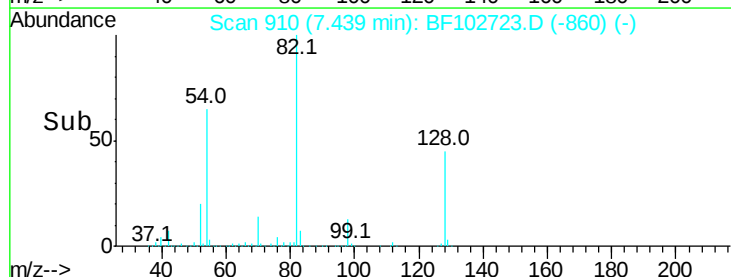


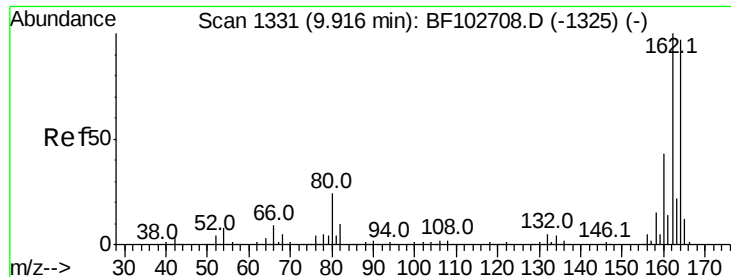

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.92 min Scan# 1331
Delta R.T. 0.00 min
Lab File: BF102723.D
Acq: 3 Feb 2018 18:03




Instrument :
BNA_F
ClientSampleId :
B25


Tot Ion:164 Resp: 345937
Ion Ratio Lower Upper
164 100
162 104.7 86.1 129.1
160 45.9 38.3 57.5

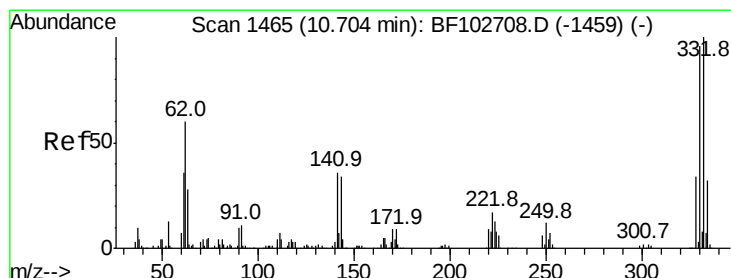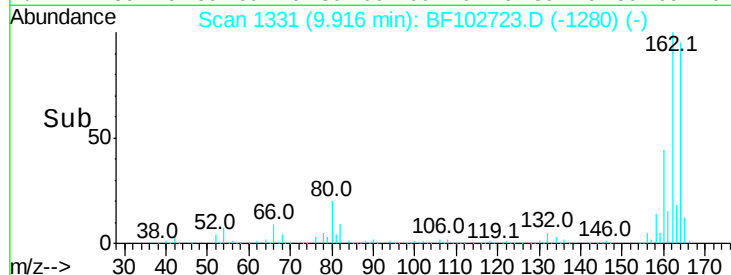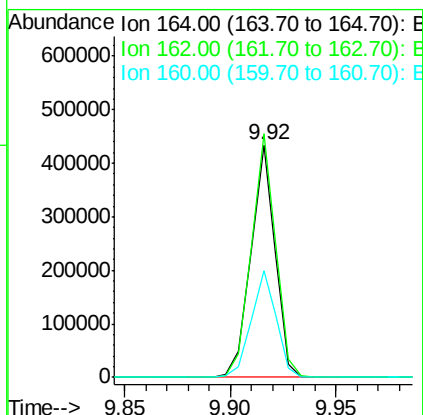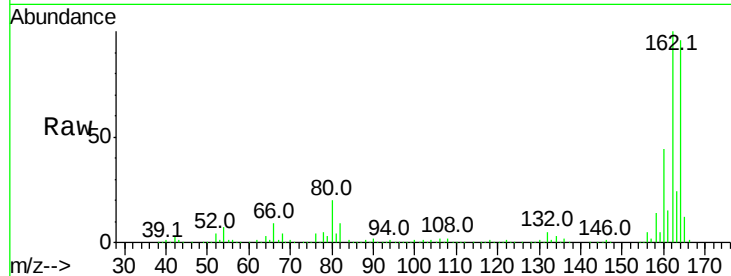

#41
2,4,6-Tribromophenol
Concen: 106.195 ng
RT: 10.70 min Scan# 1465
Delta R.T. 0.00 min
Lab File: BF102723.D
Acq: 3 Feb 2018 18:03

Tgt Ion:330 Resp: 295688
Ion Ratio Lower Upper
330 100
332 104.4 77.0 115.6
141 38.9 29.9 44.9

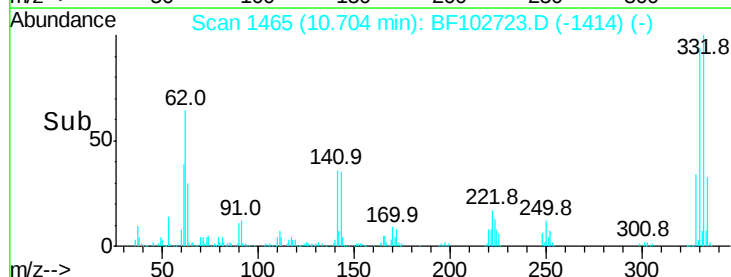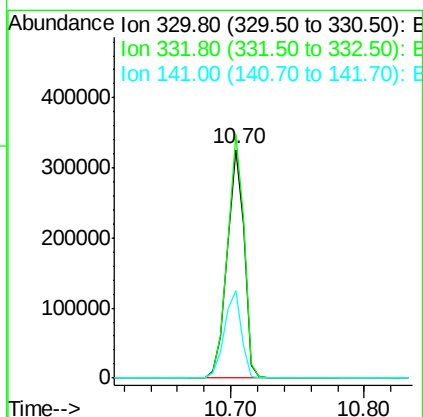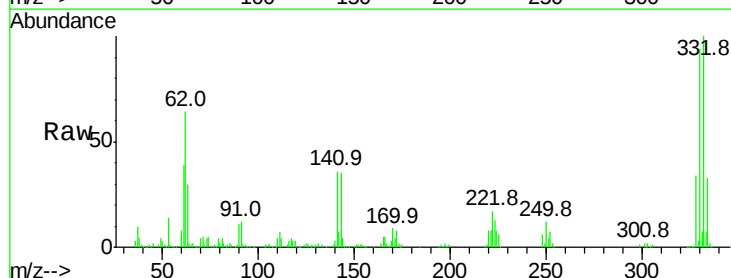


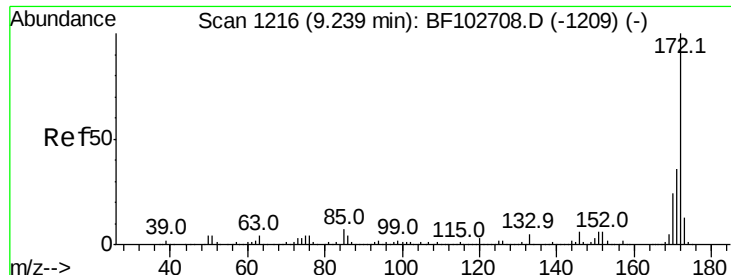




#44
2-Fluorobiphenyl
Concen: 74.400 ng
RT: 9.24 min Scan# 1216
Delta R.T. 0.00 min
Lab File: BF102723.D
Acq: 3 Feb 2018 18:03

Instrument :
BNA_F
ClientSampleId :
B25

Tot Ion:172 Resp: 1551058
Ion Ratio Lower Upper
172 100
171 36.6 29.7 44.5
170 24.5 19.6 29.4

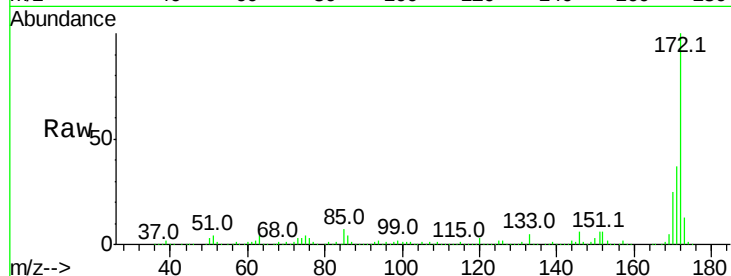


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

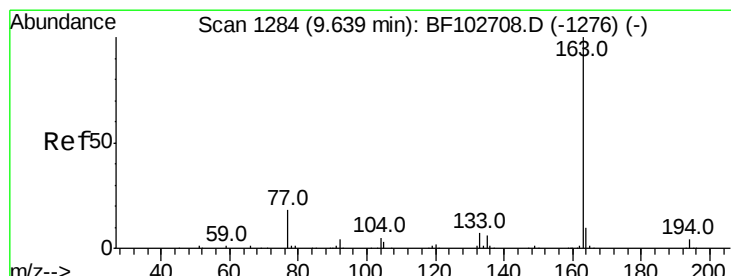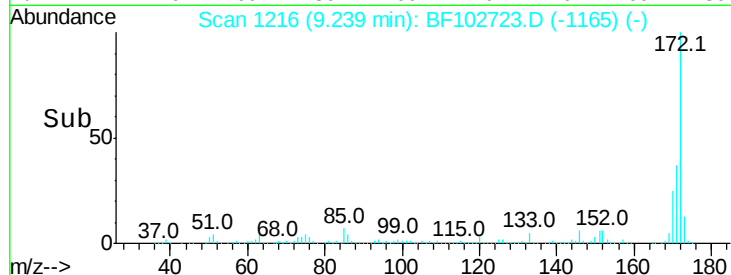
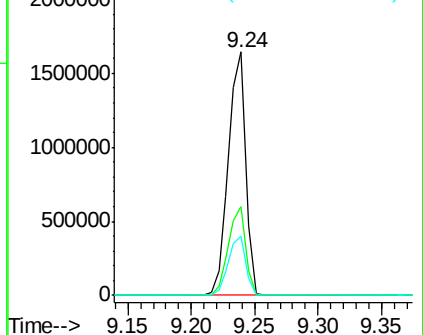



#49
Dimethylphthalate
Concen: 6.206 ng
RT: 9.63 min Scan# 1282
Delta R.T. -0.01 min
Lab File: BF102723.D
Acq: 3 Feb 2018 18:03

Tgt Ion:163 Resp: 167386
Ion Ratio Lower Upper
163 100
194 3.3 2.7 4.1
164 9.5 8.2 12.2

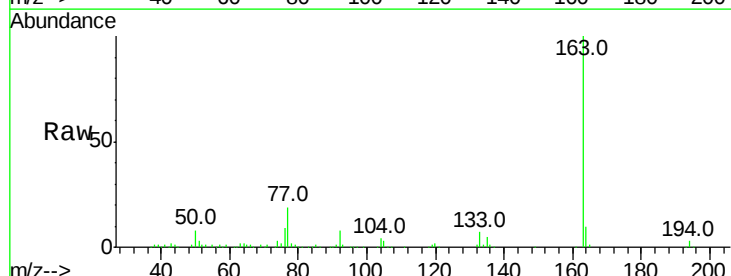

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

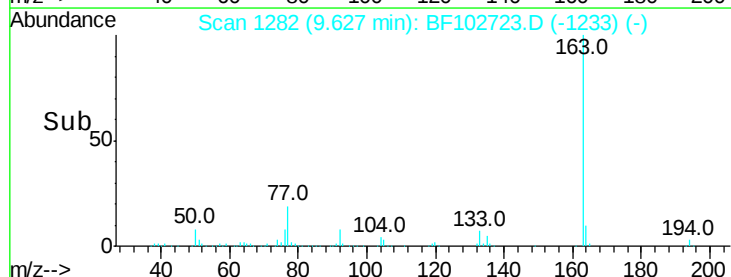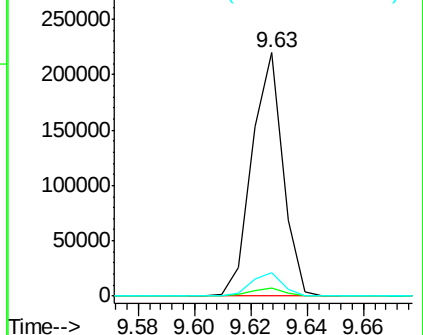


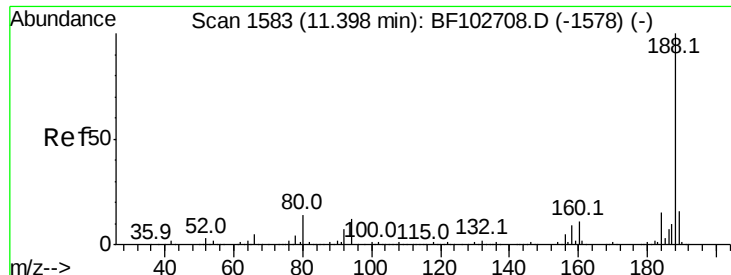




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.40 min Scan# 1584
Delta R.T. 0.01 min
Lab File: BF102723.D
Acq: 3 Feb 2018 18:03

Instrument :
BNA_F
ClientSampleId :
B25

Tot Ion:188 Resp: 519665
Ion Ratio Lower Upper
188 100
94 10.1 8.5 12.7
80 10.8 9.2 13.8

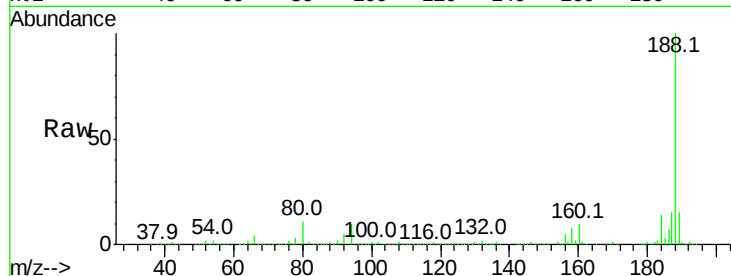


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

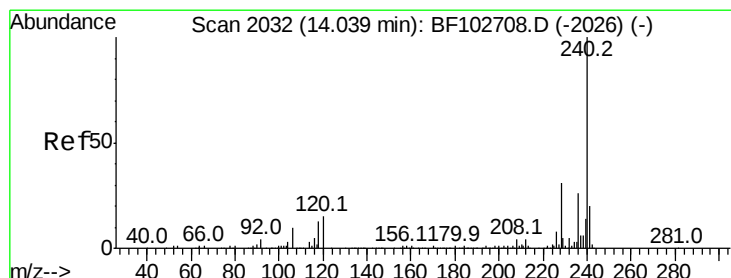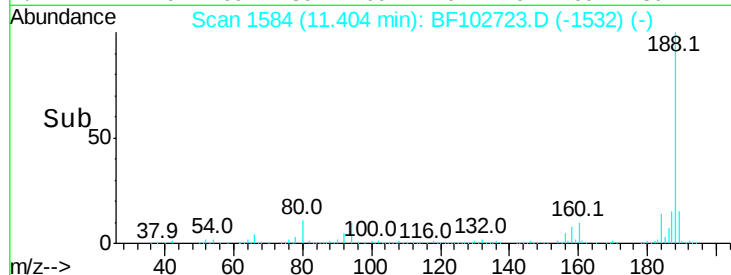
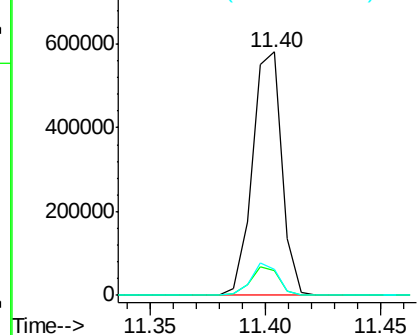



#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.04 min Scan# 2032
Delta R.T. 0.00 min
Lab File: BF102723.D
Acq: 3 Feb 2018 18:03

Tgt Ion:240 Resp: 359267
Ion Ratio Lower Upper
240 100
120 14.1 9.5 14.3
236 25.8 20.7 31.1

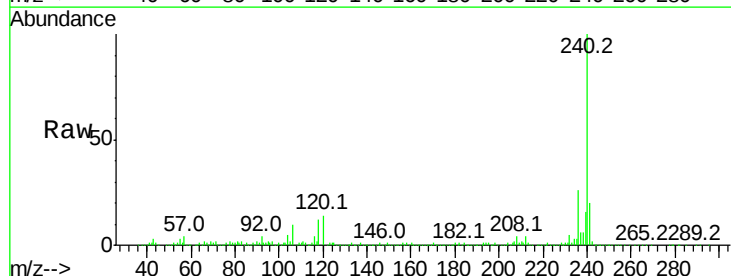

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

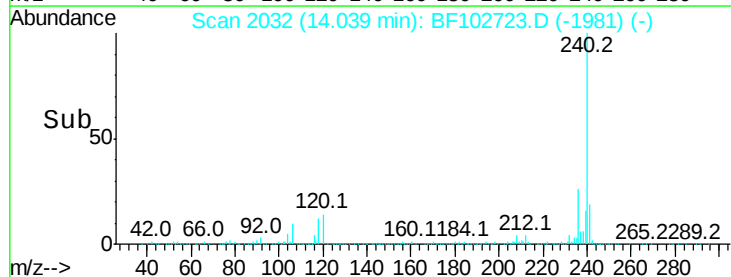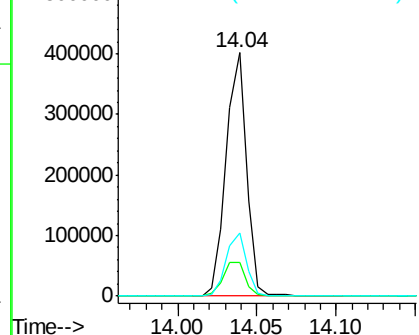

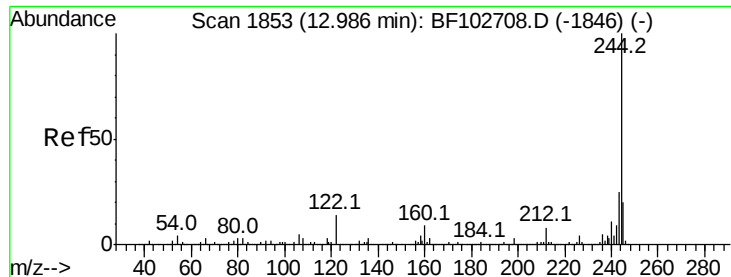

#78

Terphenyl-d14

Concen: 70.196 ng

RT: 12.99 min Scan# 1853

Delta R.T. 0.00 min

Lab File: BF102723.D

Acq: 3 Feb 2018 18:03

Instrument :

BNA_F

ClientSampleId :

B25


Tot Ion:244 Resp: 1065098

Ion Ratio Lower Upper

244 100

212 6.9 5.4 8.0




122 14.5 11.0 16.4

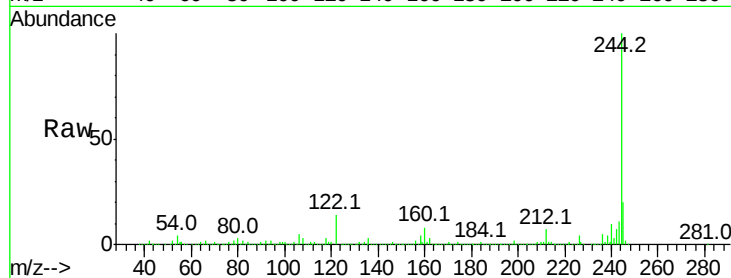

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

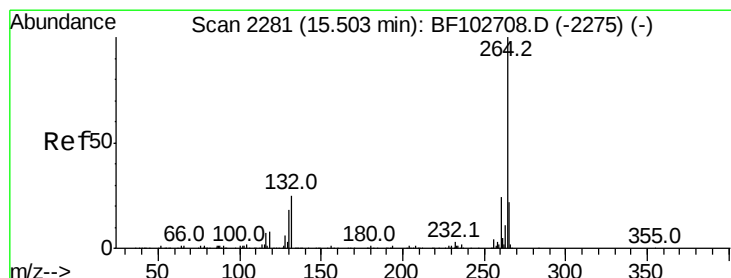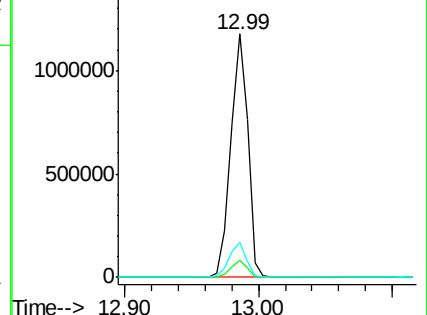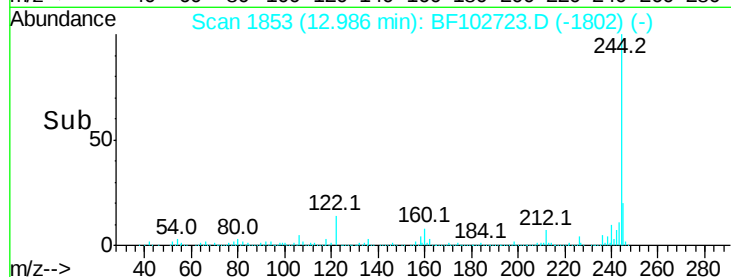

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.52 min Scan# 2283

Delta R.T. 0.01 min

Lab File: BF102723.D

Acq: 3 Feb 2018 18:03


Tgt Ion:264 Resp: 367881

Ion Ratio Lower Upper

264 100

260 24.8 19.2 28.8

265 21.9 17.5 26.3

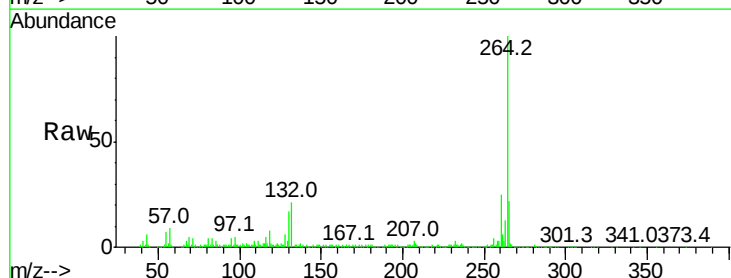

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

