


Data Path : U:\HPCHEM1\BNA_F\Data\BF020318\
 Data File : BF102713.D
 Acq On : 3 Feb 2018 13:08
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 05 00:38:27 2018

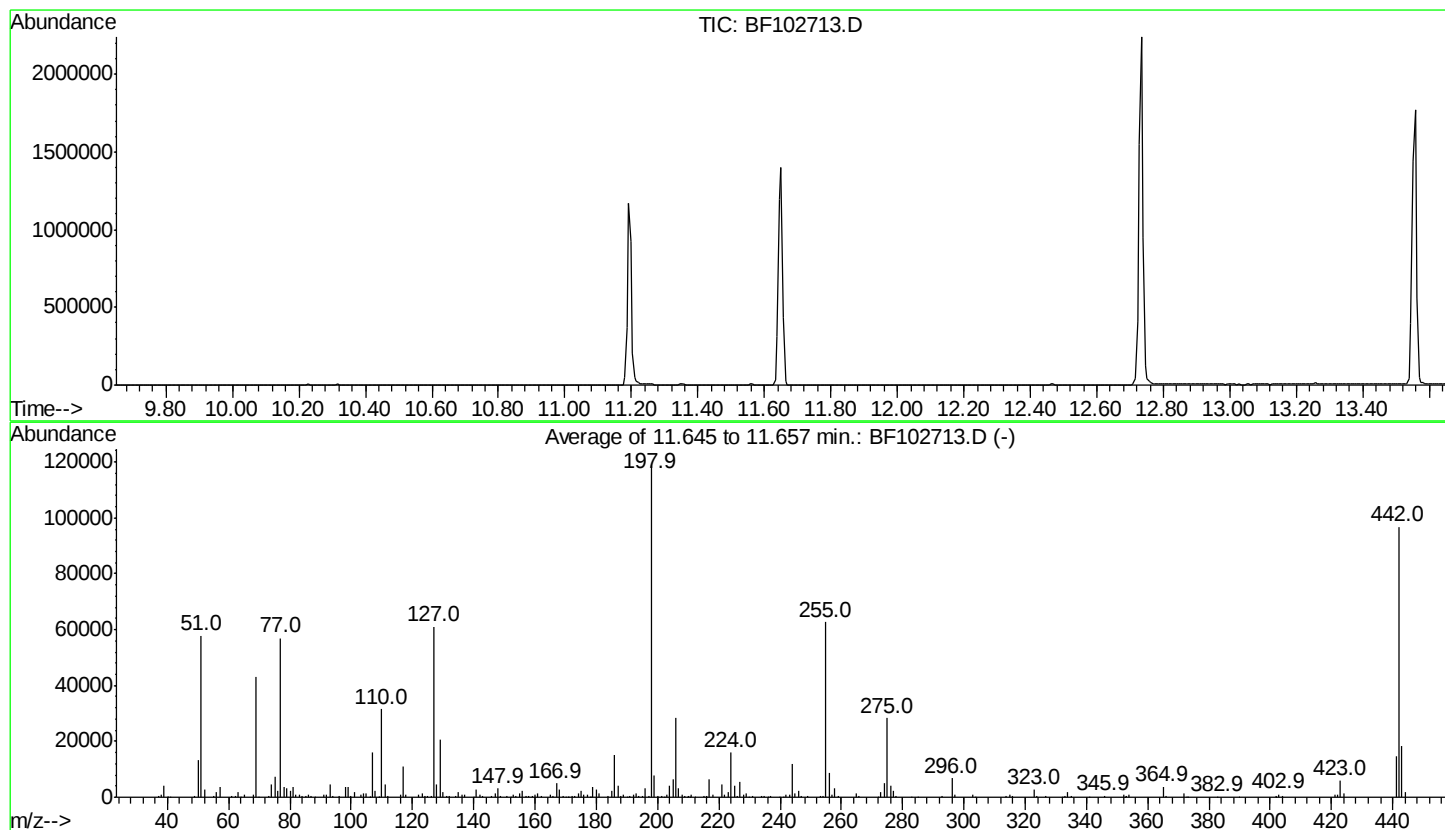

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.8	57966	PASS
68	69	0.00	2	1.7	746	PASS
69	198	0.00	100	36.4	43170	PASS
70	69	0.00	2	0.2	100	PASS
127	198	10	80	51.5	61176	PASS
197	198	0.00	2	0.4	504	PASS
198	198	100	100	100.0	118693	PASS
199	198	5	9	6.5	7682	PASS
275	198	10	60	23.8	28282	PASS
365	198	1	100	3.2	3754	PASS
441	443	0.01	100	80.8	14779	PASS
442	198	50	100	81.5	96701	PASS
443	442	15	24	18.9	18298	PASS